

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
 Data File : VU043850.D
 Acq On : 20 May 2021 00:41
 Operator : SY/MD
 Sample : M2459-07 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0GM7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043850.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	94	rBV	85590	94740	13.91%	1.615%
2	1.916	171	179	194	rVB	61316	79978	11.74%	1.363%
3	2.572	370	383	403	rBV	146228	238592	35.02%	4.068%
4	3.051	521	532	546	rVB3	9317	17448	2.56%	0.297%
5	4.645	1012	1028	1059	rBV	82131	266359	39.10%	4.541%
6	5.073	1145	1161	1187	rBV	126635	284648	41.78%	4.853%
7	5.533	1285	1304	1322	rBV	102883	223726	32.84%	3.814%
8	5.735	1344	1367	1390	rBV2	256636	662197	97.20%	11.289%
9	6.256	1515	1529	1550	rBV	236980	456539	67.01%	7.783%
10	6.549	1609	1620	1638	rVB2	27390	51045	7.49%	0.870%
11	6.700	1652	1667	1686	rBV	158624	310295	45.55%	5.290%
12	7.575	1926	1939	1958	rBV	70786	124934	18.34%	2.130%
13	7.906	2024	2042	2056	rBV	296121	507305	74.47%	8.649%
14	8.186	2117	2129	2146	rBV	44836	76241	11.19%	1.300%
15	8.645	2259	2272	2310	rBV	326718	681266	100.00%	11.614%
16	8.928	2350	2360	2376	rBV3	4795	9007	1.32%	0.154%
17	9.423	2501	2514	2537	rBV	351874	588045	86.32%	10.025%
18	10.764	2919	2931	2947	rBV	126878	204025	29.95%	3.478%
19	11.819	3246	3259	3278	rBV	330742	523578	76.85%	8.926%
20	12.201	3364	3378	3395	rBV	289325	465719	68.36%	7.940%




Sum of corrected areas: 5865687

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043850.D
Acq On : 20 May 2021 00:41
Operator : SY/MD
Sample : M2459-07 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

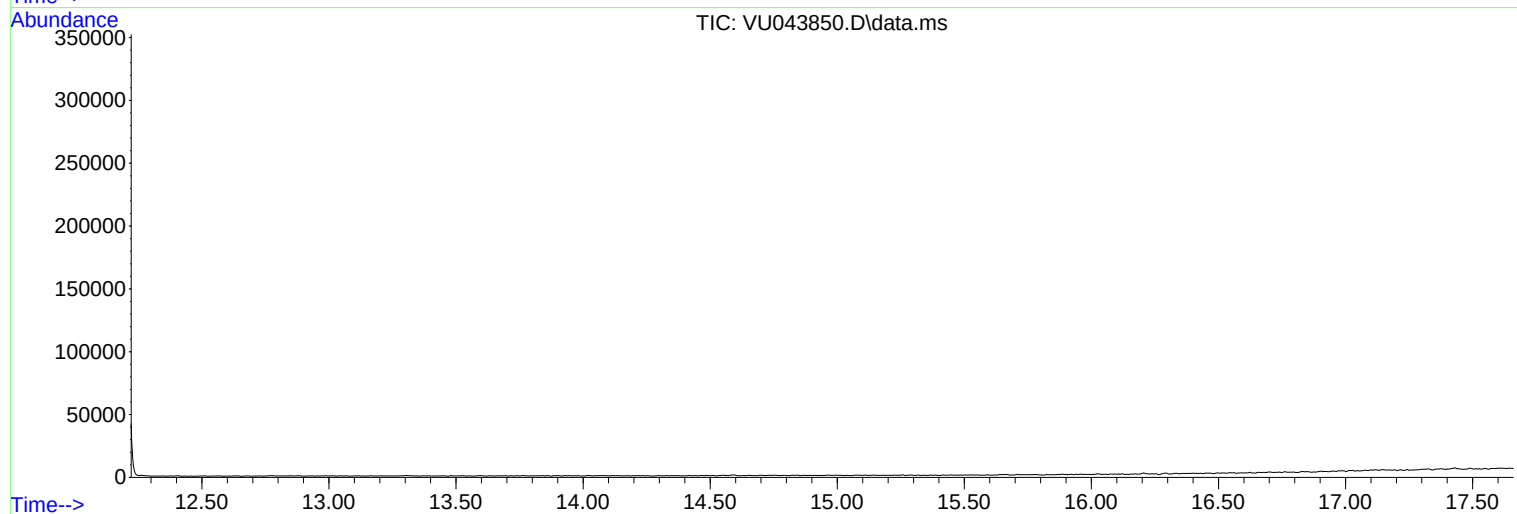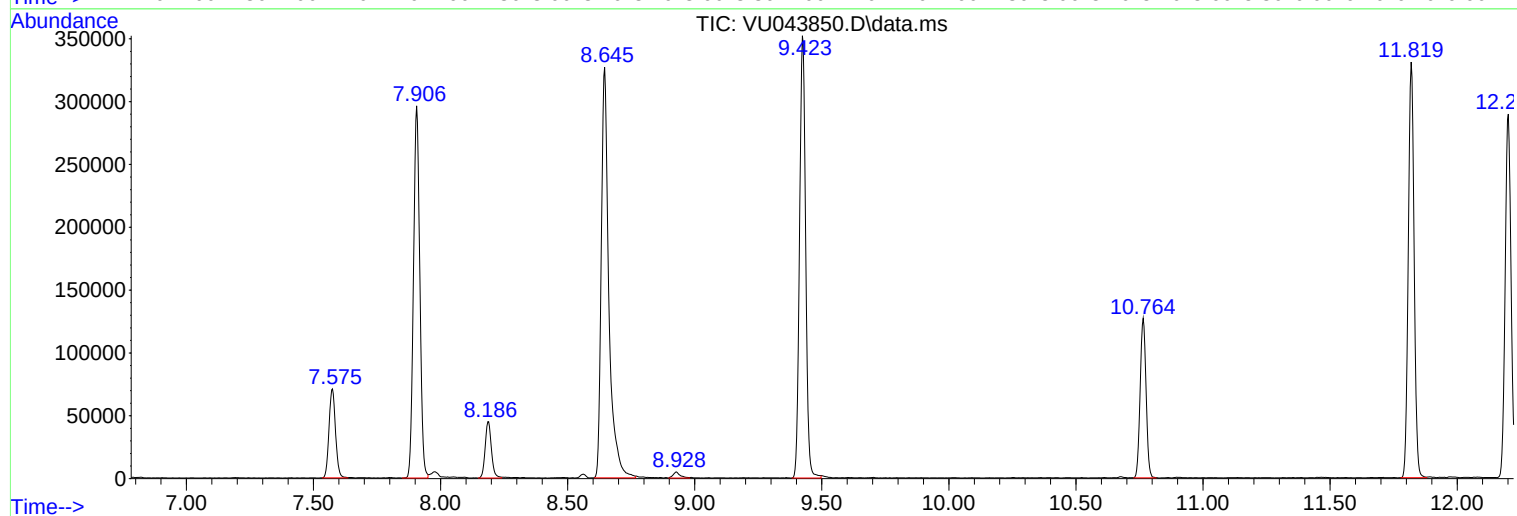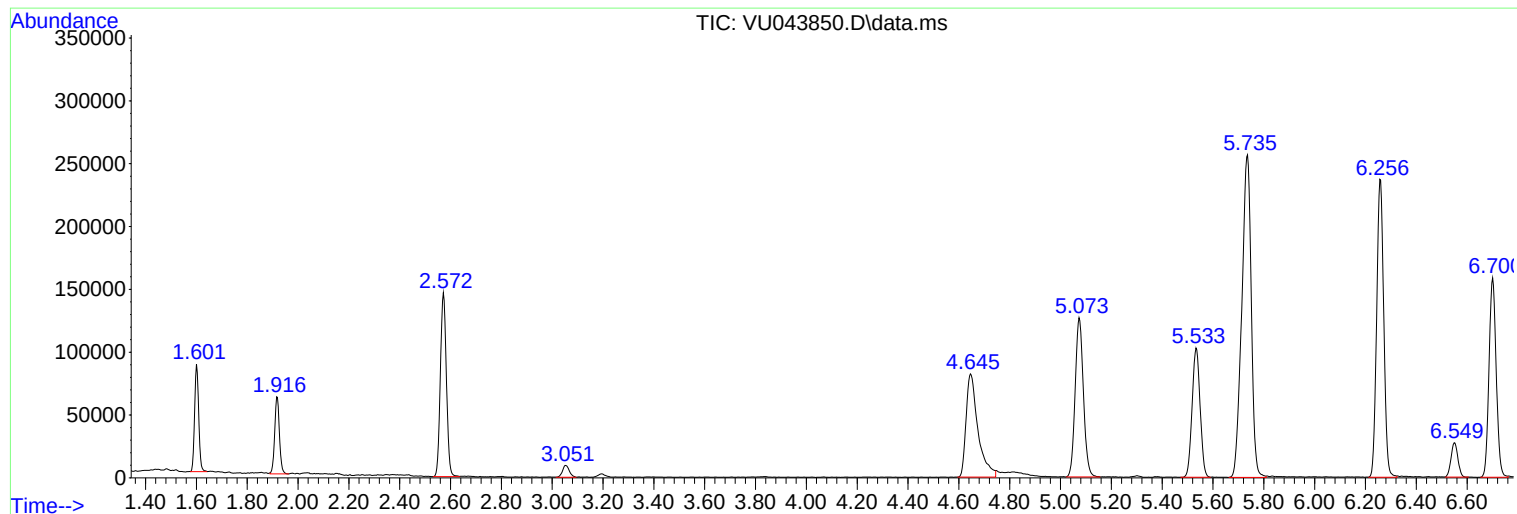

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043850.D
Acq On : 20 May 2021 00:41
Operator : SY/MD
Sample : M2459-07 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043850.D
Acq On : 20 May 2021 00:41
Operator : SY/MD
Sample : M2459-07 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
