

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
 Data File : VU043867.D
 Acq On : 20 May 2021 16:02
 Operator : SY/MD
 Sample : M2464-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	96	rVB	84157	96527	13.68%	1.654%
2	1.919	171	180	195	rVB	61363	77891	11.04%	1.335%
3	2.572	372	383	401	rBV	141445	232892	33.00%	3.992%
4	3.054	521	533	546	rBV	19337	36196	5.13%	0.620%
5	4.639	1008	1026	1051	rBV	100547	274759	38.93%	4.709%
6	5.073	1145	1161	1189	rVB	121998	292450	41.44%	5.012%
7	5.735	1345	1367	1388	rBV2	262606	674001	95.50%	11.552%
8	6.256	1515	1529	1553	rBV	244604	468853	66.43%	8.036%
9	6.700	1653	1667	1692	rBV	163348	317107	44.93%	5.435%
10	7.575	1925	1939	1958	rBV	76270	134920	19.12%	2.312%
11	7.906	2027	2042	2058	rBV	303193	523965	74.24%	8.981%
12	7.977	2058	2064	2080	rVB2	4813	8763	1.24%	0.150%
13	8.186	2118	2129	2146	rBV2	47268	80972	11.47%	1.388%
14	8.645	2258	2272	2303	rBV	358492	705759	100.00%	12.096%
15	9.423	2500	2514	2553	rBV	369494	615882	87.27%	10.556%
16	10.764	2919	2931	2948	rBV	133933	214105	30.34%	3.670%
17	10.899	2964	2973	2985	rVB2	5939	10409	1.47%	0.178%
18	11.819	3244	3259	3277	rBV	368236	571544	80.98%	9.796%
19	12.201	3364	3378	3396	rBV	305643	497471	70.49%	8.526%




Sum of corrected areas: 5834466

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043867.D
Acq On : 20 May 2021 16:02
Operator : SY/MD
Sample : M2464-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

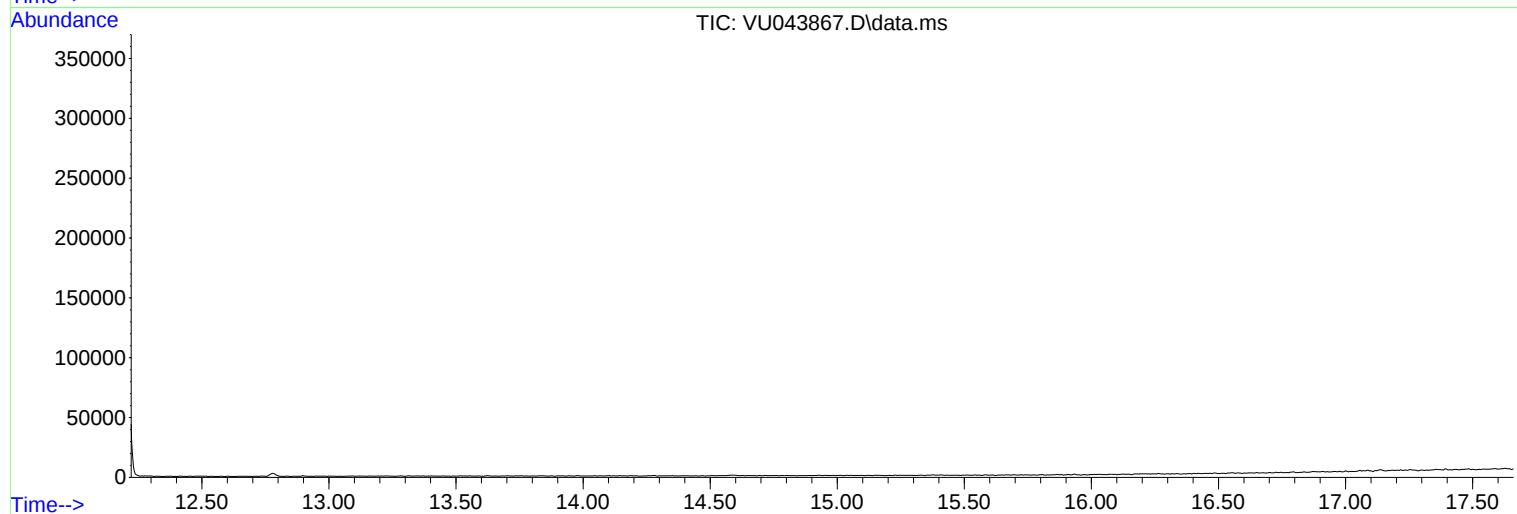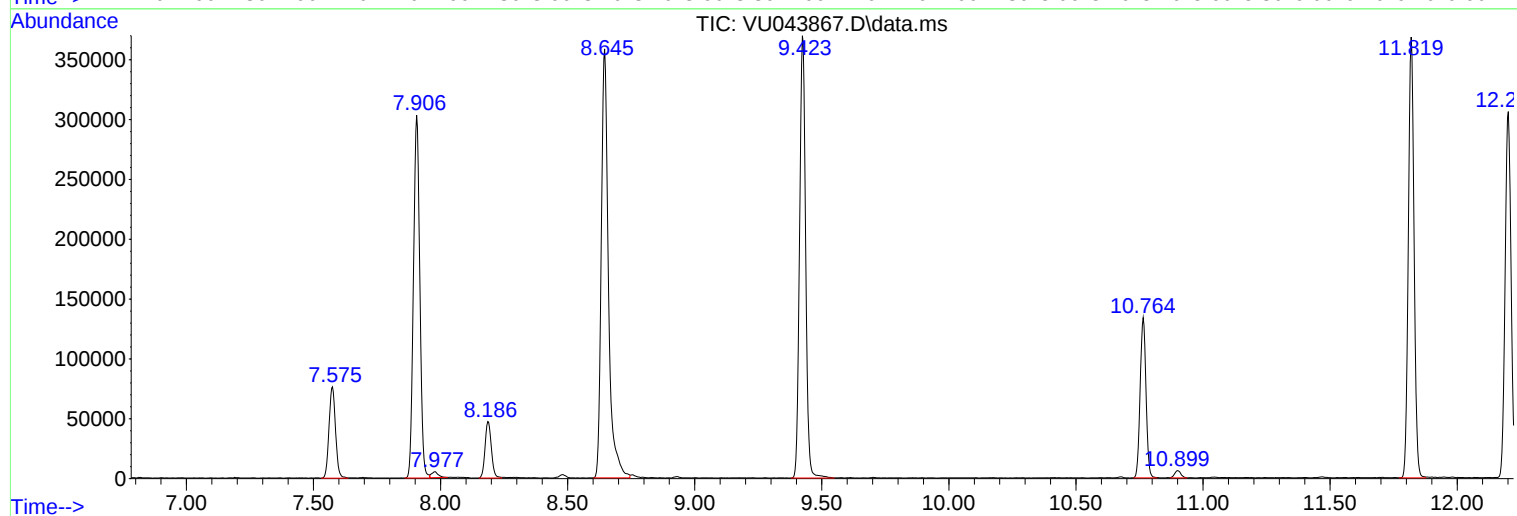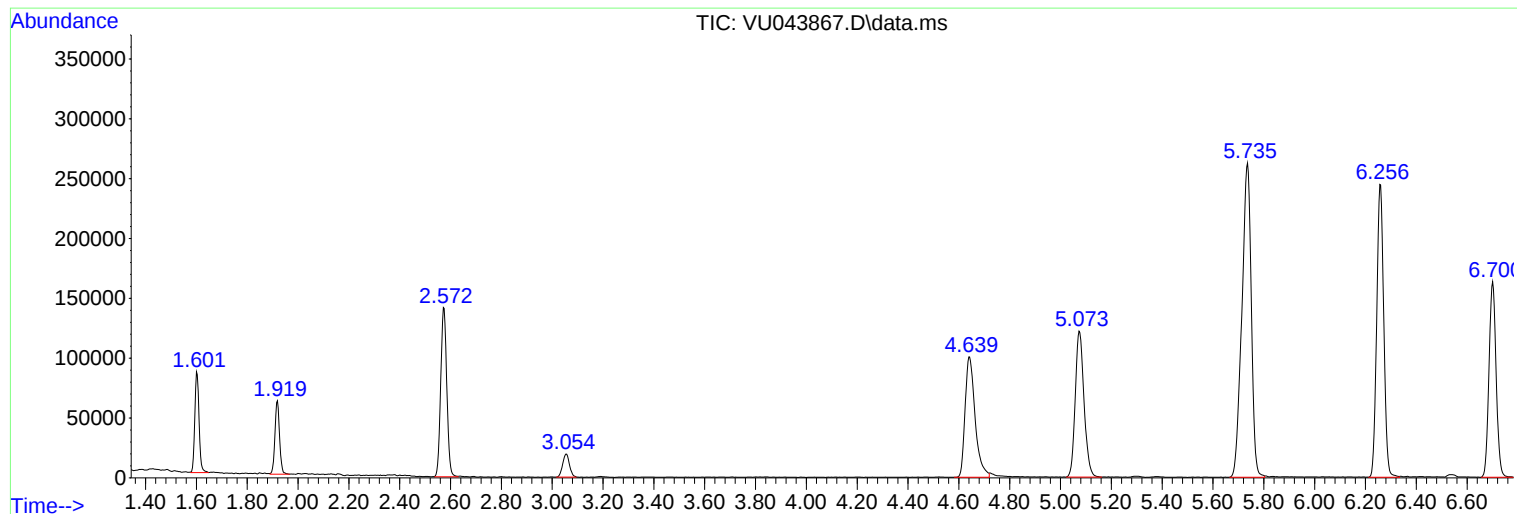

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043867.D
Acq On : 20 May 2021 16:02
Operator : SY/MD
Sample : M2464-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043867.D
Acq On : 20 May 2021 16:02
Operator : SY/MD
Sample : M2464-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
