

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
 Data File : VU043868.D
 Acq On : 20 May 2021 16:27
 Operator : SY/MD
 Sample : M2475-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB401

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	94	rVB	82309	92209	1.89%	0.725%
2	1.919	171	180	190	rVB	60952	78706	1.62%	0.619%
3	2.575	371	384	399	rBV2	137744	244840	5.03%	1.925%
4	4.639	1010	1026	1063	rBV2	119746	327058	6.72%	2.571%
5	5.073	1144	1161	1186	rBV3	131921	315204	6.47%	2.478%
6	5.327	1219	1240	1266	rBV	2154643	4870324	100.00%	38.289%
7	5.735	1346	1367	1391	rBV2	267224	685905	14.08%	5.392%
8	6.256	1515	1529	1551	rBV	250031	475739	9.77%	3.740%
9	6.700	1652	1667	1684	rBV2	163531	322174	6.62%	2.533%
10	7.575	1926	1939	1952	rBV	77624	136014	2.79%	1.069%
11	7.906	2025	2042	2056	rBV	306061	524861	10.78%	4.126%
12	8.186	2118	2129	2144	rBV	49402	82194	1.69%	0.646%
13	8.562	2232	2246	2260	rBV	1088924	1827652	37.53%	14.369%
14	8.642	2260	2271	2304	rVB	389797	760025	15.61%	5.975%
15	8.816	2312	2325	2339	rVB	29208	50821	1.04%	0.400%
16	9.423	2501	2514	2539	rBV	381373	623593	12.80%	4.903%
17	10.764	2912	2931	2950	rVB	133635	221359	4.55%	1.740%
18	11.819	3247	3259	3284	rBV	361771	576064	11.83%	4.529%
19	12.201	3365	3378	3396	rBV	311011	505034	10.37%	3.970%




Sum of corrected areas: 12719776

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043868.D
Acq On : 20 May 2021 16:27
Operator : SY/MD
Sample : M2475-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB401

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

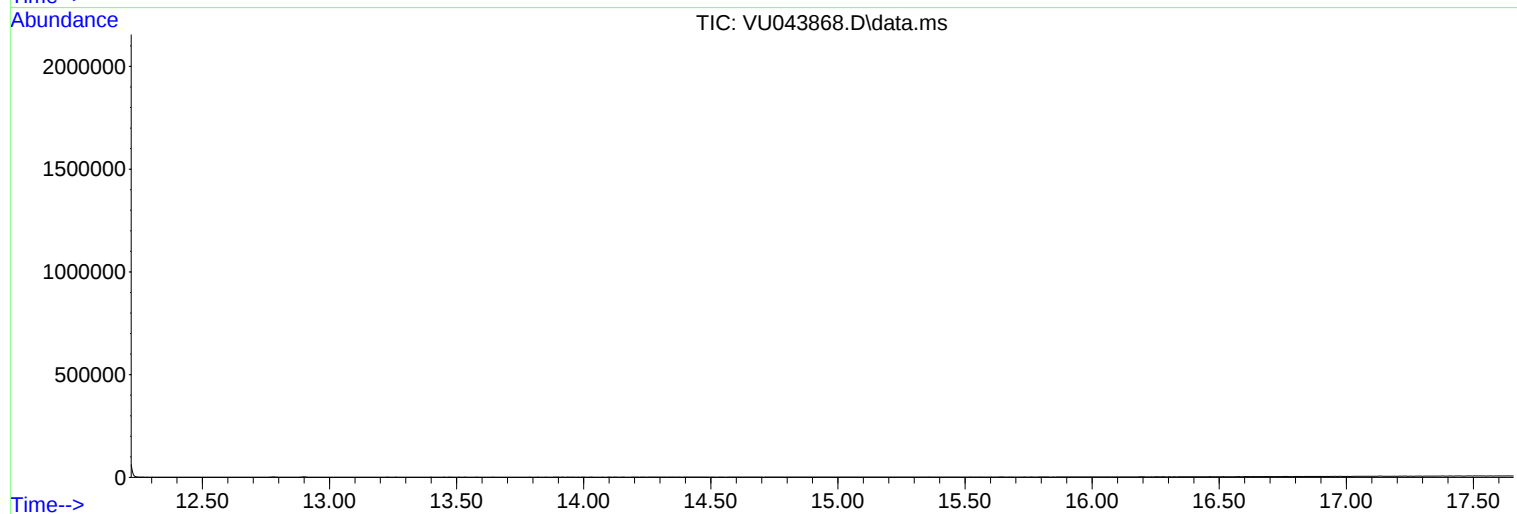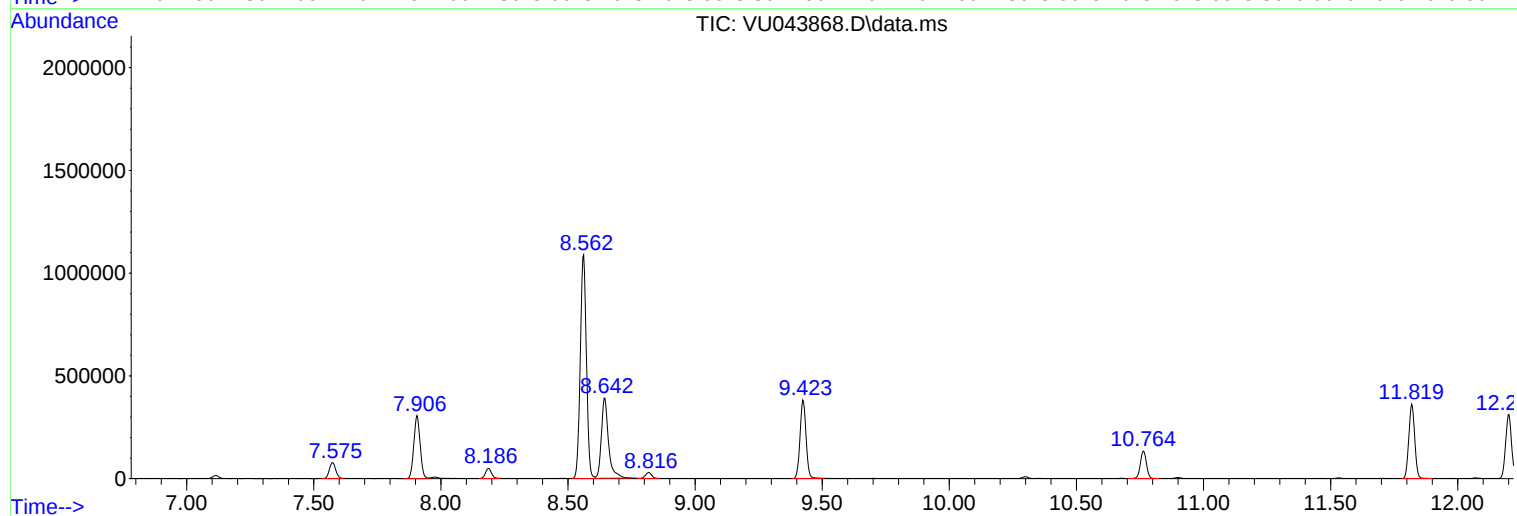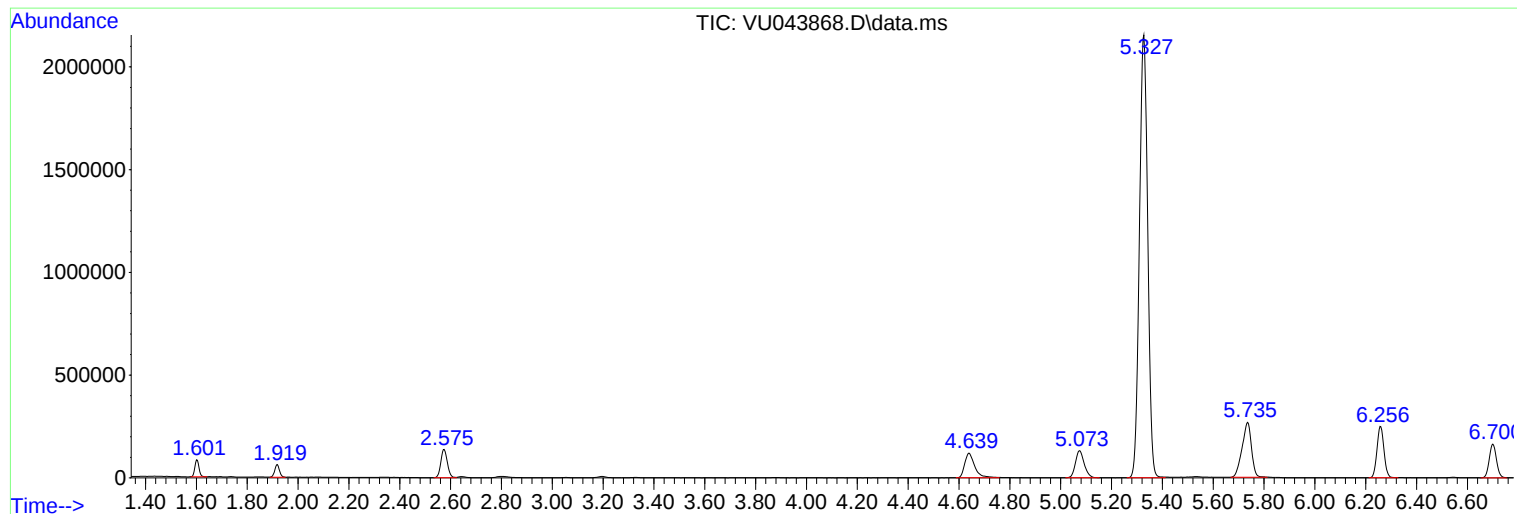

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043868.D
Acq On : 20 May 2021 16:27
Operator : SY/MD
Sample : M2475-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB401

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043868.D
Acq On : 20 May 2021 16:27
Operator : SY/MD
Sample : M2475-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB401

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
