

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
 Data File : VU043874.D
 Acq On : 20 May 2021 18:52
 Operator : SY/MD
 Sample : M2475-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB407

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043874.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	95	rVB	79706	88942	3.77%	1.010%
2	1.919	171	180	194	rVB	56857	75332	3.19%	0.855%
3	2.575	371	384	398	rBV2	117178	206773	8.77%	2.348%
4	3.883	775	791	808	rVB2	17945	40977	1.74%	0.465%
5	4.639	1009	1026	1071	rBV	100569	278033	11.79%	3.157%
6	5.076	1144	1162	1186	rBV2	120309	288767	12.24%	3.279%
7	5.327	1221	1240	1272	rBV	1052020	2358584	100.00%	26.780%
8	5.735	1346	1367	1384	rBV2	254501	655967	27.81%	7.448%
9	6.256	1509	1529	1550	rBV	249549	475287	20.15%	5.397%
10	6.700	1653	1667	1685	rBV	159957	309972	13.14%	3.520%
11	7.574	1926	1939	1954	rBV	72208	126270	5.35%	1.434%
12	7.906	2028	2042	2057	rBV	288902	498228	21.12%	5.657%
13	8.189	2116	2130	2145	rBV	46340	79649	3.38%	0.904%
14	8.562	2232	2246	2260	rBV	443071	751162	31.85%	8.529%
15	8.645	2260	2272	2311	rVB	353196	693693	29.41%	7.876%
16	9.423	2501	2514	2537	rBV	374391	620053	26.29%	7.040%
17	10.764	2919	2931	2946	rBV	127036	203624	8.63%	2.312%
18	11.819	3246	3259	3275	rBV	363714	572785	24.29%	6.504%
19	12.201	3363	3378	3391	rBV	295203	483038	20.48%	5.485%




Sum of corrected areas: 8807136

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043874.D
Acq On : 20 May 2021 18:52
Operator : SY/MD
Sample : M2475-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB407

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

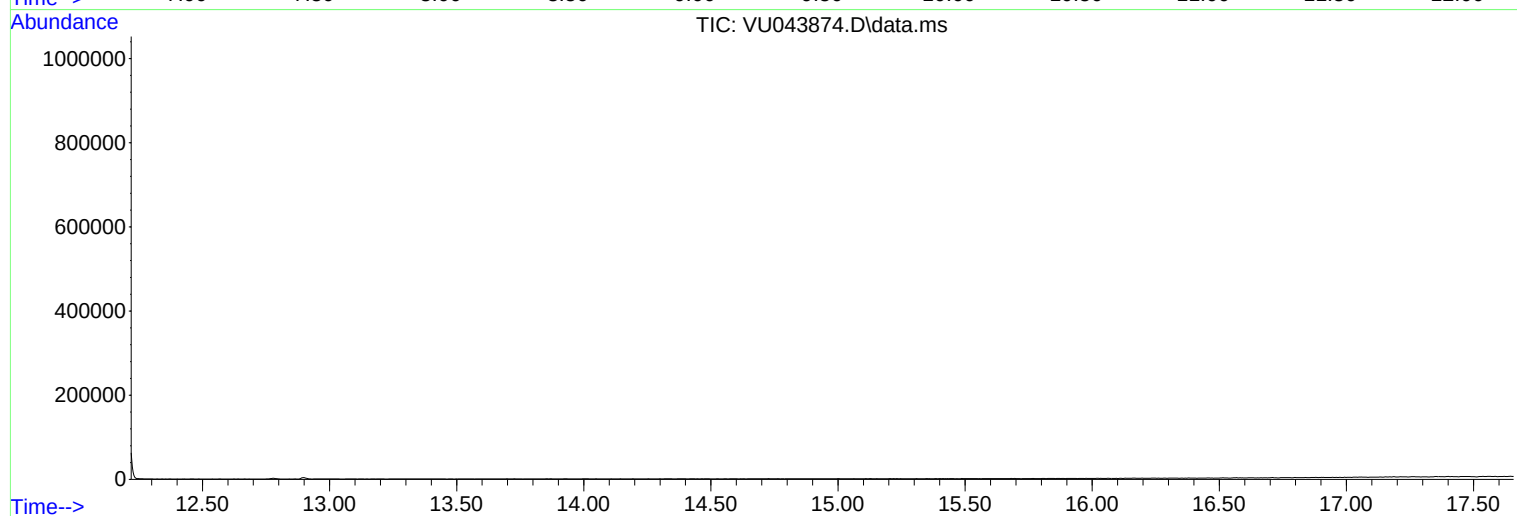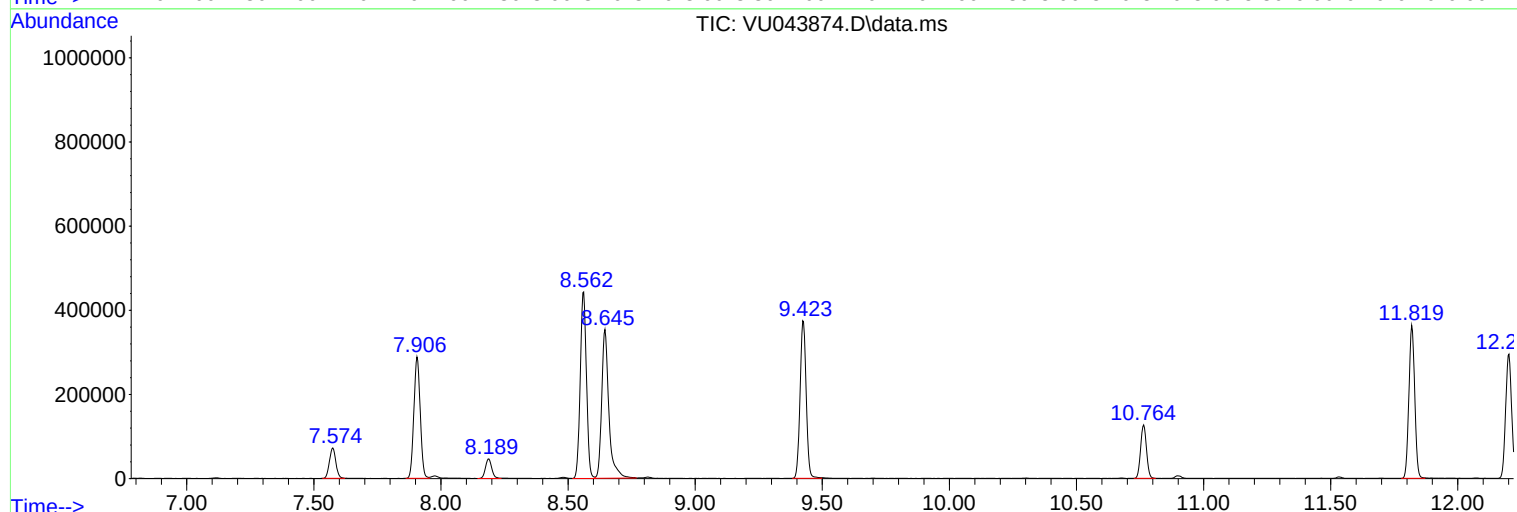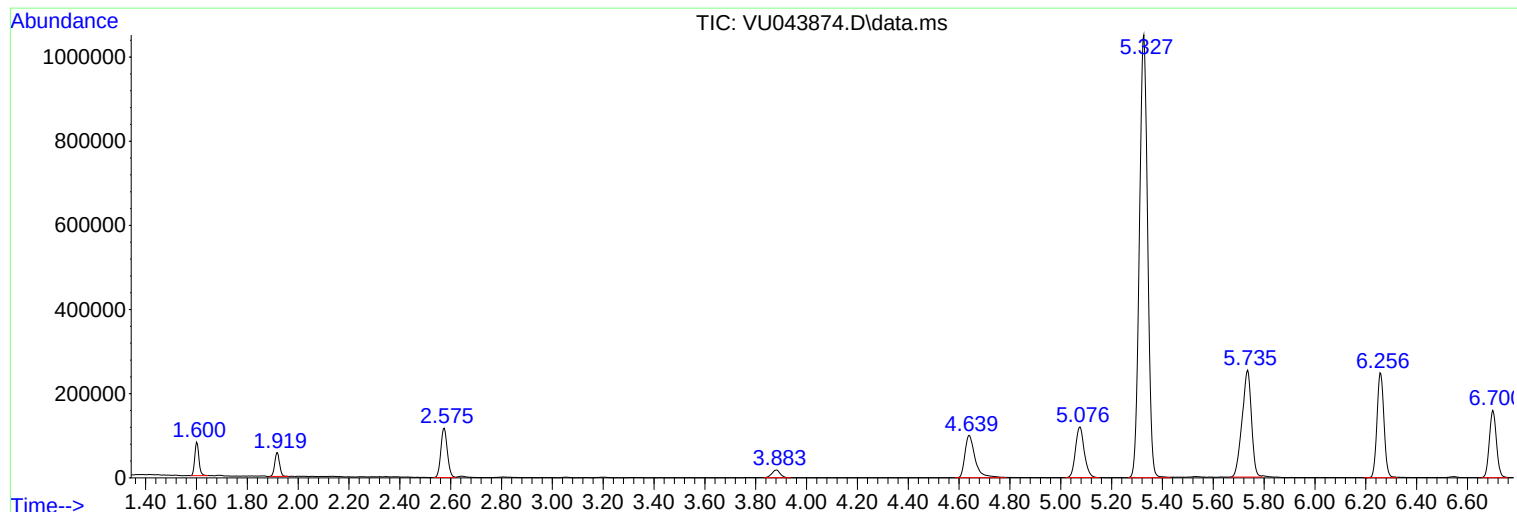

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043874.D
Acq On : 20 May 2021 18:52
Operator : SY/MD
Sample : M2475-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB407

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043874.D
Acq On : 20 May 2021 18:52
Operator : SY/MD
Sample : M2475-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB407

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
