


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
 Data File : VU043825.D
 Acq On : 19 May 2021 13:57
 Operator : SY/MD
 Sample : BFB47
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB147

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri May 21 01:15:23 2021

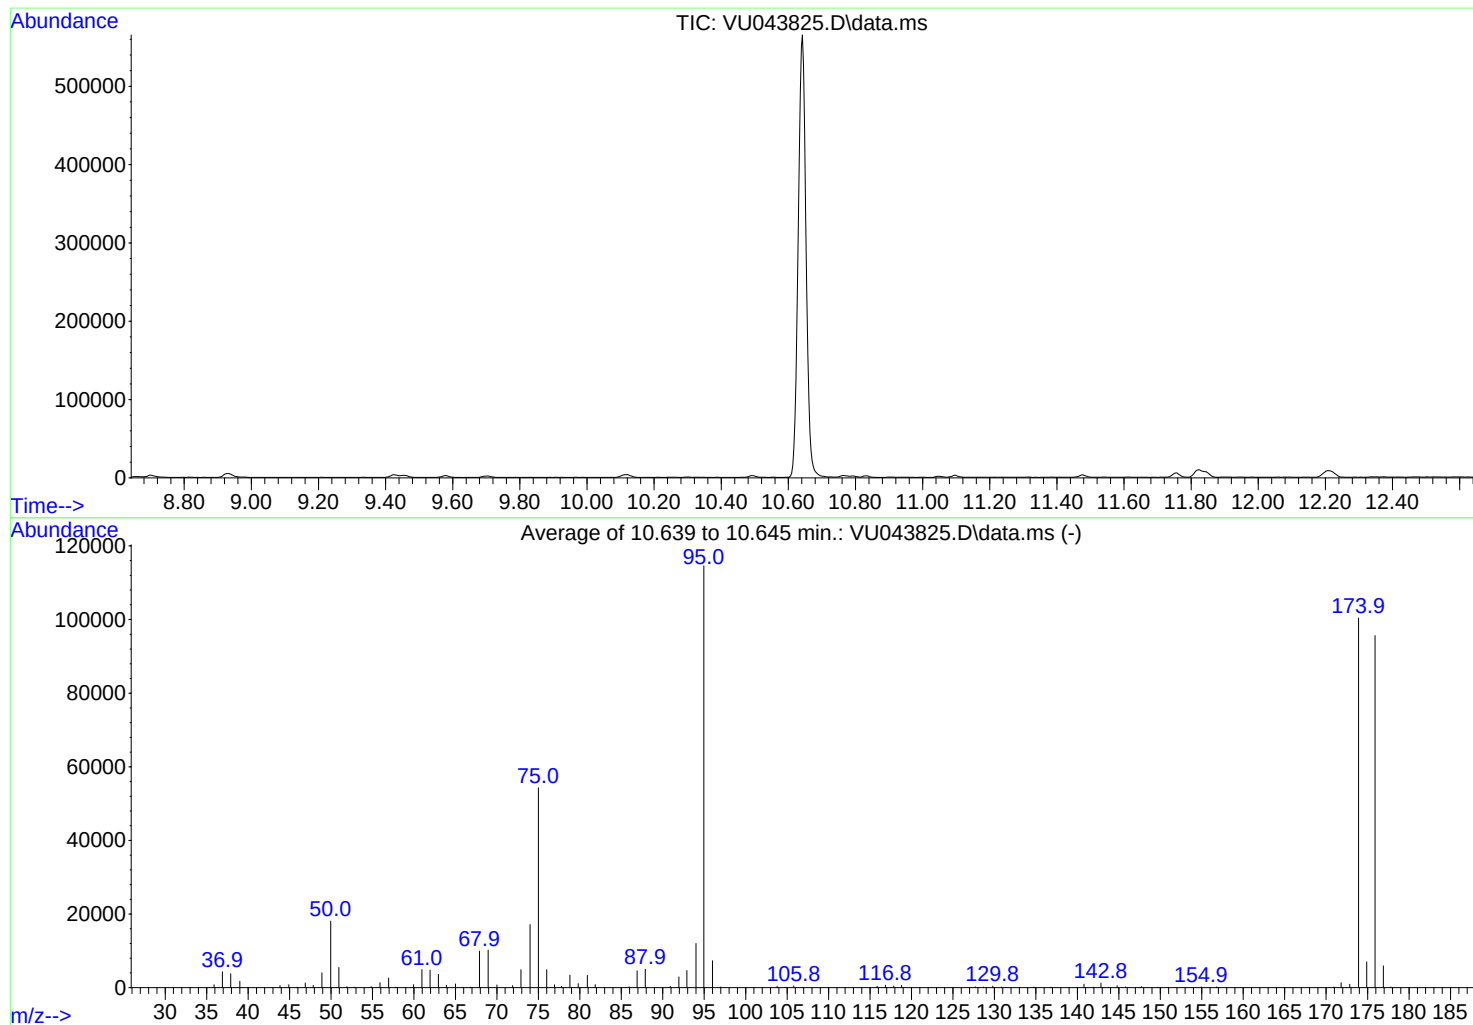

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	18099	PASS
75	95	30	80	47.4	54304	PASS
95	95	100	100	100.0	114592	PASS
96	95	5	9	6.4	7317	PASS
173	174	0.00	2	0.9	922	PASS
174	95	50	120	87.6	100392	PASS
175	174	5	9	7.0	7008	PASS
176	174	95	101	95.3	95635	PASS
177	176	5	9	6.2	5922	PASS

m/z	Abundance
39.90	202.0
43.80	592.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147

m/z	Abundance
35.90	825.0
36.90	4474.0
37.90	3908.0
39.00	1749.0
39.90	226.0
43.90	1159.0
44.90	807.0
45.90	127.0
46.90	1242.0
47.80	601.0
48.90	4120.0
50.00	18512.0
50.90	5677.0
51.90	265.0
52.80	166.0
54.90	280.0
55.90	1374.0
57.00	2535.0
57.80	148.0
60.00	877.0
61.00	5122.0
62.00	4976.0
63.00	3664.0
63.90	735.0
65.00	995.0
66.80	236.0
67.90	10054.0
68.90	10484.0
70.00	757.0
71.90	639.0
72.90	4792.0
74.00	17296.0
75.00	55352.0
76.00	4974.0
76.90	838.0
77.80	402.0
78.80	3454.0
79.80	1144.0
80.90	3422.0
81.80	790.0
86.00	203.0
86.90	4538.0
87.90	5274.0
90.90	372.0
91.90	3038.0
92.90	4813.0
94.00	12001.0
95.00	115696.0
96.00	7541.0
97.00	184.0
103.80	431.0
104.80	132.0
105.80	458.0
106.90	117.0
115.80	399.0
116.90	694.0
117.80	434.0
118.80	604.0
127.70	269.0
128.70	194.0
129.80	399.0
130.80	151.0
134.80	192.0
136.70	162.0
140.80	918.0
142.90	1287.0
143.80	121.0
144.80	543.0
145.80	238.0
147.80	235.0
154.90	263.0
156.80	224.0
171.00	202.0
171.80	1268.0
172.90	990.0
173.90	99840.0
174.90	7234.0
175.90	94536.0
176.90	5837.0
177.80	167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147

m/z	Abundance
35.90	813.0
36.90	4461.0
37.90	3825.0
39.00	1831.0
39.90	237.0
43.90	1196.0
44.90	795.0
45.90	136.0
46.90	1303.0
47.80	644.0
48.90	4192.0
49.90	18744.0
51.00	5671.0
51.90	289.0
52.90	156.0
54.90	271.0
55.90	1379.0
56.90	2690.0
57.80	130.0
59.90	862.0
60.90	5101.0
61.90	4818.0
63.00	3684.0
63.90	683.0
65.00	1048.0
66.80	209.0
67.90	10289.0
68.90	10498.0
70.00	769.0
71.90	606.0
72.90	5116.0
74.00	17560.0
75.00	56424.0
76.00	5022.0
76.90	812.0
77.80	413.0
78.80	3506.0
79.80	1119.0
80.90	3396.0
81.80	855.0
86.00	212.0
86.90	4635.0
87.90	5154.0
90.90	355.0
92.00	2990.0
92.90	4800.0
94.00	12459.0
94.90	118320.0
96.00	7602.0
97.00	156.0
103.80	425.0
104.80	128.0
105.80	466.0
106.90	115.0
115.80	410.0
116.80	661.0
117.80	482.0
118.80	636.0
127.70	226.0
128.70	197.0
129.80	465.0
130.80	174.0
134.70	162.0
136.80	149.0
140.80	1014.0
142.00	200.0
142.80	1271.0
143.70	114.0
144.80	538.0
145.80	224.0
147.80	290.0
149.70	113.0
154.90	236.0
156.80	227.0
171.00	201.0
171.80	1385.0
172.80	922.0
173.90	103696.0
174.90	7168.0
175.90	98616.0
176.90	6114.0
177.80	172.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147

m/z	Abundance
35.90	702.0
36.90	3989.0
37.90	3611.0
39.00	1684.0
39.90	253.0
43.90	1135.0
44.90	730.0
45.90	110.0
46.90	1242.0
47.90	574.0
48.90	3782.0
49.90	17040.0
51.00	5109.0
51.90	253.0
52.90	138.0
54.80	244.0
55.90	1274.0
56.90	2598.0
57.80	113.0
59.90	785.0
60.90	4567.0
61.90	4368.0
62.90	3510.0
63.90	575.0
65.00	976.0
65.80	115.0
67.00	166.0
67.90	9446.0
69.00	9668.0
70.00	758.0
71.90	482.0
72.90	4737.0
74.00	16480.0
75.00	51136.0
76.00	4614.0
77.00	678.0
77.80	386.0
78.80	3221.0
79.80	1019.0
80.90	3205.0
81.90	825.0
85.90	212.0
86.90	4571.0
87.90	4618.0
90.90	317.0
92.00	2690.0
92.90	4397.0
94.00	11573.0
94.90	109760.0
96.00	6809.0
96.90	139.0
103.80	355.0
104.70	125.0
105.80	463.0
115.90	380.0
116.80	592.0
117.90	430.0
118.80	577.0
127.70	212.0
128.70	162.0
129.80	491.0
130.90	158.0
134.80	136.0
136.90	155.0
140.80	943.0
141.90	241.0
142.80	1181.0
144.80	453.0
145.80	184.0
147.70	293.0
149.70	119.0
153.80	101.0
155.00	199.0
156.80	205.0
170.90	162.0
171.80	1376.0
172.80	854.0
173.90	97640.0
174.90	6622.0
175.90	93752.0
176.90	5814.0
177.80	177.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147