
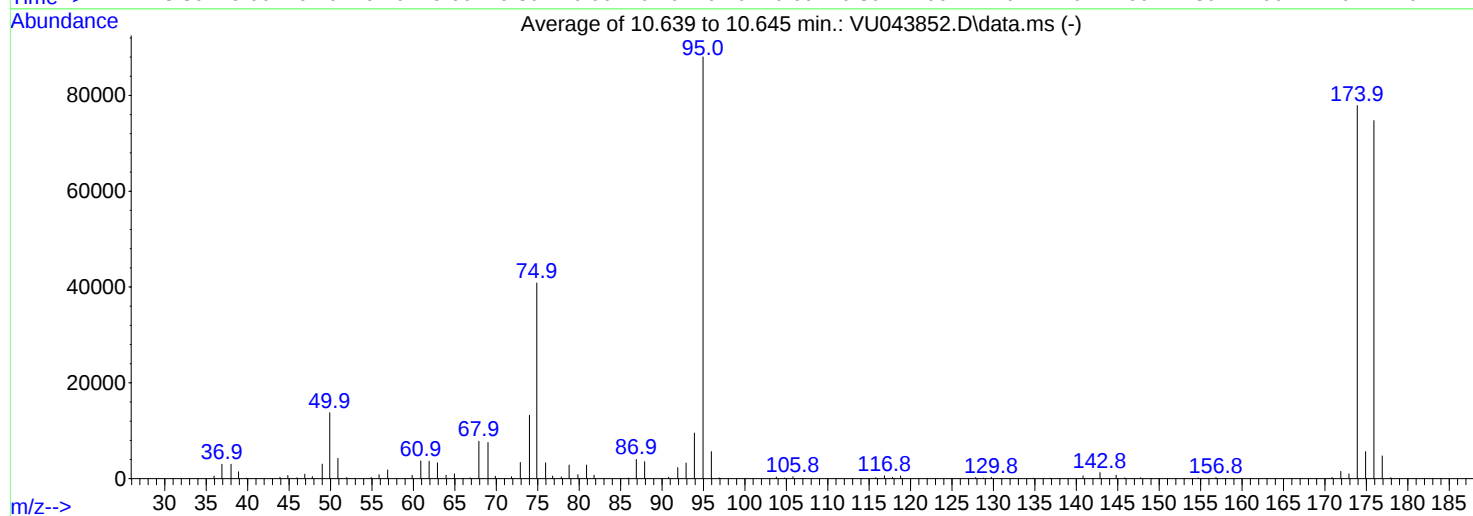


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
 Data File : VU043852.D
 Acq On : 20 May 2021 09:09
 Operator : SY/MD
 Sample : BFB48
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB148

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri May 21 01:15:23 2021

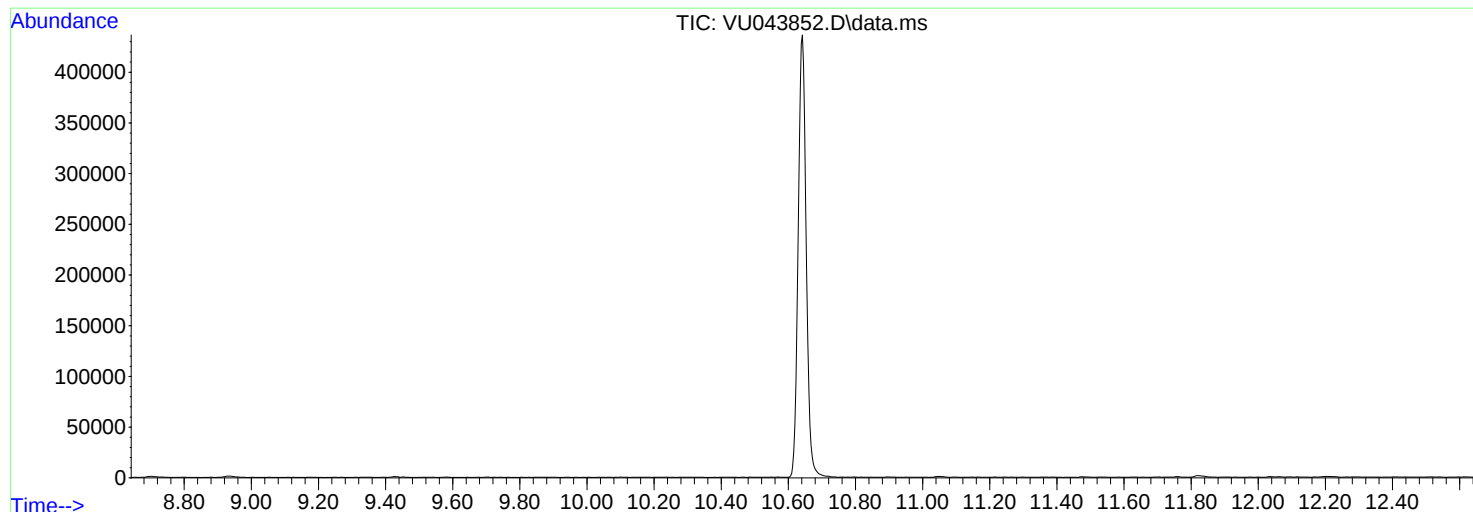

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	13764	PASS
75	95	30	80	46.4	40853	PASS
95	95	100	100	100.0	88056	PASS
96	95	5	9	6.4	5636	PASS
173	174	0.00	2	1.3	998	PASS
174	95	50	120	88.5	77893	PASS
175	174	5	9	7.3	5650	PASS
176	174	95	101	96.0	74755	PASS
177	176	5	9	6.4	4748	PASS

m/z	Abundance
39.80	147.0
43.90	492.0

Instrument :
MSVOA_U
ClientSampleId :
BFB148

m/z	Abundance
35.90	487.0
36.90	3043.0
38.00	3080.0
38.90	1496.0
39.90	267.0
43.90	797.0
44.90	763.0
46.00	170.0
46.90	945.0
47.80	479.0
49.00	3101.0
49.90	14249.0
50.90	4357.0
52.00	211.0
53.00	114.0
54.90	247.0
55.80	896.0
56.90	1889.0
59.90	756.0
60.90	3775.0
61.90	3702.0
62.90	3431.0
63.90	750.0
65.00	944.0
66.00	106.0
66.90	163.0
67.90	8071.0
69.00	7788.0
69.90	509.0
71.90	349.0
72.90	3281.0
74.00	13482.0
74.90	41800.0
76.00	3401.0
76.80	576.0
77.80	377.0
78.80	3042.0
79.80	876.0
80.90	2811.0
81.80	741.0
85.80	190.0
86.90	3970.0
87.90	3618.0
90.80	330.0
91.90	2412.0
92.90	3138.0
93.90	9556.0
95.00	88936.0
96.00	5943.0
96.90	162.0
103.80	358.0
104.70	121.0
105.80	419.0
115.80	220.0
116.90	603.0
117.90	296.0
118.80	529.0
127.80	290.0
128.80	143.0
129.70	273.0
130.80	123.0
134.90	124.0
140.80	573.0
142.90	1308.0
144.80	721.0
145.80	200.0
146.70	105.0
147.70	237.0
154.70	154.0
156.80	225.0
170.80	271.0
171.90	1553.0
172.90	1005.0
173.90	77448.0
174.90	5837.0
175.90	74168.0
176.90	4903.0
178.00	192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB148

m/z	Abundance
36.00	526.0
36.90	3084.0
38.00	3101.0
38.90	1475.0
39.90	264.0
43.90	828.0
44.80	685.0
45.90	228.0
46.90	968.0
47.80	462.0
49.00	3092.0
49.90	14122.0
50.90	4354.0
51.90	241.0
53.00	117.0
54.90	271.0
55.80	839.0
56.90	1832.0
59.90	698.0
60.90	3790.0
61.90	3678.0
62.90	3444.0
64.00	738.0
64.90	1015.0
66.00	103.0
66.80	176.0
67.90	8033.0
69.00	7674.0
69.90	501.0
71.90	421.0
72.90	3497.0
74.00	13649.0
74.90	42160.0
76.00	3407.0
76.80	561.0
77.80	364.0
78.80	2886.0
79.90	863.0
80.90	2926.0
81.80	756.0
86.00	189.0
86.90	4149.0
87.90	3646.0
90.80	334.0
91.90	2351.0
92.90	3340.0
93.90	9794.0
94.90	90808.0
96.00	5815.0
96.90	164.0
103.80	353.0
104.80	130.0
105.80	431.0
115.80	250.0
116.80	640.0
117.80	288.0
118.80	619.0
127.90	228.0
128.80	128.0
129.80	281.0
130.80	108.0
134.80	121.0
136.90	127.0
140.80	589.0
142.90	1267.0
144.80	754.0
145.90	174.0
147.80	197.0
154.70	152.0
156.80	236.0
170.80	289.0
171.90	1565.0
172.90	1041.0
173.90	80128.0
174.90	5881.0
175.90	77112.0
176.90	4921.0
177.90	205.0

Instrument :
MSVOA_U
ClientSampleId :
BFB148

m/z	Abundance
36.00	550.0
36.90	2902.0
38.00	2838.0
38.90	1328.0
39.90	217.0
43.90	785.0
44.90	537.0
45.90	209.0
46.90	873.0
47.80	370.0
49.00	2910.0
49.90	12920.0
50.90	4035.0
51.90	218.0
53.00	112.0
54.90	253.0
55.90	769.0
56.90	1656.0
59.80	634.0
60.90	3571.0
61.90	3562.0
62.90	3053.0
64.00	650.0
64.90	1014.0
66.80	180.0
67.90	7391.0
69.00	7150.0
69.90	509.0
71.80	443.0
72.90	3384.0
74.00	12588.0
74.90	38600.0
75.90	3118.0
76.80	494.0
77.90	366.0
78.80	2600.0
79.90	820.0
80.90	2820.0
81.80	736.0
86.00	212.0
86.90	3923.0
87.90	3403.0
90.80	253.0
91.90	2177.0
92.90	3375.0
93.90	9208.0
94.90	84424.0
95.90	5149.0
96.90	144.0
103.80	316.0
104.90	132.0
105.80	372.0
115.80	263.0
116.80	607.0
117.70	299.0
118.80	613.0
127.80	210.0
128.80	114.0
129.80	240.0
134.70	102.0
136.80	158.0
140.80	574.0
142.80	1218.0
144.80	694.0
145.90	162.0
147.80	140.0
154.70	176.0
156.90	209.0
170.90	279.0
171.90	1444.0
172.90	948.0
173.90	76104.0
174.90	5233.0
175.90	72984.0
176.90	4421.0
177.90	168.0

Instrument :
MSVOA_U
ClientSampleId :
BFB148