

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
 Data File : VU048643.D
 Acq On : 20 May 2022 11:15
 Operator : SY/MD
 Sample : VU0520MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK134

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048643.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	94	rVB	64328	72391	8.97%	1.092%
2	1.912	170	178	194	rVB	56085	71785	8.89%	1.083%
3	2.260	283	286	290	rVB	344	233	0.03%	0.004%
4	2.462	345	349	353	rVB2	322	296	0.04%	0.004%
5	2.568	370	382	398	rBV	154298	254127	31.48%	3.834%
6	2.793	445	452	460	rVV	879	1307	0.16%	0.020%
7	2.835	463	465	469	rVB2	226	147	0.02%	0.002%
8	2.896	480	484	487	rBB2	249	146	0.02%	0.002%
9	2.973	504	508	511	rBB	178	177	0.02%	0.003%
10	3.047	524	531	539	rVV2	1533	2272	0.28%	0.034%
11	3.189	566	575	578	rBV2	1898	2829	0.35%	0.043%
12	3.359	625	628	632	rBV	210	198	0.02%	0.003%
13	3.382	632	635	638	rVV2	368	221	0.03%	0.003%
14	3.530	678	681	685	rBB	160	163	0.02%	0.002%
15	3.655	717	720	725	rBB	212	180	0.02%	0.003%
16	3.890	790	793	797	rBB	179	144	0.02%	0.002%
17	4.083	851	853	857	rBB	203	153	0.02%	0.002%
18	4.118	861	864	867	rBV	165	156	0.02%	0.002%
19	4.446	963	966	969	rBB	190	146	0.02%	0.002%
20	4.626	1009	1022	1048	rBV	84201	219408	27.18%	3.310%
21	4.845	1087	1090	1091	rBV	276	154	0.02%	0.002%
22	4.899	1105	1107	1111	rVB	307	215	0.03%	0.003%
23	4.941	1117	1120	1123	rBB2	263	154	0.02%	0.002%
24	4.970	1128	1129	1133	rVB2	361	196	0.02%	0.003%
25	4.993	1133	1136	1140	rBV	165	188	0.02%	0.003%
26	5.067	1140	1159	1182	rBV	161584	353722	43.82%	5.337%
27	5.292	1225	1229	1232	rBB	351	307	0.04%	0.005%
28	5.726	1343	1364	1393	rBV2	292821	807222	100.00%	12.179%
29	5.851	1400	1403	1406	rBV2	390	257	0.03%	0.004%
30	5.899	1415	1418	1420	rBV	209	163	0.02%	0.002%
31	5.957	1433	1436	1440	rBB2	341	234	0.03%	0.004%
32	6.041	1460	1462	1464	rBV	256	164	0.02%	0.002%
33	6.250	1513	1527	1547	rBV	265288	501252	62.10%	7.562%
34	6.362	1560	1562	1566	rVB2	463	296	0.04%	0.004%
35	6.488	1596	1601	1604	rBV2	312	298	0.04%	0.004%
36	6.536	1606	1616	1625	rVV5	3779	7251	0.90%	0.109%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
 Data File : VU048643.D
 Acq On : 20 May 2022 11:15
 Operator : SY/MD
 Sample : VU0520MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK134

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	6.642	1645	1649	1651	rBB	277	177	0.02%	0.003%
38	6.694	1651	1665	1682	rBV	184661	358263	44.38%	5.405%
39	6.809	1697	1701	1704	rBV2	470	355	0.04%	0.005%
40	6.825	1704	1706	1709	rVB	389	185	0.02%	0.003%
41	6.841	1709	1711	1714	rBB2	385	199	0.02%	0.003%
42	6.996	1755	1759	1761	rBV	166	163	0.02%	0.002%
43	7.182	1811	1817	1826	rBV6	1581	2368	0.29%	0.036%
44	7.504	1915	1917	1921	rBB	177	150	0.02%	0.002%
45	7.565	1922	1936	1956	rBV	108503	193091	23.92%	2.913%
46	7.648	1960	1962	1968	rVB2	742	568	0.07%	0.009%
47	7.677	1968	1971	1972	rBV	402	258	0.03%	0.004%
48	7.694	1972	1976	1985	rVB5	1253	1632	0.20%	0.025%
49	7.732	1986	1988	1990	rBV	248	165	0.02%	0.002%
50	7.787	2002	2005	2007	rBV2	418	300	0.04%	0.005%
51	7.899	2024	2040	2056	rBV	375763	646287	80.06%	9.751%
52	8.179	2116	2127	2145	rBV	81742	139462	17.28%	2.104%
53	8.423	2201	2203	2206	rBV2	208	144	0.02%	0.002%
54	8.513	2227	2231	2233	rBB	274	151	0.02%	0.002%
55	8.526	2233	2235	2240	rBB2	337	268	0.03%	0.004%
56	8.552	2240	2243	2246	rBV2	281	245	0.03%	0.004%
57	8.636	2257	2269	2300	rBV	255887	477667	59.17%	7.207%
58	8.915	2354	2356	2359	rBV2	454	341	0.04%	0.005%
59	9.028	2387	2391	2394	rBB	208	189	0.02%	0.003%
60	9.105	2412	2415	2417	rBV	208	171	0.02%	0.003%
61	9.195	2441	2443	2447	rBV	185	193	0.02%	0.003%
62	9.288	2469	2472	2476	rBB	278	220	0.03%	0.003%
63	9.317	2476	2481	2485	rBV	237	301	0.04%	0.005%
64	9.417	2499	2512	2530	rBV	380823	636361	78.83%	9.601%
65	9.574	2556	2561	2567	rVB2	571	704	0.09%	0.011%
66	9.658	2580	2587	2590	rBV	376	378	0.05%	0.006%
67	9.690	2593	2597	2598	rBV2	572	384	0.05%	0.006%
68	9.835	2639	2642	2646	rBV	209	232	0.03%	0.004%
69	9.880	2652	2656	2657	rBV	274	162	0.02%	0.002%
70	9.973	2681	2685	2688	rBV	196	211	0.03%	0.003%
71	10.025	2699	2701	2704	rBV	165	140	0.02%	0.002%
72	10.086	2718	2720	2724	rBV	331	323	0.04%	0.005%
73	10.198	2753	2755	2758	rBV	331	176	0.02%	0.003%
74	10.234	2762	2766	2776	rBV	351	522	0.06%	0.008%
75	10.308	2785	2789	2791	rBV	186	187	0.02%	0.003%
76	10.359	2802	2805	2812	rBB	140	201	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
 Data File : VU048643.D
 Acq On : 20 May 2022 11:15
 Operator : SY/MD
 Sample : VU0520MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK134

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	10.423	2819	2825	2830	rBV	229	333	0.04%	0.005%
78	10.481	2838	2843	2846	rBV2	575	565	0.07%	0.009%
79	10.632	2886	2890	2898	rVB3	1126	1360	0.17%	0.021%
80	10.758	2916	2929	2948	rBV	289176	468224	58.00%	7.064%
81	10.825	2948	2950	2954	rVB	427	224	0.03%	0.003%
82	10.896	2970	2972	2977	rBV2	382	262	0.03%	0.004%
83	11.092	3029	3033	3041	rBV3	437	597	0.07%	0.009%
84	11.468	3146	3150	3159	rVB3	1102	1584	0.20%	0.024%
85	11.568	3176	3181	3183	rBV2	191	168	0.02%	0.003%
86	11.751	3230	3238	3244	rBV4	1007	1478	0.18%	0.022%
87	11.812	3244	3257	3272	rBV	424664	676865	83.85%	10.212%
88	11.941	3295	3297	3302	rVB	431	186	0.02%	0.003%
89	12.118	3348	3352	3357	rBV	253	203	0.03%	0.003%
90	12.192	3362	3375	3393	rBV	423985	693612	85.93%	10.464%
91	12.693	3529	3531	3536	rVB2	275	218	0.03%	0.003%
92	12.886	3588	3591	3594	rBV2	290	201	0.02%	0.003%
93	12.912	3597	3599	3605	rVB2	521	403	0.05%	0.006%
94	13.047	3639	3641	3647	rVB	324	182	0.02%	0.003%
95	13.221	3691	3695	3705	rVB3	912	1400	0.17%	0.021%
96	13.436	3759	3762	3767	rBV3	455	401	0.05%	0.006%
97	13.848	3883	3890	3899	rVB5	2229	3804	0.47%	0.057%
98	14.089	3958	3965	3977	rBV2	7651	12458	1.54%	0.188%
99	14.330	4036	4040	4041	rBV4	1727	1268	0.16%	0.019%
100	14.841	4197	4199	4202	rBV	519	199	0.02%	0.003%




Sum of corrected areas: 6628241

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
Data File : VU048643.D
Acq On : 20 May 2022 11:15
Operator : SY/MD
Sample : VU0520MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK134

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

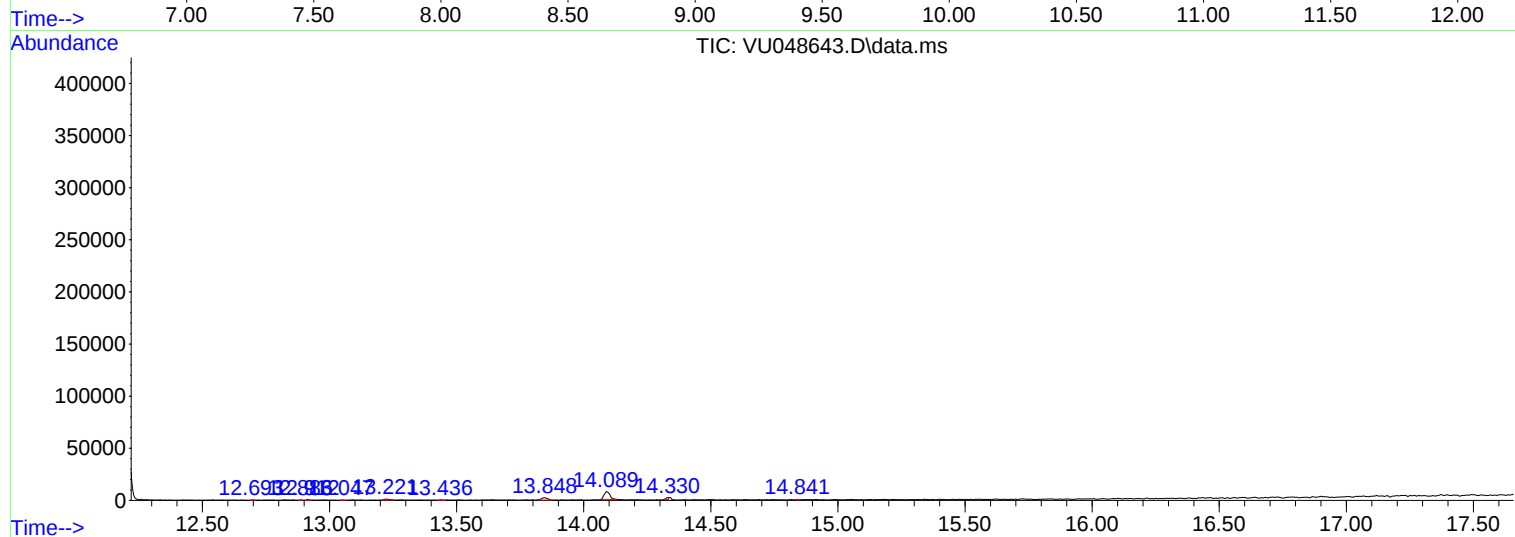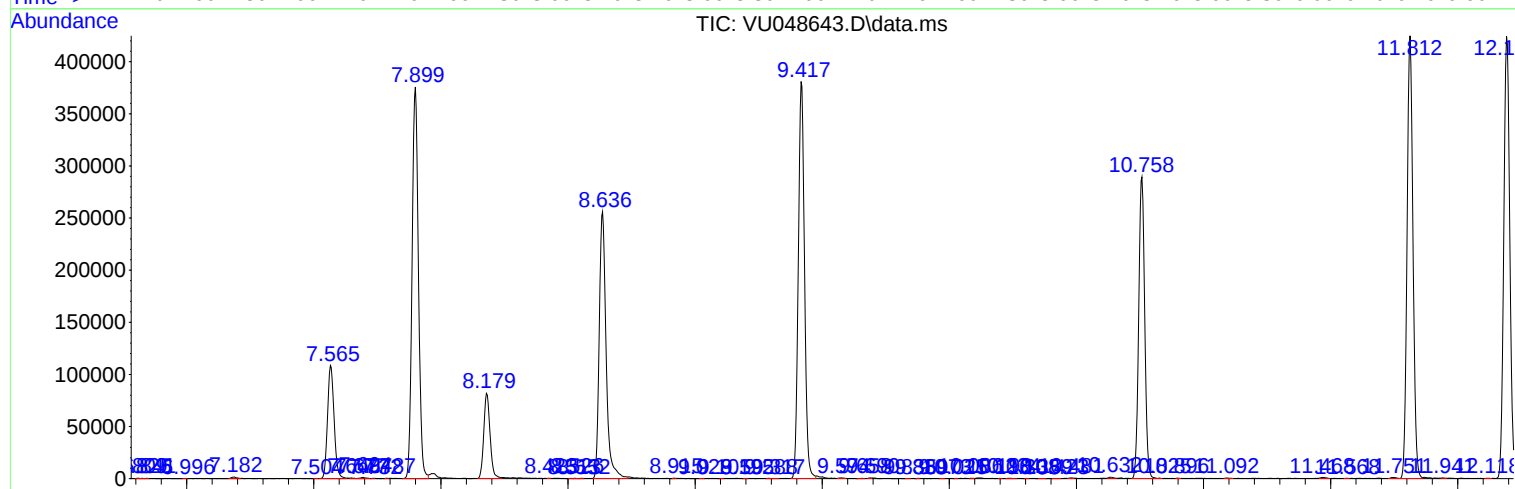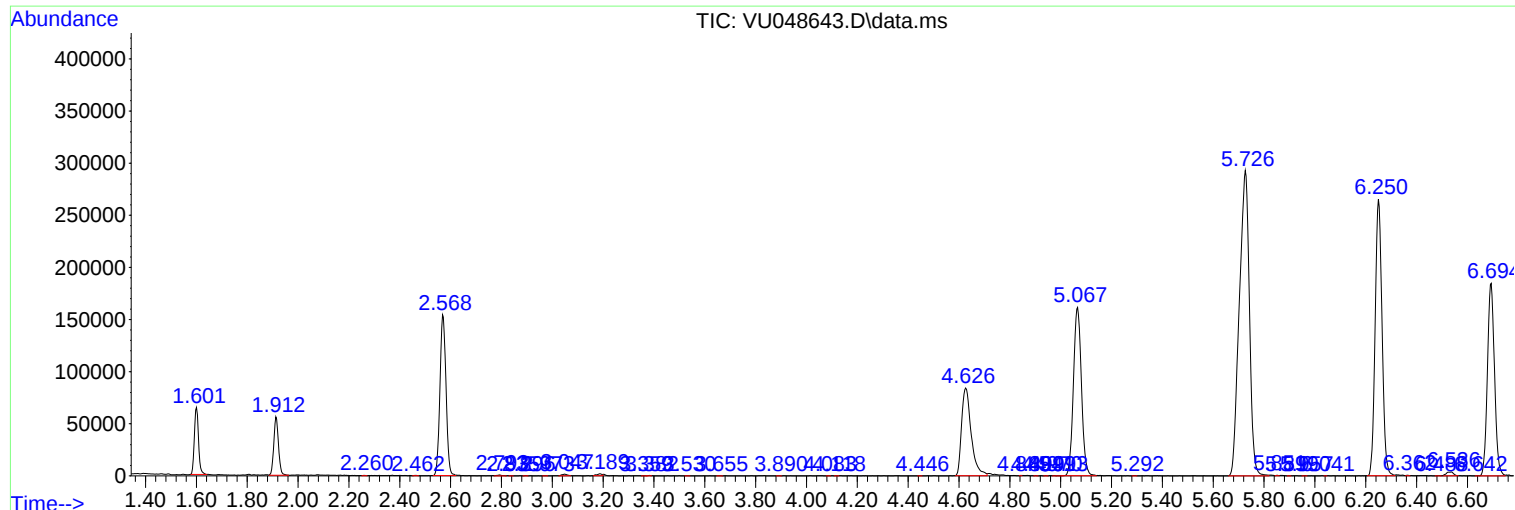

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
Data File : VU048643.D
Acq On : 20 May 2022 11:15
Operator : SY/MD
Sample : VU0520MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK134

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
Data File : VU048643.D
Acq On : 20 May 2022 11:15
Operator : SY/MD
Sample : VU0520MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK134

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
