

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
 Data File : VU048644.D
 Acq On : 20 May 2022 12:16
 Operator : SY/MD
 Sample : VU0520WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK135

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	97	rVB	66271	76711	8.97%	1.101%
2	1.912	170	178	193	rVB	61851	79838	9.34%	1.146%
3	2.568	368	382	403	rBV	164273	269914	31.57%	3.873%
4	2.735	432	434	436	rBV	299	164	0.02%	0.002%
5	2.938	493	497	499	rBV	216	185	0.02%	0.003%
6	3.041	525	529	531	rBV	879	683	0.08%	0.010%
7	3.186	568	574	577	rBV2	463	642	0.08%	0.009%
8	3.288	603	606	609	rBB	177	138	0.02%	0.002%
9	3.372	629	632	636	rVB	206	184	0.02%	0.003%
10	3.658	718	721	725	rBB	306	219	0.03%	0.003%
11	3.687	726	730	734	rBB	207	217	0.03%	0.003%
12	4.256	904	907	913	rBB2	274	231	0.03%	0.003%
13	4.308	918	923	925	rBB	297	191	0.02%	0.003%
14	4.465	967	972	977	rBB	322	291	0.03%	0.004%
15	4.629	1010	1023	1058	rBV	85592	225594	26.39%	3.237%
16	4.874	1096	1099	1104	rBV	279	263	0.03%	0.004%
17	4.922	1111	1114	1115	rBV	272	175	0.02%	0.003%
18	4.983	1128	1133	1136	rBB	330	277	0.03%	0.004%
19	5.067	1141	1159	1180	rBV	172321	374997	43.87%	5.381%
20	5.205	1200	1202	1205	rBB	272	128	0.01%	0.002%
21	5.276	1222	1224	1226	rBV	273	164	0.02%	0.002%
22	5.411	1260	1266	1268	rBB	239	205	0.02%	0.003%
23	5.462	1279	1282	1284	rBB	333	195	0.02%	0.003%
24	5.729	1341	1365	1386	rBV3	303327	854875	100.00%	12.266%
25	5.886	1412	1414	1419	rVB2	454	271	0.03%	0.004%
26	6.047	1461	1464	1468	rBB	196	163	0.02%	0.002%
27	6.115	1480	1485	1487	rBV	208	208	0.02%	0.003%
28	6.157	1494	1498	1500	rBB	244	152	0.02%	0.002%
29	6.250	1513	1527	1557	rBV	270012	515758	60.33%	7.400%
30	6.462	1590	1593	1596	rVB	336	232	0.03%	0.003%
31	6.530	1604	1614	1625	rBB3	5188	9025	1.06%	0.129%
32	6.597	1631	1635	1638	rBB	258	188	0.02%	0.003%
33	6.693	1650	1665	1690	rBV	192480	379379	44.38%	5.444%
34	6.777	1690	1691	1695	rVV	380	156	0.02%	0.002%
35	6.812	1698	1702	1705	rVB3	524	408	0.05%	0.006%
36	6.877	1720	1722	1724	rBV	276	149	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
 Data File : VU048644.D
 Acq On : 20 May 2022 12:16
 Operator : SY/MD
 Sample : VU0520WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK135

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	7.105	1790	1793	1796	rBB	211	157	0.02%	0.002%
38	7.185	1810	1818	1825	rBV3	1659	2108	0.25%	0.030%
39	7.568	1923	1937	1963	rBV	119578	210883	24.67%	3.026%
40	7.693	1969	1976	1980	rBV3	815	1072	0.13%	0.015%
41	7.735	1987	1989	1992	rBV2	257	184	0.02%	0.003%
42	7.803	2007	2010	2012	rBV2	396	236	0.03%	0.003%
43	7.899	2027	2040	2057	rBV	402855	686107	80.26%	9.845%
44	8.115	2105	2107	2110	rVB	215	138	0.02%	0.002%
45	8.182	2114	2128	2143	rBV	89380	150925	17.65%	2.166%
46	8.365	2181	2185	2187	rBV2	454	310	0.04%	0.004%
47	8.468	2214	2217	2220	rVV2	306	151	0.02%	0.002%
48	8.488	2220	2223	2229	rVB2	438	346	0.04%	0.005%
49	8.558	2243	2245	2248	rBV	283	194	0.02%	0.003%
50	8.636	2257	2269	2294	rBV2	268432	502715	58.81%	7.213%
51	8.828	2326	2329	2332	rBB	373	252	0.03%	0.004%
52	8.912	2353	2355	2356	rBV	435	186	0.02%	0.003%
53	8.963	2369	2371	2374	rBB2	321	195	0.02%	0.003%
54	9.134	2422	2424	2428	rBV	292	202	0.02%	0.003%
55	9.176	2432	2437	2438	rBV	223	171	0.02%	0.002%
56	9.256	2458	2462	2463	rBV	203	161	0.02%	0.002%
57	9.295	2471	2474	2479	rBB	191	175	0.02%	0.003%
58	9.324	2480	2483	2485	rBV	171	133	0.02%	0.002%
59	9.417	2500	2512	2530	rBV	381007	646979	75.68%	9.283%
60	9.568	2555	2559	2562	rBV2	435	463	0.05%	0.007%
61	9.626	2574	2577	2580	rVB2	418	245	0.03%	0.004%
62	9.645	2580	2583	2584	rBV2	279	139	0.02%	0.002%
63	9.697	2589	2599	2603	rBV3	881	1194	0.14%	0.017%
64	9.732	2606	2610	2613	rBB	166	160	0.02%	0.002%
65	9.822	2635	2638	2643	rBB	240	246	0.03%	0.004%
66	9.867	2649	2652	2654	rBV	192	152	0.02%	0.002%
67	10.034	2701	2704	2706	rBV	228	172	0.02%	0.002%
68	10.111	2724	2728	2732	rBB	585	354	0.04%	0.005%
69	10.137	2733	2736	2739	rBV2	298	225	0.03%	0.003%
70	10.301	2784	2787	2791	rBV	196	198	0.02%	0.003%
71	10.381	2809	2812	2814	rBV	226	173	0.02%	0.002%
72	10.568	2865	2870	2873	rBV	227	239	0.03%	0.003%
73	10.619	2883	2886	2889	rVV	300	285	0.03%	0.004%
74	10.642	2891	2893	2898	rVV2	353	279	0.03%	0.004%
75	10.668	2898	2901	2907	rVV3	713	640	0.07%	0.009%
76	10.713	2910	2915	2917	rBV	370	295	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
 Data File : VU048644.D
 Acq On : 20 May 2022 12:16
 Operator : SY/MD
 Sample : VU0520WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK135

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M

Title : VOC Analysis

77	10.758	2917	2929	2948	rVB	310134	496576	58.09%	7.125%
78	10.896	2969	2972	2975	rVB2	320	265	0.03%	0.004%
79	10.922	2976	2980	2983	rBV	249	198	0.02%	0.003%
80	10.970	2991	2995	2998	rBV	190	147	0.02%	0.002%
81	11.053	3016	3021	3026	rBB	282	366	0.04%	0.005%
82	11.089	3029	3032	3035	rBB	319	195	0.02%	0.003%
83	11.111	3035	3039	3042	rBV2	356	326	0.04%	0.005%
84	11.160	3052	3054	3057	rBV	217	138	0.02%	0.002%
85	11.224	3070	3074	3078	rBV	274	346	0.04%	0.005%
86	11.693	3217	3220	3223	rBV2	253	255	0.03%	0.004%
87	11.751	3235	3238	3245	rBV2	557	580	0.07%	0.008%
88	11.812	3245	3257	3272	rBV	446964	714794	83.61%	10.256%
89	11.951	3297	3300	3303	rBV	252	161	0.02%	0.002%
90	12.195	3361	3376	3397	rBV	464840	750926	87.84%	10.775%
91	12.536	3479	3482	3485	rBV	244	165	0.02%	0.002%
92	12.603	3500	3503	3506	rVB	256	131	0.02%	0.002%
93	13.034	3633	3637	3638	rBV2	268	176	0.02%	0.003%
94	13.404	3749	3752	3754	rBV	244	134	0.02%	0.002%
95	13.532	3789	3792	3797	rBV2	313	286	0.03%	0.004%
96	13.626	3818	3821	3822	rBV	211	131	0.02%	0.002%
97	13.893	3900	3904	3907	rVB2	469	247	0.03%	0.004%
98	13.986	3930	3933	3939	rVB2	441	318	0.04%	0.005%
99	14.198	3996	3999	4000	rBV	327	171	0.02%	0.002%
100	15.121	4284	4286	4288	rBV	501	246	0.03%	0.004%


Sum of corrected areas: 6969287

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
Data File : VU048644.D
Acq On : 20 May 2022 12:16
Operator : SY/MD
Sample : VU0520WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK135

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

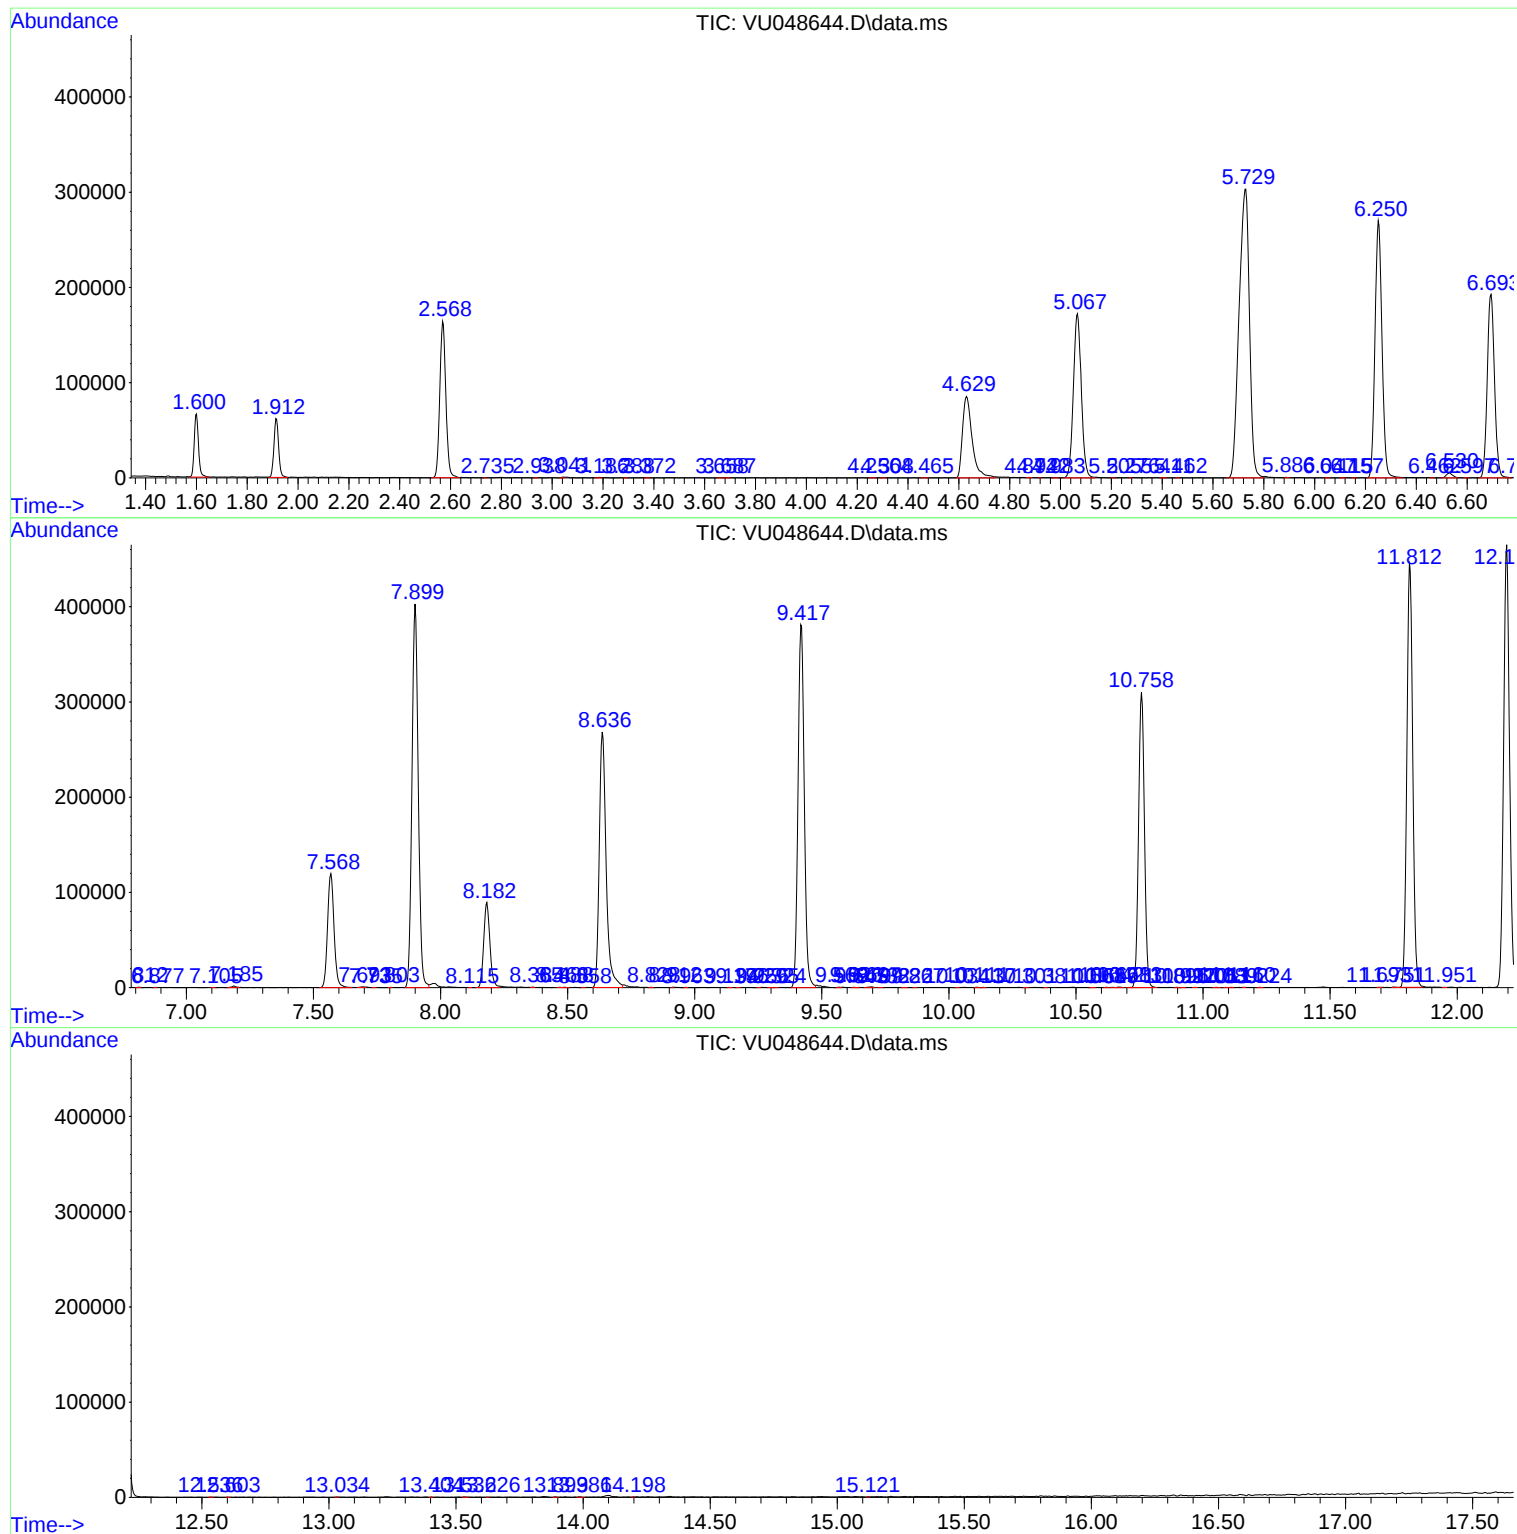

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
Data File : VU048644.D
Acq On : 20 May 2022 12:16
Operator : SY/MD
Sample : VU0520WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK135

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
Data File : VU048644.D
Acq On : 20 May 2022 12:16
Operator : SY/MD
Sample : VU0520WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK135

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------