

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
 Data File : VU048646.D
 Acq On : 20 May 2022 14:38
 Operator : SY/MD
 Sample : N2926-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXY30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048646.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	71	81	95	rVB	63110	76944	9.84%	1.154%
2	1.912	170	178	190	rBV	56839	68866	8.80%	1.033%
3	2.289	286	295	302	rBV3	1082	1397	0.18%	0.021%
4	2.568	369	382	395	rBV	151777	247463	31.63%	3.711%
5	2.716	425	428	430	rBV2	393	286	0.04%	0.004%
6	2.774	442	446	449	rVV	264	275	0.04%	0.004%
7	2.887	477	481	483	rBB	260	191	0.02%	0.003%
8	3.038	525	528	530	rBV	235	179	0.02%	0.003%
9	3.057	532	534	538	rVB2	549	386	0.05%	0.006%
10	3.182	558	573	588	rBV3	7723	16896	2.16%	0.253%
11	3.658	718	721	725	rBB	227	191	0.02%	0.003%
12	4.440	950	964	979	rBV4	5754	13384	1.71%	0.201%
13	4.494	979	981	983	rBV	311	151	0.02%	0.002%
14	4.536	992	994	996	rVB	347	163	0.02%	0.002%
15	4.549	996	998	1003	rBB2	361	217	0.03%	0.003%
16	4.623	1008	1021	1048	rBV2	75909	190799	24.39%	2.861%
17	5.067	1140	1159	1183	rBV	159687	349179	44.63%	5.236%
18	5.253	1214	1217	1220	rBB	258	162	0.02%	0.002%
19	5.729	1343	1365	1389	rBV2	284010	782333	100.00%	11.732%
20	5.941	1429	1431	1435	rVB	275	204	0.03%	0.003%
21	6.034	1457	1460	1461	rBV2	271	146	0.02%	0.002%
22	6.044	1461	1463	1466	rVV2	316	228	0.03%	0.003%
23	6.250	1513	1527	1544	rBV	278704	526490	67.30%	7.895%
24	6.398	1569	1573	1579	rVB4	1021	1131	0.14%	0.017%
25	6.452	1588	1590	1593	rVB	312	153	0.02%	0.002%
26	6.533	1605	1615	1627	rVB5	5344	9997	1.28%	0.150%
27	6.693	1651	1665	1681	rBV	179313	347594	44.43%	5.212%
28	6.809	1699	1701	1704	rBV	291	134	0.02%	0.002%
29	6.874	1719	1721	1723	rBV	201	138	0.02%	0.002%
30	6.941	1740	1742	1746	rBB2	245	156	0.02%	0.002%
31	7.047	1772	1775	1780	rBB	251	185	0.02%	0.003%
32	7.131	1791	1801	1806	rBV5	2529	3617	0.46%	0.054%
33	7.263	1836	1842	1844	rBB	287	228	0.03%	0.003%
34	7.568	1925	1937	1960	rBV	106753	193362	24.72%	2.900%
35	7.661	1965	1966	1970	rVB	343	163	0.02%	0.002%
36	7.687	1970	1974	1975	rBV2	659	531	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
 Data File : VU048646.D
 Acq On : 20 May 2022 14:38
 Operator : SY/MD
 Sample : N2926-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXY30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	7.761	1994	1997	2001	rVB2	315	278	0.04%	0.004%
38	7.790	2004	2006	2008	rBV	238	148	0.02%	0.002%
39	7.838	2018	2021	2025	rBB	205	179	0.02%	0.003%
40	7.899	2025	2040	2056	rBV	368931	631409	80.71%	9.469%
41	8.182	2117	2128	2142	rBV2	81291	138497	17.70%	2.077%
42	8.475	2210	2219	2230	rVB3	5052	8414	1.08%	0.126%
43	8.562	2244	2246	2249	rBV2	451	273	0.03%	0.004%
44	8.636	2256	2269	2295	rBV2	235666	431277	55.13%	6.467%
45	8.848	2332	2335	2339	rBB	170	126	0.02%	0.002%
46	8.925	2355	2359	2363	rBV	222	232	0.03%	0.003%
47	8.960	2367	2370	2373	rBB2	272	167	0.02%	0.003%
48	8.980	2373	2376	2379	rBB	191	144	0.02%	0.002%
49	9.102	2409	2414	2416	rBV2	356	280	0.04%	0.004%
50	9.140	2424	2426	2430	rVB2	346	182	0.02%	0.003%
51	9.166	2431	2434	2435	rBV	355	175	0.02%	0.003%
52	9.243	2455	2458	2460	rBV	209	175	0.02%	0.003%
53	9.291	2470	2473	2476	rBV	190	147	0.02%	0.002%
54	9.356	2489	2493	2495	rBV	178	168	0.02%	0.003%
55	9.420	2500	2513	2536	rBV	397428	669482	85.58%	10.039%
56	9.574	2554	2561	2564	rBV2	340	412	0.05%	0.006%
57	9.616	2572	2574	2577	rBV	159	130	0.02%	0.002%
58	9.684	2592	2595	2596	rBV	238	151	0.02%	0.002%
59	9.709	2596	2603	2606	rVB3	668	955	0.12%	0.014%
60	9.729	2607	2609	2612	rBV	203	152	0.02%	0.002%
61	9.790	2625	2628	2630	rBB	278	131	0.02%	0.002%
62	9.854	2646	2648	2652	rBB	182	138	0.02%	0.002%
63	9.925	2667	2670	2675	rBV	268	284	0.04%	0.004%
64	9.947	2675	2677	2679	rVB	291	153	0.02%	0.002%
65	9.986	2683	2689	2692	rBV	246	238	0.03%	0.004%
66	10.076	2712	2717	2722	rBB	173	245	0.03%	0.004%
67	10.102	2722	2725	2728	rBV2	339	310	0.04%	0.005%
68	10.121	2728	2731	2736	rVB2	366	333	0.04%	0.005%
69	10.343	2794	2800	2809	rBV6	1441	2237	0.29%	0.034%
70	10.462	2833	2837	2841	rBV	269	306	0.04%	0.005%
71	10.635	2889	2891	2894	rVB	277	151	0.02%	0.002%
72	10.674	2897	2903	2905	rBV2	634	582	0.07%	0.009%
73	10.758	2914	2929	2944	rBV	282373	458516	58.61%	6.876%
74	10.896	2962	2972	2985	rBV2	8668	14044	1.80%	0.211%
75	11.053	3016	3021	3024	rBV	183	230	0.03%	0.003%
76	11.086	3027	3031	3033	rBV	204	141	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
 Data File : VU048646.D
 Acq On : 20 May 2022 14:38
 Operator : SY/MD
 Sample : N2926-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXY30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	11.208	3065	3069	3071	rBV2	320	240	0.03%	0.004%
78	11.240	3077	3079	3082	rVB2	248	141	0.02%	0.002%
79	11.259	3082	3085	3089	rBV2	238	189	0.02%	0.003%
80	11.324	3098	3105	3109	rBV	221	357	0.05%	0.005%
81	11.397	3125	3128	3131	rBV	205	198	0.03%	0.003%
82	11.417	3131	3134	3139	rVV	212	131	0.02%	0.002%
83	11.462	3146	3148	3149	rBV	412	128	0.02%	0.002%
84	11.690	3216	3219	3221	rVB3	457	257	0.03%	0.004%
85	11.748	3233	3237	3245	rVB3	344	471	0.06%	0.007%
86	11.812	3245	3257	3280	rVV	466963	752364	96.17%	11.282%
87	11.967	3302	3305	3307	rBV2	333	222	0.03%	0.003%
88	12.069	3332	3337	3338	rBV	1150	854	0.11%	0.013%
89	12.195	3363	3376	3396	rVV	448064	712311	91.05%	10.682%
90	12.410	3440	3443	3445	rBV	335	222	0.03%	0.003%
91	12.449	3453	3455	3458	rVB	350	150	0.02%	0.002%
92	12.465	3458	3460	3464	rVB	289	186	0.02%	0.003%
93	12.487	3464	3467	3469	rBV	390	219	0.03%	0.003%
94	12.774	3550	3556	3564	rVB3	1144	1739	0.22%	0.026%
95	12.970	3615	3617	3621	rBV	212	140	0.02%	0.002%
96	13.105	3656	3659	3662	rBV	258	162	0.02%	0.002%
97	13.221	3693	3695	3698	rBV2	301	187	0.02%	0.003%
98	13.719	3848	3850	3853	rVB	278	135	0.02%	0.002%
99	13.796	3872	3874	3876	rBV	348	149	0.02%	0.002%
100	14.095	3959	3967	3972	rBV2	1355	1837	0.23%	0.028%




Sum of corrected areas: 6668500

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
Data File : VU048646.D
Acq On : 20 May 2022 14:38
Operator : SY/MD
Sample : N2926-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXY30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

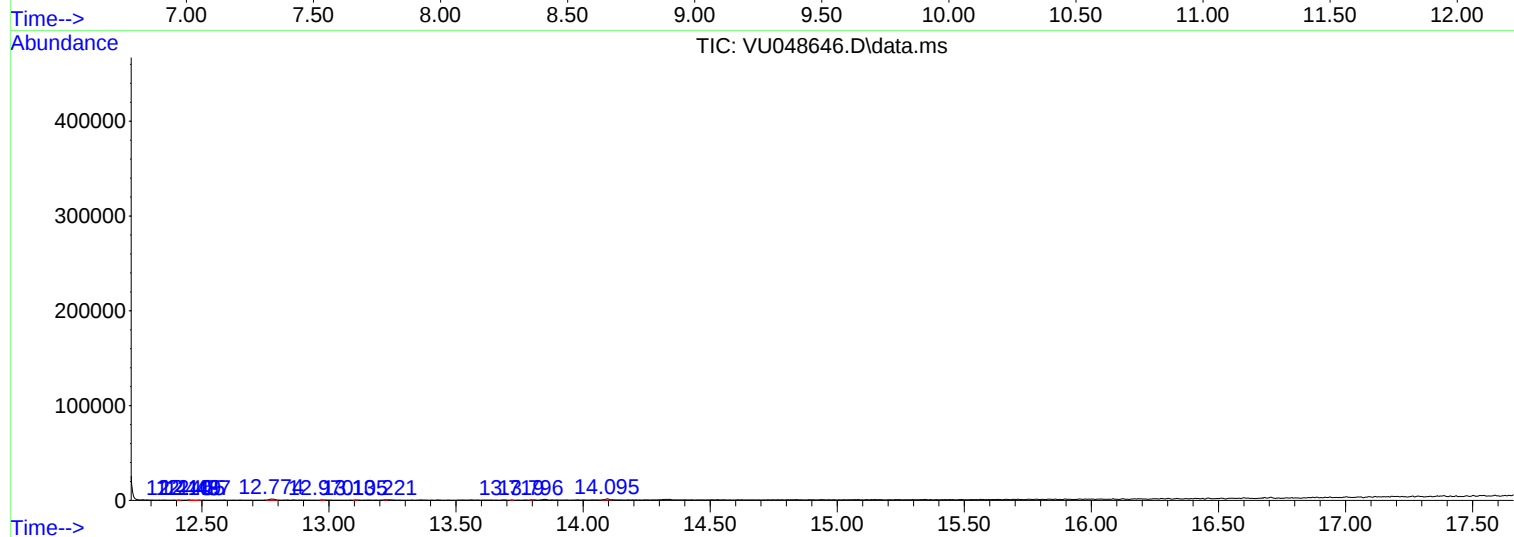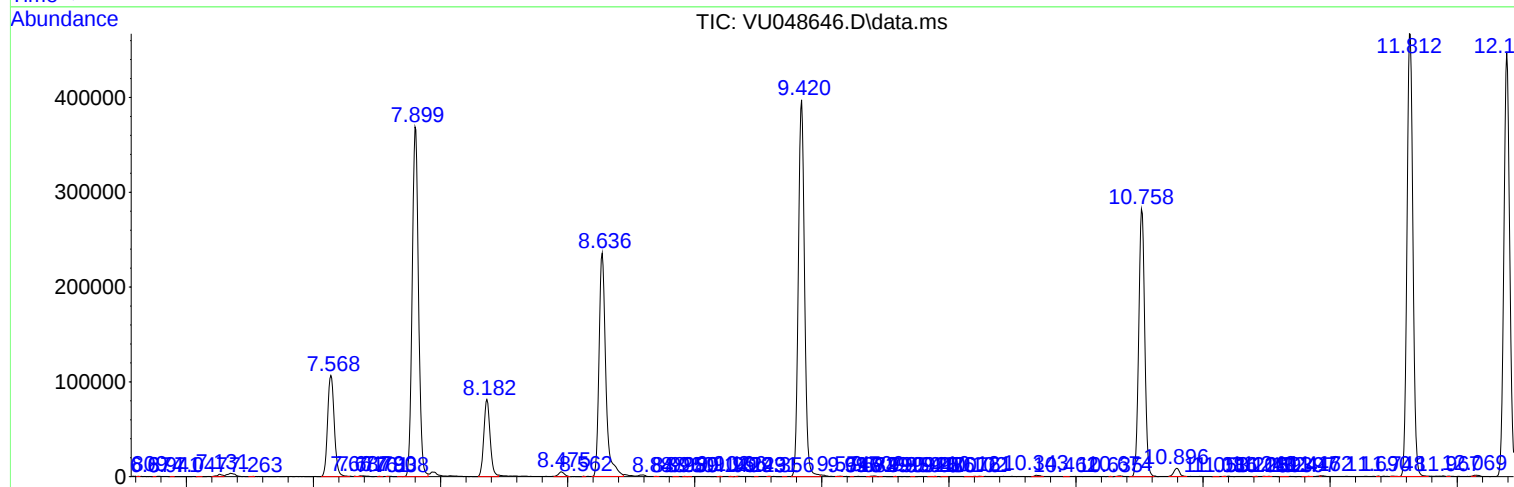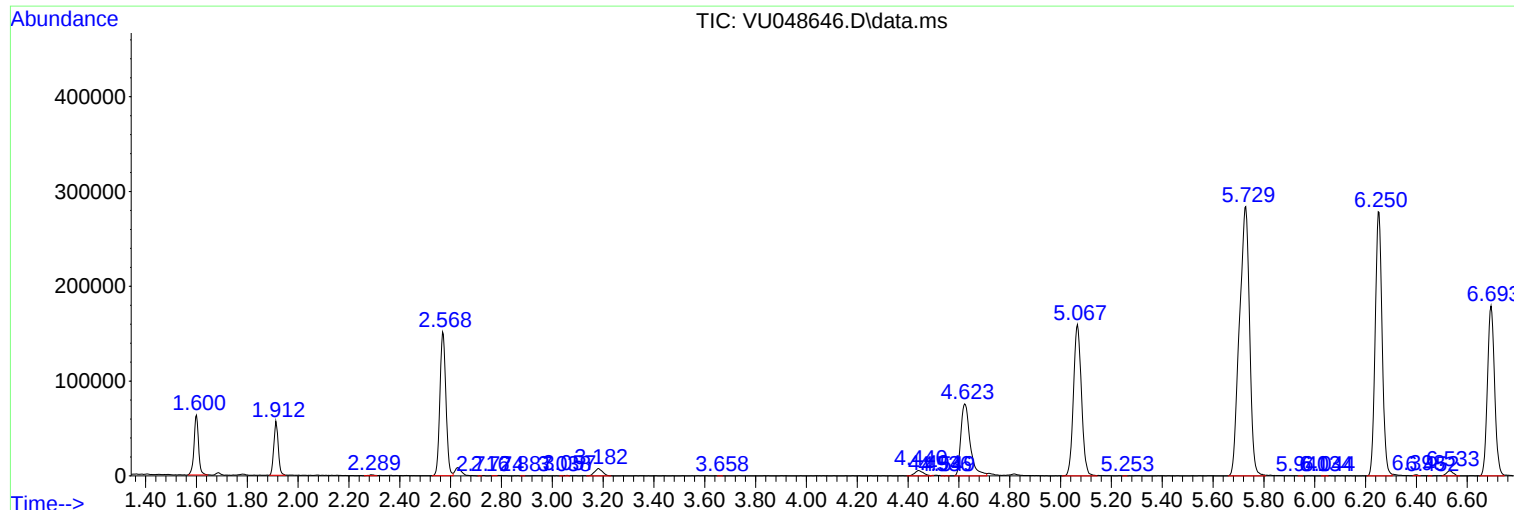

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
Data File : VU048646.D
Acq On : 20 May 2022 14:38
Operator : SY/MD
Sample : N2926-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXY30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
Data File : VU048646.D
Acq On : 20 May 2022 14:38
Operator : SY/MD
Sample : N2926-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXY30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------