

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
 Data File : VU048647.D
 Acq On : 20 May 2022 16:47
 Operator : SY/MD
 Sample : N2926-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048647.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	100	rBV	60588	69065	8.61%	1.046%
2	1.912	170	178	193	rVB	53981	69518	8.66%	1.053%
3	2.568	367	382	397	rBV	150986	244621	30.48%	3.706%
4	2.691	417	420	422	rBV	150	129	0.02%	0.002%
5	2.771	441	445	447	rVV2	308	240	0.03%	0.004%
6	2.893	478	483	487	rBB	267	280	0.03%	0.004%
7	2.925	490	493	496	rBV	213	185	0.02%	0.003%
8	3.051	523	532	541	rVV4	1028	1621	0.20%	0.025%
9	3.150	560	563	564	rBV	284	176	0.02%	0.003%
10	3.192	567	576	585	rVB2	2872	5928	0.74%	0.090%
11	3.253	593	595	599	rBB	242	147	0.02%	0.002%
12	3.356	623	627	631	rBB	188	205	0.03%	0.003%
13	3.398	638	640	643	rBB2	259	144	0.02%	0.002%
14	3.986	820	823	827	rBB	172	162	0.02%	0.002%
15	4.186	882	885	889	rBB	194	189	0.02%	0.003%
16	4.562	1000	1002	1004	rBB	265	141	0.02%	0.002%
17	4.578	1004	1007	1009	rBV	182	131	0.02%	0.002%
18	4.623	1009	1021	1051	rBV	91518	232117	28.92%	3.517%
19	4.903	1105	1108	1110	rBV2	388	253	0.03%	0.004%
20	4.928	1114	1116	1122	rVB2	356	200	0.02%	0.003%
21	4.999	1134	1138	1139	rBV	297	141	0.02%	0.002%
22	5.067	1143	1159	1180	rVB	164461	357610	44.56%	5.418%
23	5.289	1224	1228	1230	rBV2	369	226	0.03%	0.003%
24	5.301	1230	1232	1236	rVB	272	173	0.02%	0.003%
25	5.321	1236	1238	1241	rBV	164	138	0.02%	0.002%
26	5.475	1284	1286	1288	rBV	187	124	0.02%	0.002%
27	5.726	1343	1364	1383	rBV3	285759	802566	100.00%	12.160%
28	5.877	1408	1411	1416	rVB2	499	438	0.05%	0.007%
29	5.916	1421	1423	1428	rVB	370	276	0.03%	0.004%
30	6.041	1459	1462	1465	rBB	213	162	0.02%	0.002%
31	6.057	1465	1467	1469	rBV	244	138	0.02%	0.002%
32	6.250	1513	1527	1548	rBV	252024	475887	59.30%	7.210%
33	6.385	1566	1569	1575	rVB2	324	285	0.04%	0.004%
34	6.446	1586	1588	1589	rBV	255	142	0.02%	0.002%
35	6.533	1603	1615	1628	rBB4	4442	8287	1.03%	0.126%
36	6.620	1640	1642	1645	rBV	281	205	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
 Data File : VU048647.D
 Acq On : 20 May 2022 16:47
 Operator : SY/MD
 Sample : N2926-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	6.694	1651	1665	1690	rBV	184534	356253	44.39%	5.398%
38	6.809	1696	1701	1703	rBV	327	277	0.03%	0.004%
39	7.186	1811	1818	1819	rBV3	1434	1442	0.18%	0.022%
40	7.272	1842	1845	1847	rBV	185	154	0.02%	0.002%
41	7.330	1861	1863	1867	rBB	155	132	0.02%	0.002%
42	7.462	1901	1904	1907	rBB	203	146	0.02%	0.002%
43	7.568	1922	1937	1956	rBV	111922	195187	24.32%	2.957%
44	7.899	2024	2040	2056	rBV	368255	638361	79.54%	9.672%
45	8.131	2108	2112	2115	rBB	160	130	0.02%	0.002%
46	8.182	2116	2128	2144	rBV	84093	142224	17.72%	2.155%
47	8.407	2193	2198	2204	rVB2	286	362	0.05%	0.005%
48	8.456	2209	2213	2214	rVV2	309	248	0.03%	0.004%
49	8.472	2216	2218	2220	rBV	247	122	0.02%	0.002%
50	8.491	2221	2224	2228	rVV2	241	190	0.02%	0.003%
51	8.510	2228	2230	2235	rVB2	428	316	0.04%	0.005%
52	8.542	2236	2240	2244	rBV	215	226	0.03%	0.003%
53	8.636	2256	2269	2301	rVV	272602	500773	62.40%	7.587%
54	8.948	2363	2366	2368	rBV2	332	264	0.03%	0.004%
55	9.025	2387	2390	2394	rBB	206	173	0.02%	0.003%
56	9.057	2394	2400	2401	rBV	273	241	0.03%	0.004%
57	9.118	2410	2419	2423	rBV	246	393	0.05%	0.006%
58	9.189	2436	2441	2443	rBB	139	122	0.02%	0.002%
59	9.205	2443	2446	2448	rBV	234	169	0.02%	0.003%
60	9.330	2482	2485	2490	rBB2	331	293	0.04%	0.004%
61	9.366	2494	2496	2499	rBV	158	137	0.02%	0.002%
62	9.417	2499	2512	2534	rBV	359637	602102	75.02%	9.122%
63	9.668	2587	2590	2594	rVB	233	128	0.02%	0.002%
64	9.693	2594	2598	2601	rBV	306	338	0.04%	0.005%
65	9.755	2615	2617	2619	rBV	299	167	0.02%	0.003%
66	9.796	2627	2630	2633	rBV	389	264	0.03%	0.004%
67	9.899	2659	2662	2664	rBV	200	162	0.02%	0.002%
68	9.954	2676	2679	2681	rBV	222	172	0.02%	0.003%
69	10.009	2693	2696	2699	rBV	192	187	0.02%	0.003%
70	10.147	2733	2739	2742	rBV	184	261	0.03%	0.004%
71	10.343	2797	2800	2803	rBB	217	161	0.02%	0.002%
72	10.365	2804	2807	2809	rBV	261	149	0.02%	0.002%
73	10.468	2836	2839	2842	rBV	175	164	0.02%	0.002%
74	10.488	2842	2845	2849	rVB	265	200	0.02%	0.003%
75	10.546	2857	2863	2867	rBV	235	348	0.04%	0.005%
76	10.616	2881	2885	2888	rBV	166	147	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
 Data File : VU048647.D
 Acq On : 20 May 2022 16:47
 Operator : SY/MD
 Sample : N2926-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	10.674	2900	2903	2907	rVB	763	412	0.05%	0.006%
78	10.758	2916	2929	2949	rBV	303990	488418	60.86%	7.400%
79	10.880	2965	2967	2970	rVB2	288	165	0.02%	0.002%
80	10.919	2976	2979	2983	rBB	165	157	0.02%	0.002%
81	10.951	2984	2989	2990	rBV	293	226	0.03%	0.003%
82	11.150	3047	3051	3054	rVB	297	217	0.03%	0.003%
83	11.198	3062	3066	3068	rBV	237	192	0.02%	0.003%
84	11.491	3155	3157	3161	rVB	291	132	0.02%	0.002%
85	11.812	3244	3257	3279	rBV	418738	669065	83.37%	10.137%
86	12.195	3362	3376	3393	rBV	444906	722071	89.97%	10.940%
87	12.873	3581	3587	3588	rBV	230	203	0.03%	0.003%
88	12.944	3606	3609	3615	rVB2	327	289	0.04%	0.004%
89	13.028	3630	3635	3640	rBV2	358	360	0.04%	0.005%
90	13.147	3669	3672	3680	rVB	328	323	0.04%	0.005%
91	13.230	3696	3698	3704	rVB	514	411	0.05%	0.006%
92	13.262	3704	3708	3709	rBV	272	191	0.02%	0.003%
93	13.481	3774	3776	3777	rBV	320	128	0.02%	0.002%
94	13.536	3791	3793	3798	rVB	241	127	0.02%	0.002%
95	13.574	3802	3805	3811	rBV	216	204	0.03%	0.003%
96	13.960	3921	3925	3927	rBV2	382	257	0.03%	0.004%
97	14.256	4015	4017	4018	rBV	293	122	0.02%	0.002%
98	14.356	4046	4048	4051	rBV	340	222	0.03%	0.003%
99	14.407	4059	4064	4068	rBV2	364	394	0.05%	0.006%
100	14.951	4228	4233	4236	rBV	368	404	0.05%	0.006%




Sum of corrected areas: 6600225

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
Data File : VU048647.D
Acq On : 20 May 2022 16:47
Operator : SY/MD
Sample : N2926-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

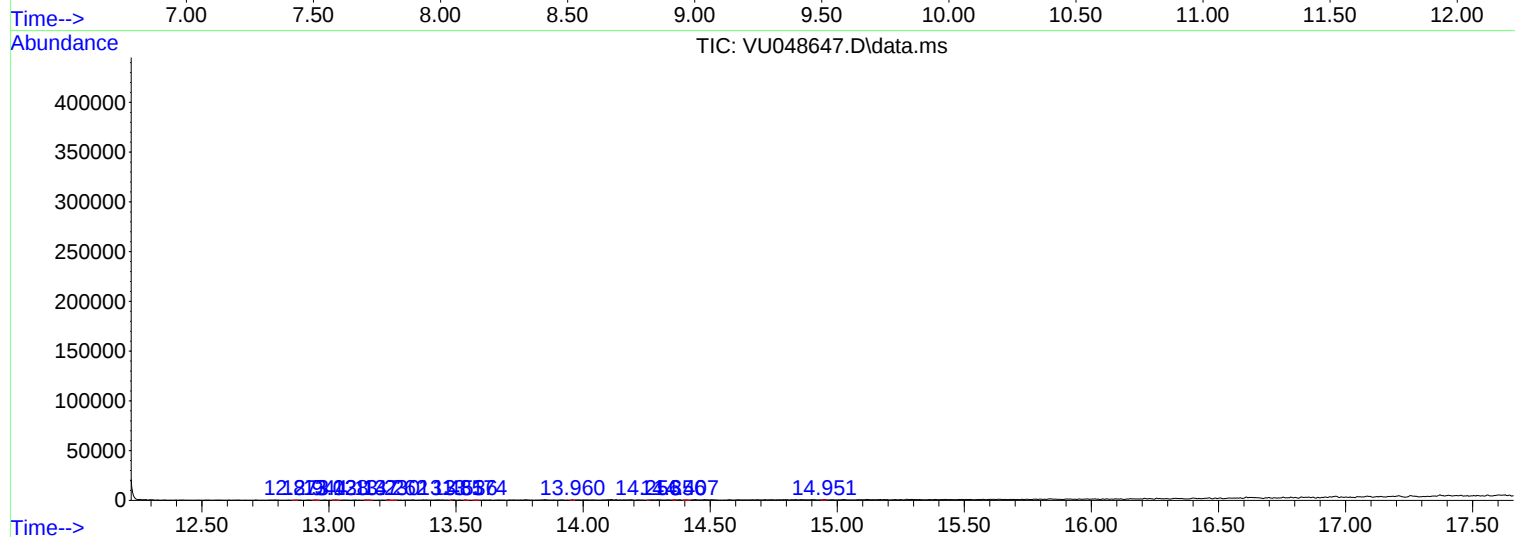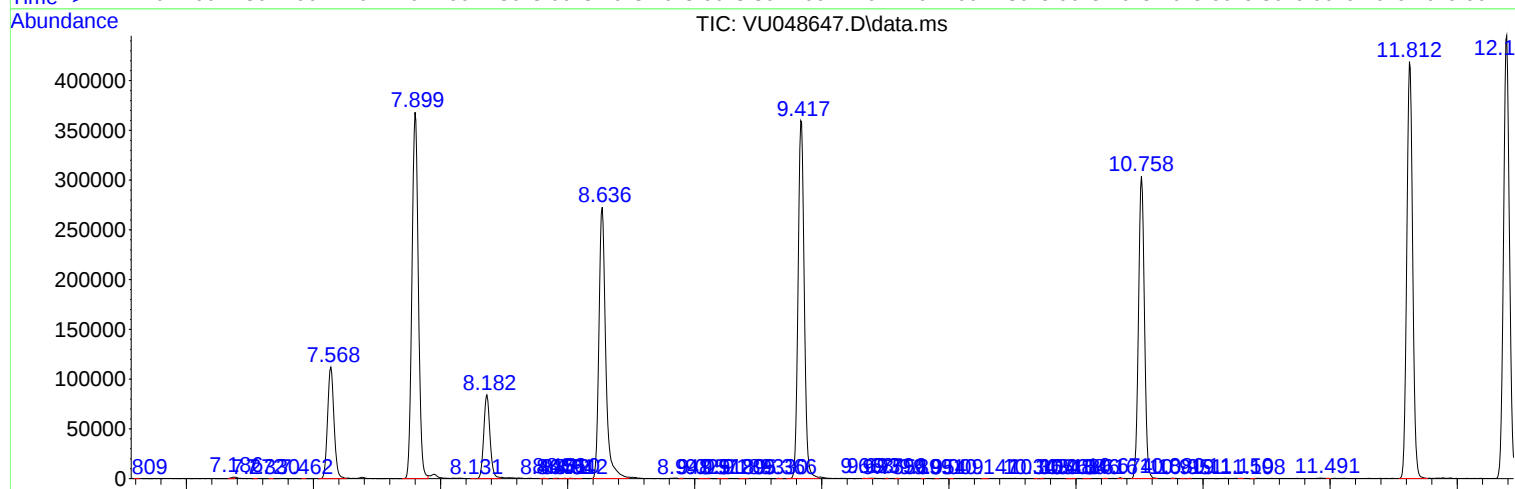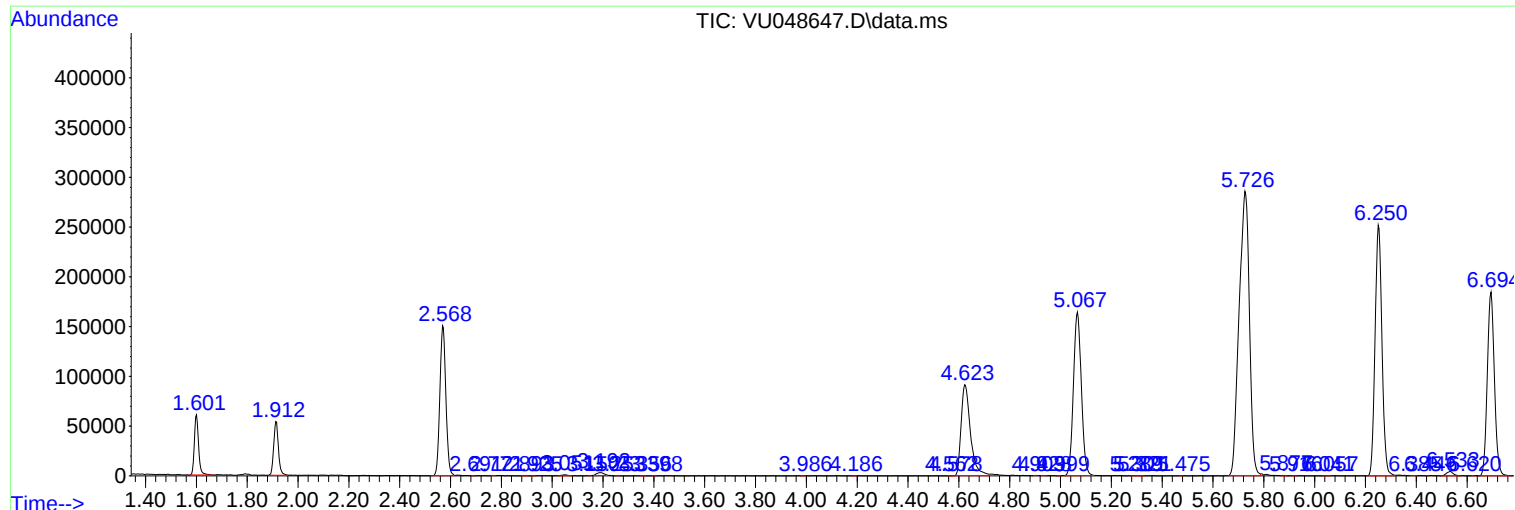

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
Data File : VU048647.D
Acq On : 20 May 2022 16:47
Operator : SY/MD
Sample : N2926-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
Data File : VU048647.D
Acq On : 20 May 2022 16:47
Operator : SY/MD
Sample : N2926-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------