


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052022\
 Data File : VU048641.D
 Acq On : 20 May 2022 09:56
 Operator : SY/MD
 Sample : BFB091
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB091

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis
 Last Update : Tue May 24 02:53:22 2022

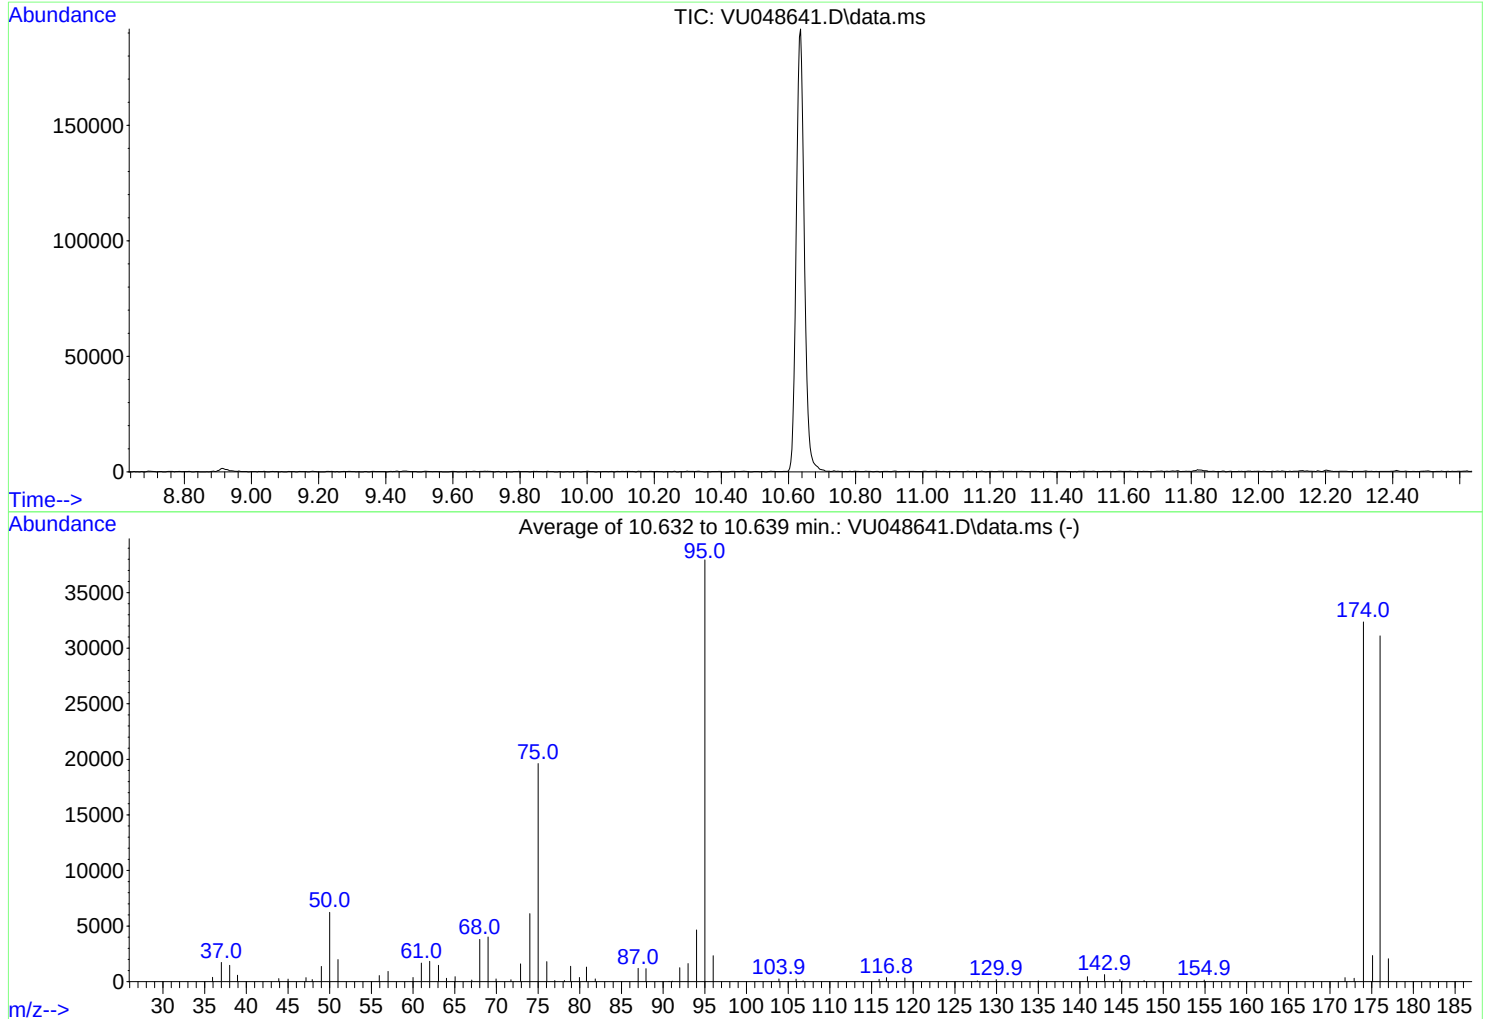

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	6241	PASS
75	95	30	80	51.7	19616	PASS
95	95	100	100	100.0	37947	PASS
96	95	5	9	6.2	2335	PASS
173	174	0.00	2	0.9	296	PASS
174	95	50	120	85.3	32363	PASS
175	174	5	9	7.2	2344	PASS
176	174	95	101	96.1	31104	PASS
177	176	5	9	6.6	2067	PASS

m/z	Abundance
43.90	181.0

Instrument :
MSVOA_U
ClientSampleId :
BFB091

m/z	Abundance
35.90	389.0
37.00	1850.0
38.00	1478.0
38.90	616.0
43.90	435.0
45.00	242.0
47.10	388.0
47.90	191.0
49.00	1449.0
50.00	6087.0
51.00	2163.0
55.90	553.0
57.00	925.0
60.00	374.0
61.00	1649.0
62.00	1818.0
63.00	1453.0
64.00	348.0
65.10	414.0
67.00	147.0
68.00	4026.0
69.00	4154.0
70.00	234.0
71.80	177.0
72.90	1543.0
74.00	6339.0
75.00	20216.0
76.10	1932.0
78.10	164.0
78.90	1479.0
80.00	438.0
80.80	1339.0
81.90	295.0
87.00	1108.0
87.90	1215.0
92.00	1283.0
93.00	1797.0
94.00	4649.0
95.00	38776.0
96.00	2463.0
103.90	238.0
106.00	254.0
106.80	107.0
115.90	223.0
116.80	395.0
119.00	352.0
130.00	159.0
135.00	117.0
140.90	418.0
142.90	615.0
144.80	229.0
155.00	167.0
171.80	366.0
172.90	426.0
174.00	32176.0
175.10	2304.0
176.00	31032.0
177.00	1992.0

Instrument :
MSVOA_U
ClientSampleId :
BFB091

m/z	Abundance
35.90	414.0
37.00	1779.0
38.00	1530.0
39.00	573.0
44.00	465.0
45.00	230.0
47.20	401.0
47.90	176.0
49.00	1393.0
50.00	6445.0
51.00	2086.0
55.90	589.0
57.00	948.0
60.00	368.0
61.00	1702.0
62.00	1919.0
63.00	1527.0
64.00	332.0
65.00	470.0
67.10	138.0
68.00	3895.0
69.00	4217.0
69.90	236.0
71.80	176.0
72.90	1692.0
74.00	6291.0
75.00	20160.0
76.10	1826.0
77.00	128.0
78.20	156.0
78.90	1453.0
80.00	385.0
80.80	1357.0
81.80	240.0
87.00	1284.0
87.90	1188.0
92.00	1302.0
93.00	1659.0
94.00	4801.0
95.00	39280.0
96.00	2395.0
103.90	281.0
106.00	225.0
106.80	113.0
115.90	240.0
116.80	349.0
119.00	353.0
127.70	112.0
129.90	199.0
135.00	100.0
140.90	472.0
142.90	652.0
144.80	193.0
147.70	156.0
154.90	147.0
171.80	382.0
172.90	463.0
174.00	33160.0
175.10	2373.0
176.00	31944.0
177.00	2132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB091

m/z	Abundance
36.00	369.0
37.00	1553.0
38.00	1411.0
39.00	553.0
44.00	461.0
45.00	235.0
47.20	296.0
47.90	199.0
49.00	1284.0
50.00	6191.0
51.00	1734.0
56.00	484.0
57.00	876.0
60.00	368.0
61.00	1673.0
62.00	1745.0
63.10	1415.0
64.00	233.0
65.00	441.0
67.10	130.0
68.00	3495.0
69.00	3663.0
69.90	276.0
71.70	151.0
72.90	1560.0
74.00	5718.0
75.00	18472.0
76.00	1654.0
77.00	179.0
78.90	1217.0
79.90	295.0
80.80	1224.0
81.90	181.0
87.00	1172.0
88.00	1096.0
90.70	107.0
91.10	149.0
92.00	1175.0
93.00	1407.0
94.00	4501.0
95.00	35784.0
96.00	2148.0
103.90	232.0
105.90	206.0
115.90	172.0
116.80	333.0
119.00	313.0
127.70	114.0
129.90	207.0
140.90	466.0
143.00	648.0
144.70	139.0
145.10	131.0
147.70	164.0
154.80	103.0
171.80	319.0
174.00	31752.0
175.10	2354.0
176.00	30336.0
177.00	2078.0

Instrument :
MSVOA_U
ClientSampleId :
BFB091