

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052024\
 Data File : VU058917.D
 Acq On : 20 May 2024 14:17
 Operator : MD/SY
 Sample : VU0520WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: May 21 03:29:13 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052024.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue May 21 03:23:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	4653	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	7369	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	2869	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	1515	0.434	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	86.000%		
4) 1,2-Dichloroethane-d4	5.709	65	2455	0.499	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	100.000%		
7) 1,2-Dichloropropane-d6	6.687	67	1976	0.564	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	112.000%		
8) Toluene-d8	7.887	98	5061	0.511	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	102.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1836	0.546	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	110.000%		
Target Compounds						
12) 1,2,3-Trichloropropane	10.865	75	50	0.020	ug/L	Qvalue # 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052024\
Data File : VU058917.D
Acq On : 20 May 2024 14:17
Operator : MD/SY
Sample : VU0520WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: May 21 03:29:13 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052024.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue May 21 03:23:43 2024
Response via : Initial Calibration

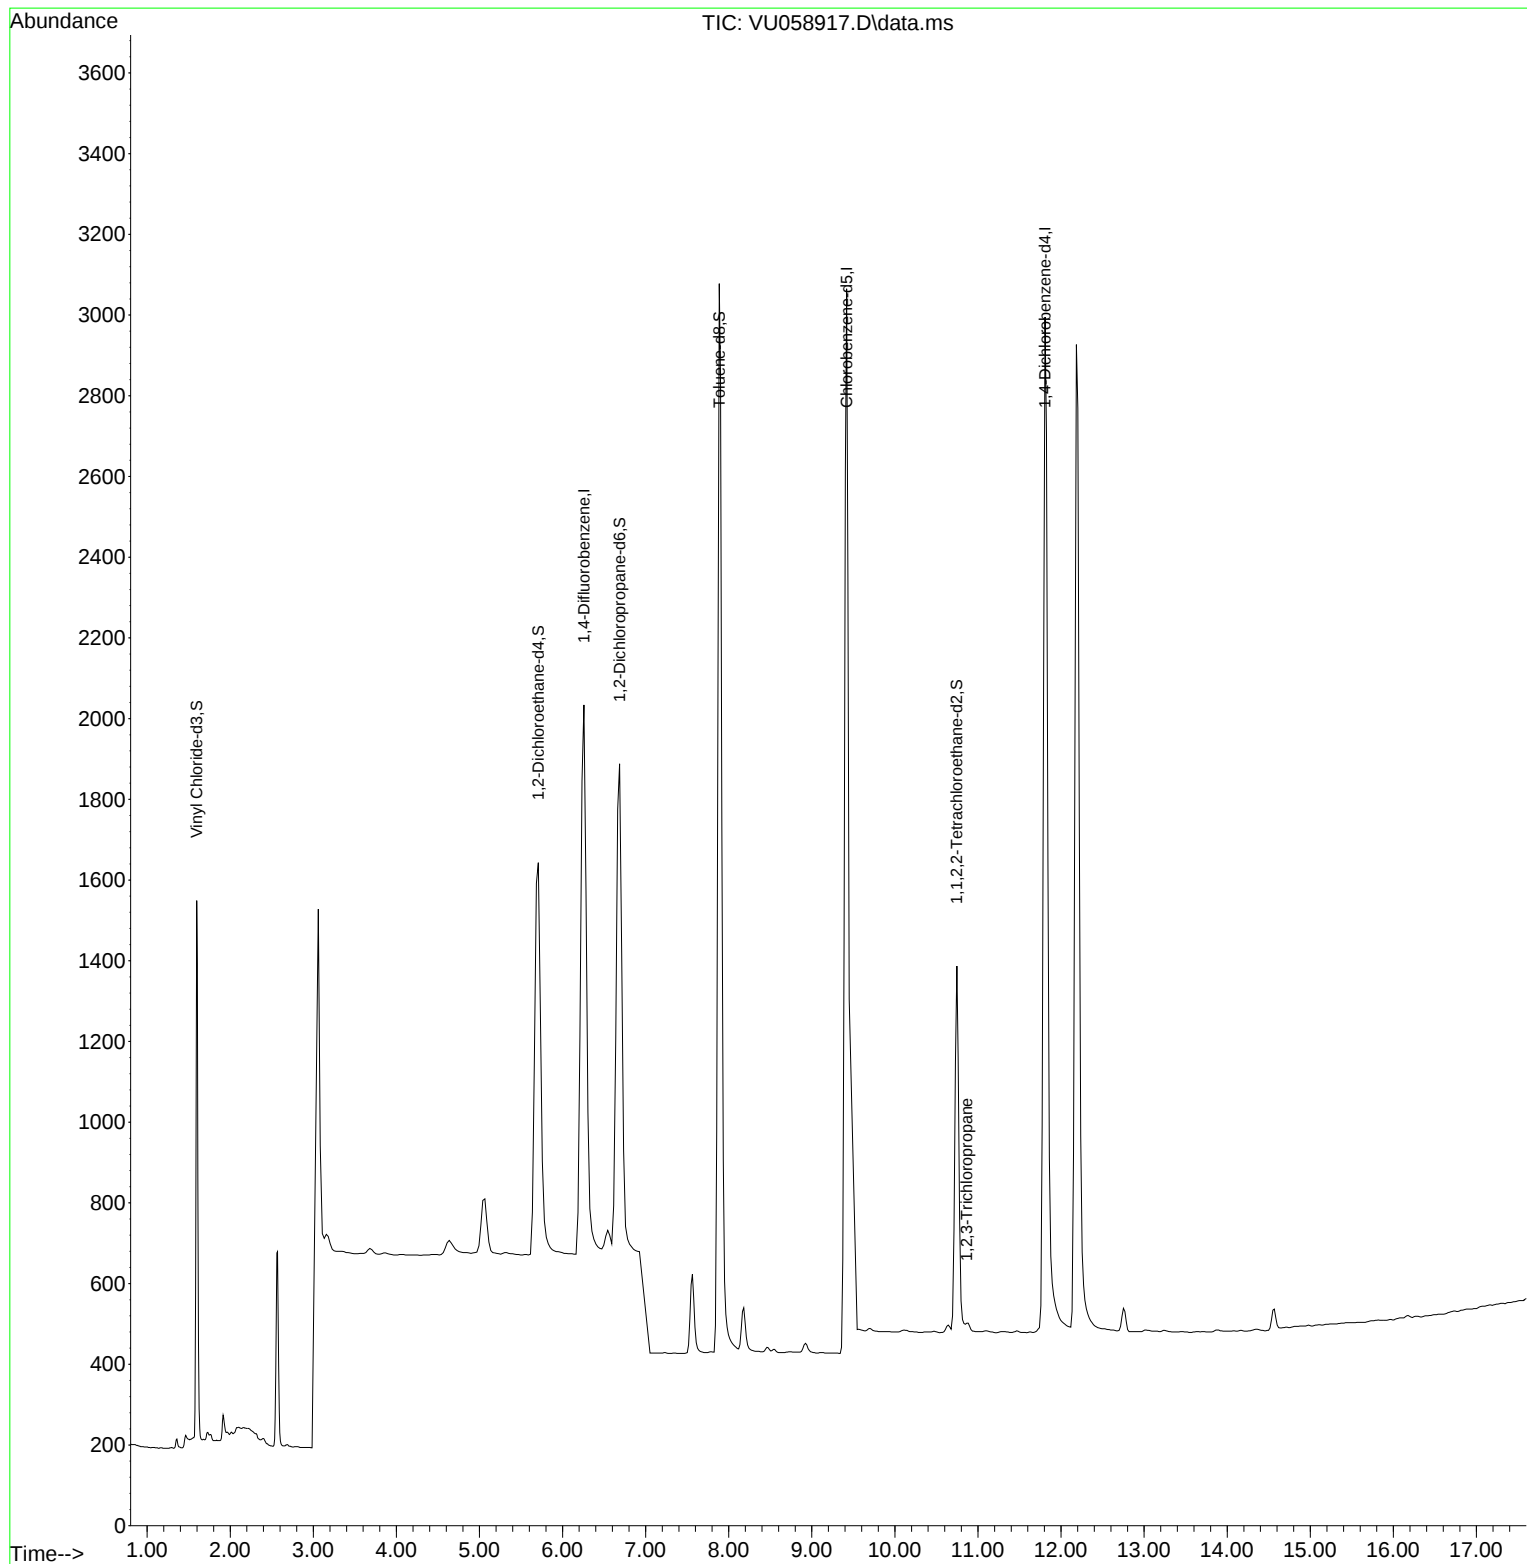

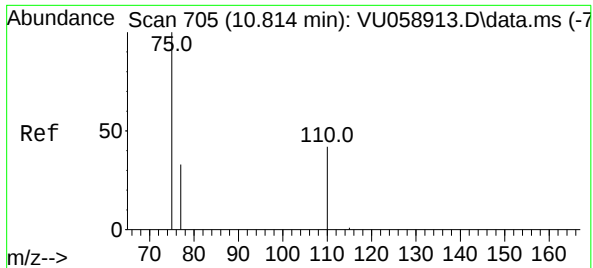

#12
 1,2,3-Trichloropropane
 Concen: 0.020 ug/L
 RT: 10.865 min Scan# 70
 Delta R.T. 0.051 min
 Lab File: VU058917.D
 Acq: 20 May 2024 14:17

Instrument :
 MSVOA_U
 ClientSampleId :

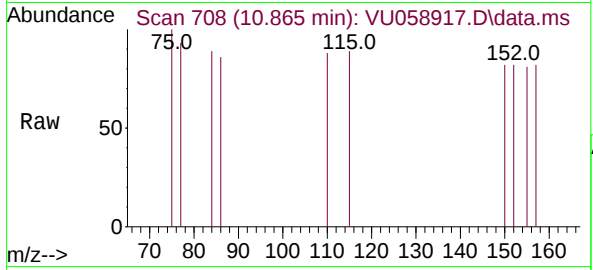

Tgt Ion: 75 Resp: 50

Ion	Ratio	Lower	Upper
75	100		
110	30.0	33.1	49.7#
77	34.0	26.2	39.2

