


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052024\
Data File : VU058910.D
Acq On : 20 May 2024 10:07
Operator : MD/SY
Sample : BFB006
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB006

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052024.M
Title : TRACE VOA SOM01.0
Last Update : Tue May 21 03:23:43 2024

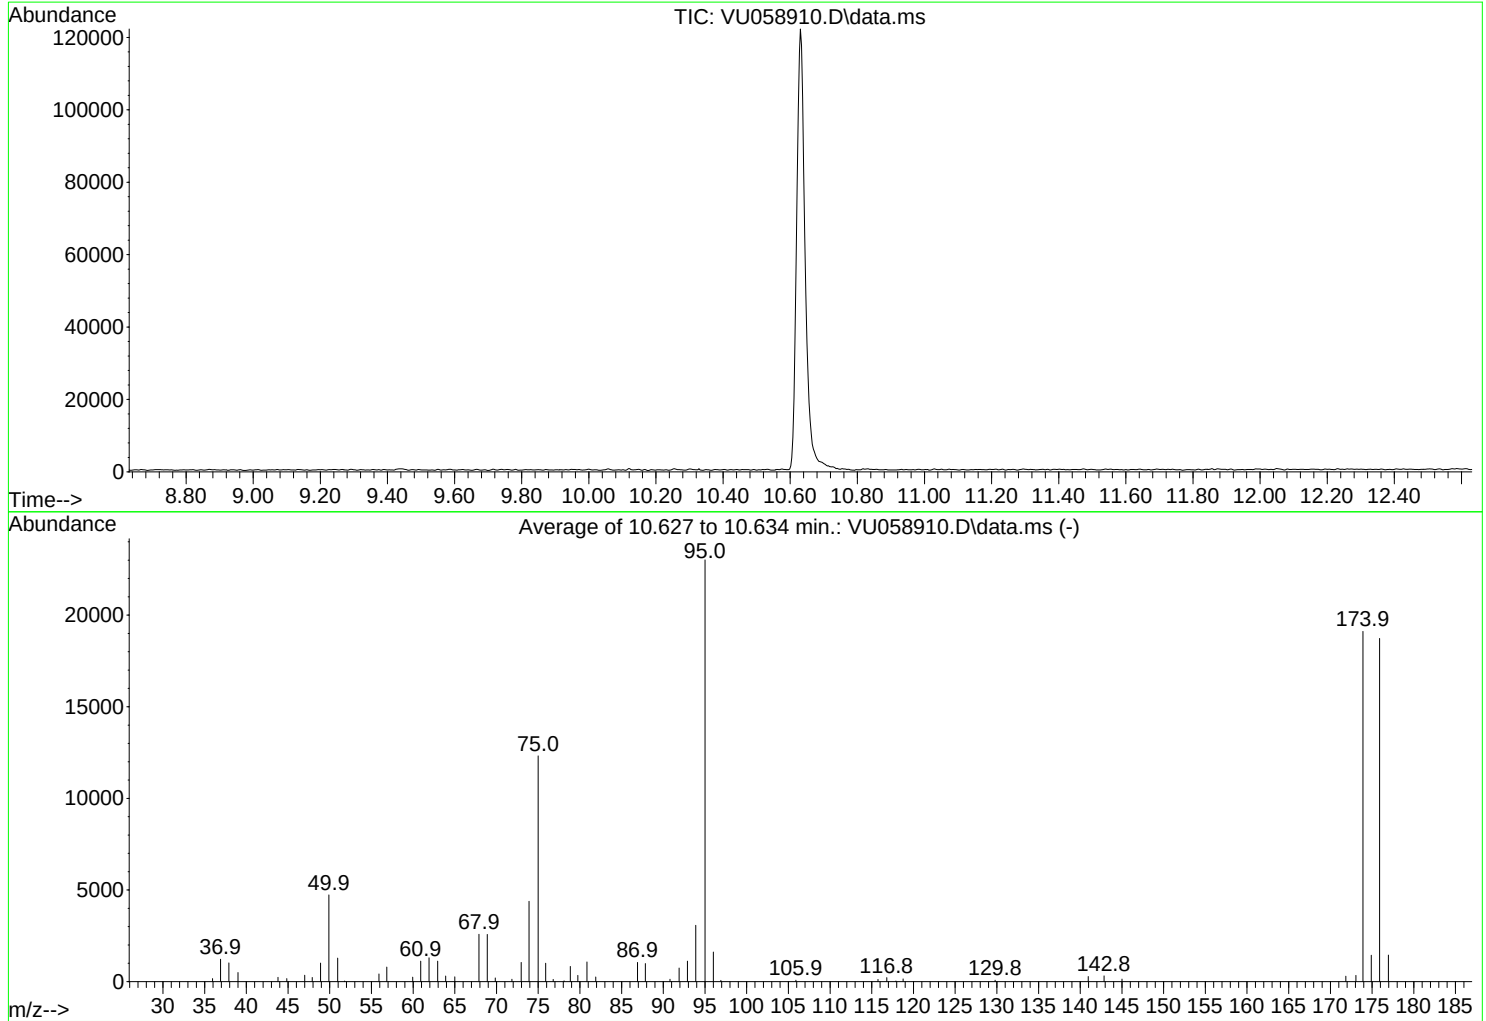

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.6	4731	PASS
75	95	30	80	53.5	12319	PASS
95	95	100	100	100.0	23016	PASS
96	95	5	9	7.0	1612	PASS
173	174	0.00	2	1.8	338	PASS
174	95	50	120	83.1	19115	PASS
175	174	5	9	7.5	1443	PASS
176	174	95	101	98.0	18725	PASS
177	176	5	9	7.7	1446	PASS

Scan 2892 (10.589 min): VU058910.D\data.ms
BFB006

m/z	Abundance
39.80	313.0
43.80	302.0

Instrument :
MSVOA_U
ClientSampleId :
BFB006

m/z	Abundance
35.90	146.0
36.90	1251.0
37.90	1057.0
39.00	516.0
39.80	294.0
43.80	535.0
44.80	179.0
47.00	341.0
47.90	214.0
48.90	1034.0
49.90	4902.0
51.00	1298.0
55.90	446.0
56.90	856.0
60.00	285.0
60.90	1102.0
61.90	1321.0
63.00	1087.0
63.90	255.0
64.90	270.0
67.90	2672.0
68.90	2520.0
69.90	151.0
71.80	155.0
73.00	1015.0
73.90	4168.0
75.00	12343.0
75.90	957.0
76.90	107.0
78.80	860.0
79.80	341.0
80.90	1019.0
81.90	223.0
86.90	1147.0
87.90	926.0
90.80	113.0
91.90	663.0
92.90	1094.0
93.90	3037.0
95.00	22472.0
96.00	1589.0
115.70	138.0
116.70	228.0
117.90	111.0
118.70	138.0
140.90	266.0
142.90	287.0
145.00	113.0
171.80	251.0
173.00	313.0
173.90	18224.0
174.90	1393.0
175.90	17960.0
176.90	1379.0

Instrument :
MSVOA_U
ClientSampleId :
BFB006

m/z	Abundance
35.90	179.0
36.90	1252.0
37.90	1036.0
39.00	508.0
39.80	300.0
43.90	553.0
44.80	170.0
47.00	385.0
47.90	229.0
48.90	1010.0
49.90	4913.0
51.00	1298.0
55.90	418.0
56.90	813.0
59.90	254.0
60.90	1125.0
61.90	1329.0
63.00	1148.0
63.90	323.0
65.00	258.0
67.90	2656.0
68.90	2647.0
69.80	204.0
71.80	132.0
72.90	1044.0
73.90	4569.0
75.00	12593.0
75.90	1065.0
76.80	129.0
78.90	867.0
79.70	354.0
80.80	1125.0
81.90	257.0
86.90	1064.0
87.80	1047.0
90.80	143.0
91.90	759.0
92.90	1141.0
93.90	3153.0
95.00	23640.0
96.00	1662.0
96.90	108.0
105.90	110.0
115.80	127.0
116.80	214.0
118.80	157.0
129.80	101.0
141.00	295.0
142.80	337.0
145.00	159.0
171.90	306.0
173.00	365.0
173.90	19736.0
174.90	1487.0
175.90	19504.0
176.90	1529.0

Instrument :
MSVOA_U
ClientSampleId :
BFB006

m/z	Abundance
36.00	173.0
36.90	1166.0
37.90	964.0
39.00	471.0
39.80	288.0
43.90	516.0
44.90	150.0
47.00	311.0
47.90	228.0
48.90	989.0
49.90	4378.0
50.90	1252.0
51.80	113.0
55.90	399.0
56.80	727.0
59.90	206.0
60.90	1123.0
61.90	1244.0
62.90	1117.0
63.90	328.0
65.10	249.0
67.90	2430.0
68.90	2568.0
69.90	235.0
71.90	104.0
72.90	1073.0
73.90	4399.0
75.00	12020.0
75.90	1001.0
76.70	140.0
78.10	135.0
78.90	768.0
79.70	317.0
80.80	1077.0
81.90	272.0
86.90	937.0
87.80	978.0
90.80	148.0
91.90	810.0
92.90	1130.0
93.90	3029.0
95.00	22936.0
96.00	1586.0
96.90	100.0
105.90	131.0
115.80	114.0
116.90	203.0
118.80	150.0
129.80	127.0
140.90	271.0
142.80	326.0
145.00	161.0
171.90	341.0
173.10	336.0
173.90	19384.0
174.90	1450.0
175.90	18712.0
177.00	1431.0

Instrument :
MSVOA_U
ClientSampleId :
BFB006