

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052119\
 Data File : VU032199.D
 Acq On : 21 May 2019 14:57
 Operator : JC/SP
 Sample : K2862-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFHK0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.396	89	95	106	rBV	394358	397991	14.06%	1.805%
2	1.669	173	180	202	rVB	295243	387797	13.70%	1.759%
3	2.267	356	366	379	rVB	666180	1000570	35.36%	4.539%
4	2.601	468	470	472	rBV3	465	224	0.01%	0.001%
5	2.634	478	480	484	rVB3	1480	896	0.03%	0.004%
6	2.659	484	488	489	rBV2	631	389	0.01%	0.002%
7	2.724	506	508	510	rVB	869	348	0.01%	0.002%
8	2.756	516	518	522	rVB2	561	366	0.01%	0.002%
9	2.830	532	541	542	rBV5	2489	3551	0.13%	0.016%
10	3.039	602	606	611	rBV4	687	607	0.02%	0.003%
11	3.064	611	614	618	rBV3	699	469	0.02%	0.002%
12	3.087	618	621	623	rVB3	705	383	0.01%	0.002%
13	3.103	623	626	628	rBV2	527	366	0.01%	0.002%
14	3.187	647	652	653	rBV	452	363	0.01%	0.002%
15	3.248	669	671	672	rVB	462	124	0.00%	0.001%
16	3.273	677	679	681	rBV	256	105	0.00%	0.000%
17	3.347	700	702	704	rVB2	209	87	0.00%	0.000%
18	3.363	704	707	710	rBV3	422	262	0.01%	0.001%
19	3.383	710	713	717	rBV2	821	807	0.03%	0.004%
20	3.453	729	735	737	rBV4	607	590	0.02%	0.003%
21	3.524	754	757	759	rBV	266	161	0.01%	0.001%
22	3.540	759	762	764	rBV2	557	407	0.01%	0.002%
23	3.576	770	773	776	rBV3	436	280	0.01%	0.001%
24	3.627	787	789	790	rBV	138	38	0.00%	0.000%
25	3.637	791	792	795	rVB2	435	221	0.01%	0.001%
26	3.653	795	797	800	rBV	631	238	0.01%	0.001%
27	3.672	801	803	805	rBV2	217	108	0.00%	0.000%
28	3.772	831	834	835	rVB	521	221	0.01%	0.001%
29	3.785	835	838	839	rBV	164	102	0.00%	0.000%
30	3.804	841	844	850	rVV2	328	260	0.01%	0.001%
31	3.830	850	852	855	rVV2	187	103	0.00%	0.000%
32	3.849	857	858	860	rVB2	396	128	0.00%	0.001%
33	3.865	860	863	865	rBV	295	178	0.01%	0.001%
34	3.884	865	869	872	rVB2	449	398	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052119\
 Data File : VU032199.D
 Acq On : 21 May 2019 14:57
 Operator : JC/SP
 Sample : K2862-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFHK0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052119WMA.M
 Title : VOC Analysis

35	3.897	872	873	874	rBV	261	78	0.00%	0.000%
36	3.916	877	879	880	rBV	52	19	0.00%	0.000%
37	3.933	880	884	888	rVB2	429	284	0.01%	0.001%
38	3.955	888	891	896	rBV2	472	440	0.02%	0.002%
39	3.984	896	900	901	rBV2	308	241	0.01%	0.001%
40	4.013	907	909	910	rBV2	312	150	0.01%	0.001%
41	4.042	915	918	922	rVV3	629	429	0.02%	0.002%
42	4.077	926	929	933	rVB	809	594	0.02%	0.003%
43	4.103	933	937	941	rBV3	952	698	0.02%	0.003%
44	4.170	946	958	996	rBV	266452	702879	24.84%	3.188%
45	4.643	1089	1105	1137	rBV2	465168	1097918	38.79%	4.980%
46	4.865	1170	1174	1175	rBV4	969	744	0.03%	0.003%
47	4.958	1200	1203	1206	rBV3	764	524	0.02%	0.002%
48	4.974	1206	1208	1211	rBV4	1023	696	0.02%	0.003%
49	5.048	1226	1231	1235	rVB3	674	597	0.02%	0.003%
50	5.170	1265	1269	1270	rBV2	475	319	0.01%	0.001%
51	5.183	1270	1273	1275	rVV3	595	400	0.01%	0.002%
52	5.212	1280	1282	1284	rBV2	248	113	0.00%	0.001%
53	5.235	1286	1289	1294	rBV3	694	588	0.02%	0.003%
54	5.334	1296	1320	1348	rBV2	960663	2830057	100.00%	12.838%
55	5.881	1477	1490	1517	rBV	854559	1728197	61.07%	7.840%
56	6.174	1572	1581	1599	rVB5	17002	40798	1.44%	0.185%
57	6.325	1615	1628	1649	rBV	586292	1187784	41.97%	5.388%
58	6.598	1709	1713	1715	rBV2	1261	1163	0.04%	0.005%
59	6.649	1726	1729	1731	rBV	1000	591	0.02%	0.003%
60	6.749	1757	1760	1764	rBV2	656	556	0.02%	0.003%
61	6.794	1772	1774	1779	rVB2	724	426	0.02%	0.002%
62	6.965	1823	1827	1830	rBV3	592	479	0.02%	0.002%
63	7.026	1843	1846	1849	rBV3	289	186	0.01%	0.001%
64	7.106	1865	1871	1874	rBV4	970	973	0.03%	0.004%
65	7.161	1886	1888	1891	rBV	473	174	0.01%	0.001%
66	7.183	1893	1895	1896	rBV	386	143	0.01%	0.001%
67	7.225	1896	1908	1932	rBV	315786	580169	20.50%	2.632%
68	7.399	1960	1962	1964	rBV3	1067	664	0.02%	0.003%
69	7.559	1999	2012	2045	rBV	1312698	2387499	84.36%	10.830%
70	7.846	2091	2101	2127	rBV	215228	385643	13.63%	1.749%
71	8.138	2189	2192	2194	rBV3	703	475	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052119\
 Data File : VU032199.D
 Acq On : 21 May 2019 14:57
 Operator : JC/SP
 Sample : K2862-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFHK0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052119WMA.M
 Title : VOC Analysis

72	8.173	2197	2203	2211	rVB7	2763	4254	0.15%	0.019%
73	8.305	2234	2244	2279	rBV	857367	1655768	58.51%	7.511%
74	8.752	2381	2383	2385	rVB	730	316	0.01%	0.001%
75	8.784	2390	2393	2398	rBV3	1141	947	0.03%	0.004%
76	8.833	2405	2408	2410	rBV2	919	639	0.02%	0.003%
77	9.087	2474	2487	2536	rBV	1265121	2202761	77.83%	9.992%
78	9.736	2687	2689	2692	rVB2	406	183	0.01%	0.001%
79	9.817	2710	2714	2719	rBV4	934	941	0.03%	0.004%
80	9.942	2751	2753	2754	rBV2	458	136	0.00%	0.001%
81	10.000	2766	2771	2775	rBV2	565	683	0.02%	0.003%
82	10.042	2781	2784	2786	rBV3	989	588	0.02%	0.003%
83	10.077	2793	2795	2802	rVV4	883	801	0.03%	0.004%
84	10.109	2802	2805	2807	rVB2	716	414	0.01%	0.002%
85	10.161	2817	2821	2824	rBV6	1144	1069	0.04%	0.005%
86	10.312	2862	2868	2872	rBV3	538	723	0.03%	0.003%
87	10.427	2891	2904	2931	rBV	963406	1559765	55.11%	7.075%
88	10.640	2967	2970	2972	rBV2	592	370	0.01%	0.002%
89	10.726	2995	2997	3002	rVB2	986	618	0.02%	0.003%
90	10.855	3034	3037	3038	rBV	575	325	0.01%	0.001%
91	11.154	3127	3130	3133	rBV3	786	600	0.02%	0.003%
92	11.347	3187	3190	3192	rBV	407	286	0.01%	0.001%
93	11.479	3219	3231	3258	rBV	1119396	1825608	64.51%	8.281%
94	11.855	3336	3348	3368	rBV	1220304	2032920	71.83%	9.222%
95	12.656	3595	3597	3600	rBV2	1117	787	0.03%	0.004%
96	13.382	3821	3823	3825	rBV	516	299	0.01%	0.001%


Sum of corrected areas: 22044627

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU052119\
Data File : VU032199.D
Acq On : 21 May 2019 14:57
Operator : JC/SP
Sample : K2862-05
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFHK0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

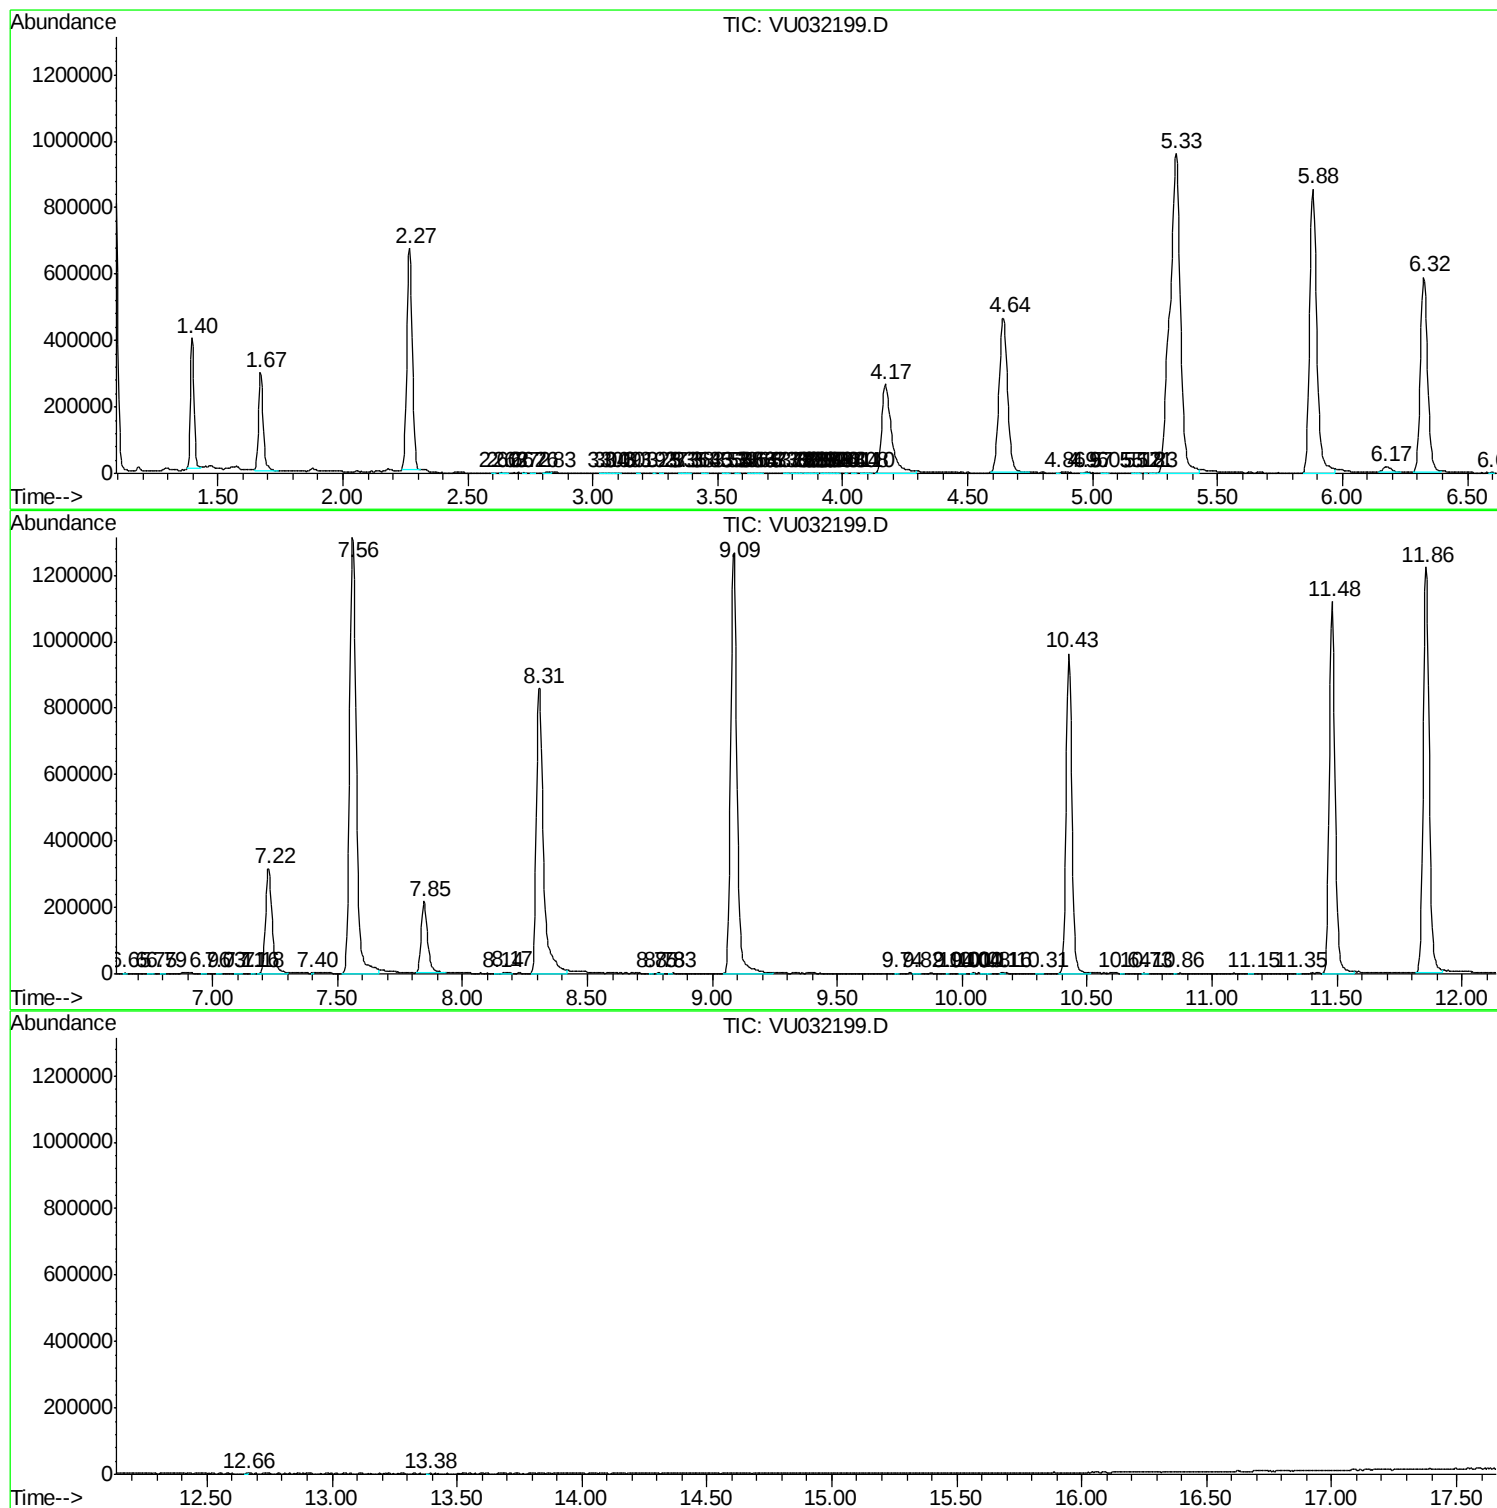

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU052119\
Data File : VU032199.D
Acq On : 21 May 2019 14:57
Operator : JC/SP
Sample : K2862-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFHK0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU052119\
Data File : VU032199.D
Acq On : 21 May 2019 14:57
Operator : JC/SP
Sample : K2862-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFHK0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc