

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052119\
 Data File : VU032208.D
 Acq On : 21 May 2019 18:54
 Operator : JC/SP
 Sample : K2862-10
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFHG1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.396	89	95	107	rBV	403625	409436	14.13%	1.871%
2	1.672	173	181	203	rVB	301643	401385	13.85%	1.834%
3	2.267	355	366	379	rBV	685902	1045592	36.07%	4.778%
4	2.434	416	418	420	rVB2	608	256	0.01%	0.001%
5	2.453	420	424	429	rBV4	1537	1946	0.07%	0.009%
6	2.550	450	454	456	rBV3	441	355	0.01%	0.002%
7	2.563	456	458	460	rVB2	785	358	0.01%	0.002%
8	2.579	460	463	464	rBV2	334	154	0.01%	0.001%
9	2.698	495	500	503	rBV3	1428	1559	0.05%	0.007%
10	2.788	526	528	530	rBV2	467	210	0.01%	0.001%
11	2.836	530	543	554	rBV5	4329	9582	0.33%	0.044%
12	2.878	554	556	559	rVB	498	231	0.01%	0.001%
13	2.916	565	568	569	rBV	382	248	0.01%	0.001%
14	2.926	569	571	573	rVV	525	290	0.01%	0.001%
15	3.000	590	594	595	rBV	504	364	0.01%	0.002%
16	3.032	602	604	607	rVB2	757	335	0.01%	0.002%
17	3.058	610	612	614	rBV	365	146	0.01%	0.001%
18	3.068	614	615	617	rVB	465	169	0.01%	0.001%
19	3.077	617	618	620	rBV	54	19	0.00%	0.000%
20	3.106	620	627	629	rBV4	786	824	0.03%	0.004%
21	3.132	632	635	637	rBV2	363	192	0.01%	0.001%
22	3.186	649	652	655	rBV3	640	516	0.02%	0.002%
23	3.215	659	661	664	rBV	475	321	0.01%	0.001%
24	3.244	667	670	673	rBV3	357	300	0.01%	0.001%
25	3.302	686	688	691	rBV2	669	435	0.02%	0.002%
26	3.344	698	701	702	rBV	530	322	0.01%	0.001%
27	3.418	722	724	726	rVB	399	170	0.01%	0.001%
28	3.444	729	732	735	rVB2	793	413	0.01%	0.002%
29	3.486	741	745	748	rBV2	575	498	0.02%	0.002%
30	3.518	753	755	757	rVB	584	247	0.01%	0.001%
31	3.531	757	759	762	rVB	293	123	0.00%	0.001%
32	3.556	762	767	773	rBV2	732	811	0.03%	0.004%
33	3.595	777	779	780	rBV	368	160	0.01%	0.001%
34	3.633	787	791	793	rBV3	616	376	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052119\
 Data File : VU032208.D
 Acq On : 21 May 2019 18:54
 Operator : JC/SP
 Sample : K2862-10
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFHG1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052119WMA.M
 Title : VOC Analysis

35	3.656	793	798	800	rBV3	671	460	0.02%	0.002%
36	3.701	809	812	815	rBV2	593	337	0.01%	0.002%
37	3.736	819	823	826	rVB3	649	513	0.02%	0.002%
38	3.756	826	829	830	rBV	205	131	0.00%	0.001%
39	3.765	830	832	836	rVB2	645	354	0.01%	0.002%
40	3.788	836	839	842	rBV2	550	459	0.02%	0.002%
41	3.830	849	852	855	rBV2	319	187	0.01%	0.001%
42	3.846	855	857	860	rBV	396	264	0.01%	0.001%
43	3.913	877	878	880	rBV	193	89	0.00%	0.000%
44	3.961	888	893	897	rBV2	753	808	0.03%	0.004%
45	4.000	901	905	908	rBV	299	292	0.01%	0.001%
46	4.026	911	913	916	rVB2	639	348	0.01%	0.002%
47	4.048	916	920	922	rBV3	386	295	0.01%	0.001%
48	4.093	932	934	937	rVB2	390	203	0.01%	0.001%
49	4.170	946	958	991	rBV	221701	591898	20.42%	2.705%
50	4.643	1089	1105	1131	rBV	477347	1124729	38.80%	5.140%
51	5.045	1228	1230	1233	rVB2	450	208	0.01%	0.001%
52	5.071	1236	1238	1241	rVV2	374	178	0.01%	0.001%
53	5.103	1246	1248	1250	rBV	449	213	0.01%	0.001%
54	5.119	1250	1253	1254	rBV2	323	157	0.01%	0.001%
55	5.129	1254	1256	1257	rBV	334	155	0.01%	0.001%
56	5.228	1285	1287	1290	rVB3	417	240	0.01%	0.001%
57	5.334	1296	1320	1357	rBV3	975946	2898645	100.00%	13.246%
58	5.739	1443	1446	1449	rBV	984	816	0.03%	0.004%
59	5.813	1466	1469	1472	rBV3	511	419	0.01%	0.002%
60	5.881	1477	1490	1523	rBV	859840	1738629	59.98%	7.945%
61	6.325	1615	1628	1651	rBV	600931	1212396	41.83%	5.540%
62	6.614	1716	1718	1720	rBV2	426	272	0.01%	0.001%
63	6.669	1733	1735	1738	rBV3	667	520	0.02%	0.002%
64	6.727	1751	1753	1755	rBV2	403	157	0.01%	0.001%
65	6.746	1757	1759	1760	rBV	651	255	0.01%	0.001%
66	6.772	1765	1767	1771	rBV3	466	244	0.01%	0.001%
67	6.807	1776	1778	1781	rBV	530	373	0.01%	0.002%
68	6.829	1783	1785	1790	rBV3	479	394	0.01%	0.002%
69	7.045	1850	1852	1856	rVB3	596	453	0.02%	0.002%
70	7.074	1856	1861	1864	rBV3	755	709	0.02%	0.003%
71	7.222	1895	1907	1933	rBV2	316870	585515	20.20%	2.676%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052119\
 Data File : VU032208.D
 Acq On : 21 May 2019 18:54
 Operator : JC/SP
 Sample : K2862-10
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFHG1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052119WMA.M
 Title : VOC Analysis

72	7.559	1999	2012	2050	rBV	1333606	2433898	83.97%	11.123%
73	7.845	2091	2101	2132	rBV	216297	394257	13.60%	1.802%
74	8.308	2233	2245	2279	rBV	680438	1307275	45.10%	5.974%
75	8.868	2416	2419	2422	rBV2	892	654	0.02%	0.003%
76	8.913	2430	2433	2438	rBV3	428	407	0.01%	0.002%
77	8.935	2438	2440	2445	rVV3	771	429	0.01%	0.002%
78	8.977	2451	2453	2454	rBV	529	248	0.01%	0.001%
79	9.025	2466	2468	2472	rVB3	1036	588	0.02%	0.003%
80	9.083	2474	2486	2511	rBV	1269583	2174874	75.03%	9.939%
81	9.521	2618	2622	2627	rVB3	906	704	0.02%	0.003%
82	9.656	2661	2664	2666	rBV2	755	527	0.02%	0.002%
83	9.842	2719	2722	2725	rBV	823	468	0.02%	0.002%
84	10.048	2784	2786	2792	rVB3	912	588	0.02%	0.003%
85	10.122	2807	2809	2810	rBV	376	95	0.00%	0.000%
86	10.135	2810	2813	2815	rBV2	821	531	0.02%	0.002%
87	10.305	2863	2866	2869	rBV3	588	390	0.01%	0.002%
88	10.427	2892	2904	2929	rBV	933487	1509443	52.07%	6.898%
89	10.652	2967	2974	2977	rBV5	1207	1252	0.04%	0.006%
90	10.781	3011	3014	3017	rVB3	769	477	0.02%	0.002%
91	10.800	3017	3020	3021	rBV	463	239	0.01%	0.001%
92	10.884	3044	3046	3049	rVB2	817	400	0.01%	0.002%
93	11.177	3135	3137	3139	rBV2	580	334	0.01%	0.002%
94	11.193	3139	3142	3143	rBV	944	544	0.02%	0.002%
95	11.479	3219	3231	3260	rBV	1168717	1876319	64.73%	8.575%
96	11.855	3336	3348	3376	rBV	1271821	2135738	73.68%	9.760%
97	12.549	3562	3564	3567	rVB2	1319	445	0.02%	0.002%
98	12.829	3649	3651	3655	rBV3	1197	740	0.03%	0.003%


Sum of corrected areas: 21882522

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU052119\
Data File : VU032208.D
Acq On : 21 May 2019 18:54
Operator : JC/SP
Sample : K2862-10
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFHG1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

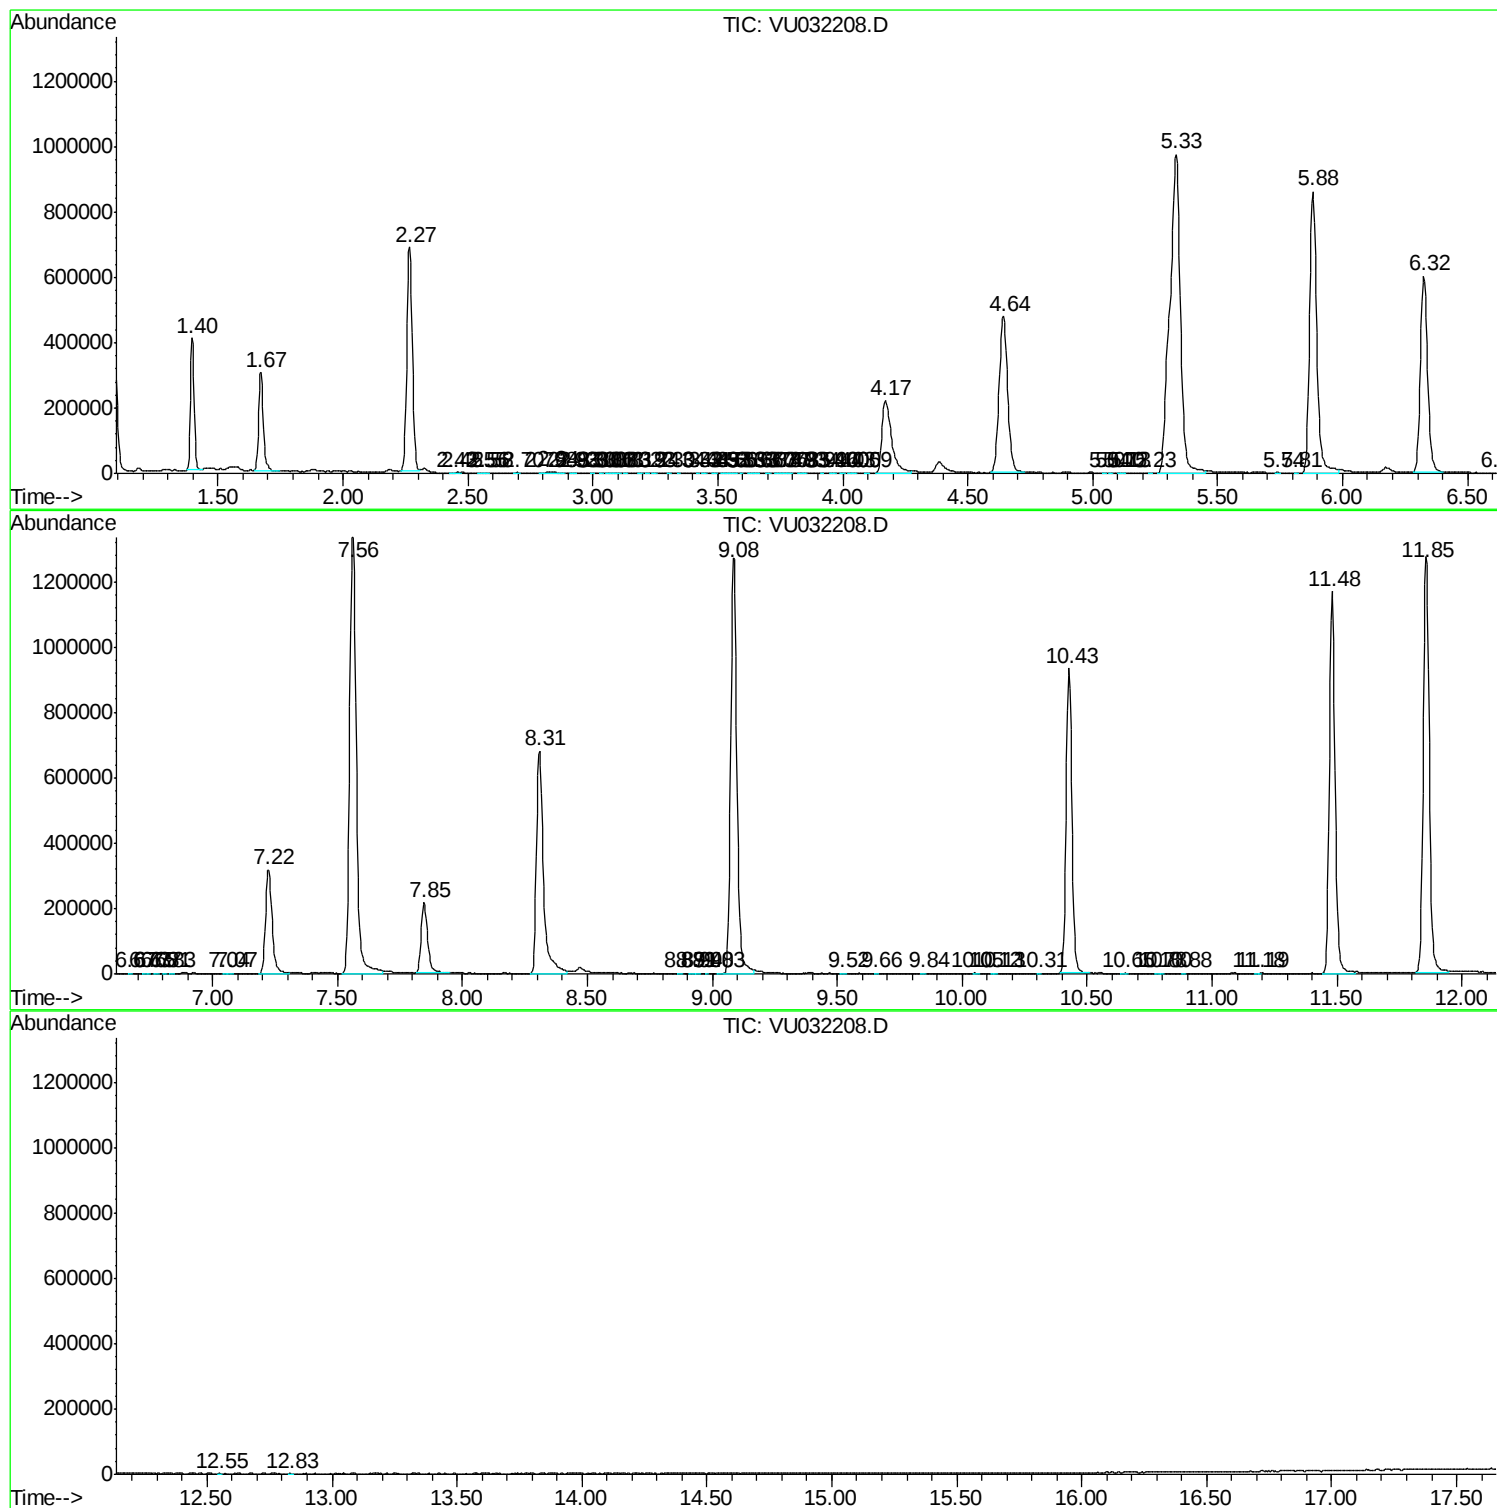

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU052119\
Data File : VU032208.D
Acq On : 21 May 2019 18:54
Operator : JC/SP
Sample : K2862-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFHG1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU052119\
Data File : VU032208.D
Acq On : 21 May 2019 18:54
Operator : JC/SP
Sample : K2862-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFHG1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc