


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052119\
 Data File : VU032183.D
 Acq On : 21 May 2019 07:59
 Operator : JC/SP
 Sample : BFB44
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB44

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052119WMA.M
 Title : VOC Analysis
 Last Update : Wed May 22 02:08:11 2019

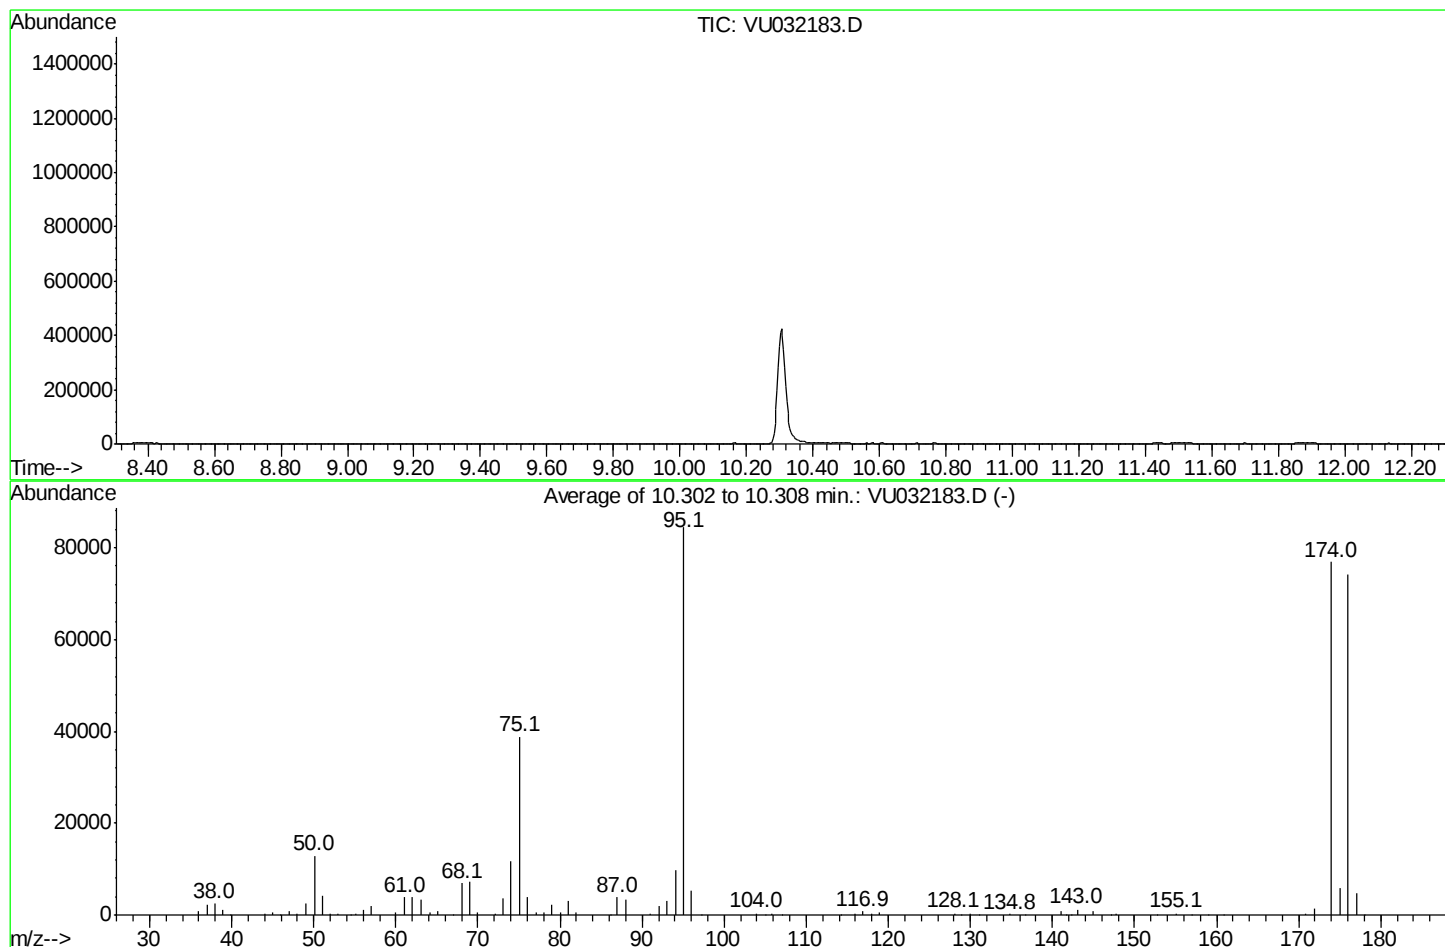

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	12973	PASS
75	95	30	80	46.1	38904	PASS
95	95	100	100	100.0	84448	PASS
96	95	5	9	6.4	5391	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	91.0	76882	PASS
175	174	5	9	7.6	5859	PASS
176	174	95	101	96.5	74157	PASS
177	176	5	9	6.3	4693	PASS

Scan 2853 (10.263 min): VU032183.D
BFB44

m/z	Abundance
35.90	317.0
37.90	211.0
39.90	538.0
44.00	408.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	1119.0
37.00	2302.0
38.00	2468.0
38.90	1339.0
39.90	519.0
44.10	701.0
45.00	604.0
45.90	129.0
47.00	1144.0
47.90	340.0
49.00	2112.0
50.00	13457.0
51.00	4414.0
52.00	201.0
53.00	167.0
54.50	144.0
55.10	248.0
56.00	1086.0
57.00	1910.0
60.00	706.0
61.00	4028.0
62.10	4109.0
63.10	3468.0
64.20	574.0
65.00	720.0
67.00	135.0
68.10	7159.0
69.10	7119.0
70.00	738.0
72.10	199.0
73.10	3618.0
74.10	11489.0
75.10	39104.0
76.00	3728.0
77.10	660.0
78.00	523.0
79.00	2291.0
80.10	628.0
81.00	2752.0
82.00	461.0
86.10	129.0
87.00	3813.0
88.00	3214.0
91.00	414.0
92.10	1970.0
93.00	3437.0
94.10	9665.0
95.10	84784.0
96.00	5316.0
97.20	212.0
104.00	322.0
105.10	175.0
105.90	339.0
107.00	171.0
116.00	262.0
116.90	762.0
117.90	337.0
118.80	559.0
128.10	423.0
130.00	318.0
131.00	126.0
134.90	230.0
141.00	936.0
141.70	104.0
143.00	1226.0
144.90	855.0
147.10	108.0
147.80	203.0
152.80	107.0
155.10	350.0
157.00	167.0
160.90	147.0
170.90	166.0
171.90	1426.0
174.00	75584.0
175.10	6015.0
176.00	72168.0
177.00	4758.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	1130.0
37.10	2274.0
38.00	2669.0
39.00	1256.0
39.90	607.0
44.00	770.0
45.00	599.0
47.00	989.0
47.90	384.0
49.00	2568.0
50.00	13413.0
51.00	4281.0
52.00	219.0
53.00	253.0
55.00	293.0
56.00	1104.0
57.00	2101.0
60.00	643.0
61.00	4089.0
62.10	4152.0
63.10	3664.0
64.20	532.0
65.00	732.0
66.90	108.0
68.10	6959.0
69.10	7473.0
70.00	734.0
72.10	195.0
73.10	3742.0
74.10	12207.0
75.10	40104.0
76.10	4112.0
77.10	637.0
78.00	482.0
79.00	2257.0
80.00	721.0
81.00	3148.0
82.00	399.0
87.00	3824.0
88.00	3516.0
91.00	365.0
92.10	2127.0
93.00	2937.0
94.10	10077.0
95.10	87152.0
96.10	5578.0
97.20	143.0
104.00	350.0
105.00	166.0
105.90	300.0
107.00	169.0
116.00	318.0
116.90	835.0
117.90	318.0
118.90	558.0
128.10	389.0
128.90	126.0
130.00	322.0
131.00	108.0
134.90	231.0
141.00	937.0
141.80	151.0
143.00	1173.0
144.90	715.0
147.10	126.0
147.80	292.0
155.10	357.0
157.00	133.0
159.00	131.0
170.90	208.0
171.90	1492.0
174.00	78864.0
175.10	6048.0
176.00	76912.0
177.00	4839.0
178.00	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	1066.0
37.10	2268.0
38.00	2730.0
39.00	1178.0
40.00	648.0
43.90	692.0
45.00	522.0
47.00	560.0
48.00	353.0
49.00	2723.0
50.10	12049.0
51.10	3588.0
52.00	237.0
53.00	247.0
55.00	325.0
56.00	955.0
57.00	1908.0
60.00	538.0
61.10	3566.0
62.00	3643.0
63.10	3263.0
64.20	427.0
65.10	781.0
66.80	115.0
68.10	6460.0
69.00	7413.0
70.00	584.0
72.00	265.0
73.10	3396.0
74.00	11824.0
75.10	37504.0
76.10	3865.0
77.20	620.0
78.00	383.0
78.90	2050.0
80.00	663.0
81.00	3041.0
81.90	425.0
87.00	3740.0
88.00	3376.0
91.00	280.0
92.00	2191.0
93.10	2717.0
94.10	9646.0
95.10	81408.0
96.10	5279.0
103.90	363.0
105.00	107.0
105.80	272.0
114.30	120.0
116.00	318.0
116.90	809.0
117.90	259.0
119.00	525.0
128.00	287.0
128.90	200.0
129.90	245.0
134.80	202.0
136.70	107.0
141.00	761.0
141.80	123.0
142.30	180.0
143.00	1091.0
144.90	608.0
147.80	250.0
155.10	276.0
159.00	208.0
170.90	222.0
171.90	1483.0
174.00	76200.0
175.00	5514.0
176.00	73392.0
177.00	4482.0
178.00	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44