

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052120\
 Data File : VU038273.D
 Acq On : 21 May 2020 18:58
 Operator : JC/MD
 Sample : L2724-11DL 40X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BE4T7DL

Quant Time: May 22 03:25:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 22 01:03:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	469685	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	449291	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	221209	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	121078	2.82	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	56.40%
7) Chloroethane-d5	1.93	69	140550	3.78	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	75.60%
11) 1,1-Dichloroethene-d2	2.59	63	185630	2.58	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	51.60%#
20) 2-Butanone-d5	4.66	46	524820	49.51	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.02%
24) Chloroform-d	5.10	84	284842	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.40%
26) 1,2-Dichloroethane-d4	5.74	65	167008	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.40%
32) Benzene-d6	5.76	84	587004	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.20%
36) 1,2-Dichloropropane-d6	6.72	67	192409	4.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.60%
41) Toluene-d8	7.92	98	518844	4.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.80%
43) trans-1,3-Dichloropropene-	8.20	79	67719	3.89	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.80%
46) 2-Hexanone-d5	8.65	63	468678	57.02	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	114.04%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	165296	4.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.40%
64) 1,2-Dichlorobenzene-d4	12.20	152	202789	4.71	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.20%

Target Compounds


					Ovalue
33) Benzene	5.81	78	2516590	17.491 ug/L	100
42) Toluene	7.99	91	12308	0.081 ug/L	97
51) Chlorobenzene	9.47	112	766993	8.137 ug/L	98
52) Ethylbenzene	9.59	91	51522	0.313 ug/L	99
53) m,p-Xylene	9.71	106	123484	1.957 ug/L	99
54) o-Xylene	10.12	106	21952	0.360 ug/L	99
56) Isopropylbenzene	10.50	105	135232	0.863 ug/L	100
63) 1,4-Dichlorobenzene	11.85	146	14166	0.194 ug/L	91
65) 1,2-Dichlorobenzene	12.22	146	10056	0.145 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU052120\
Data File : VU038273.D
Acq On : 21 May 2020 18:58
Operator : JC/MD
Sample : L2724-11DL 40X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BE4T7DL

Quant Time: May 22 03:25:16 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 22 01:03:14 2020
Response via : Initial Calibration

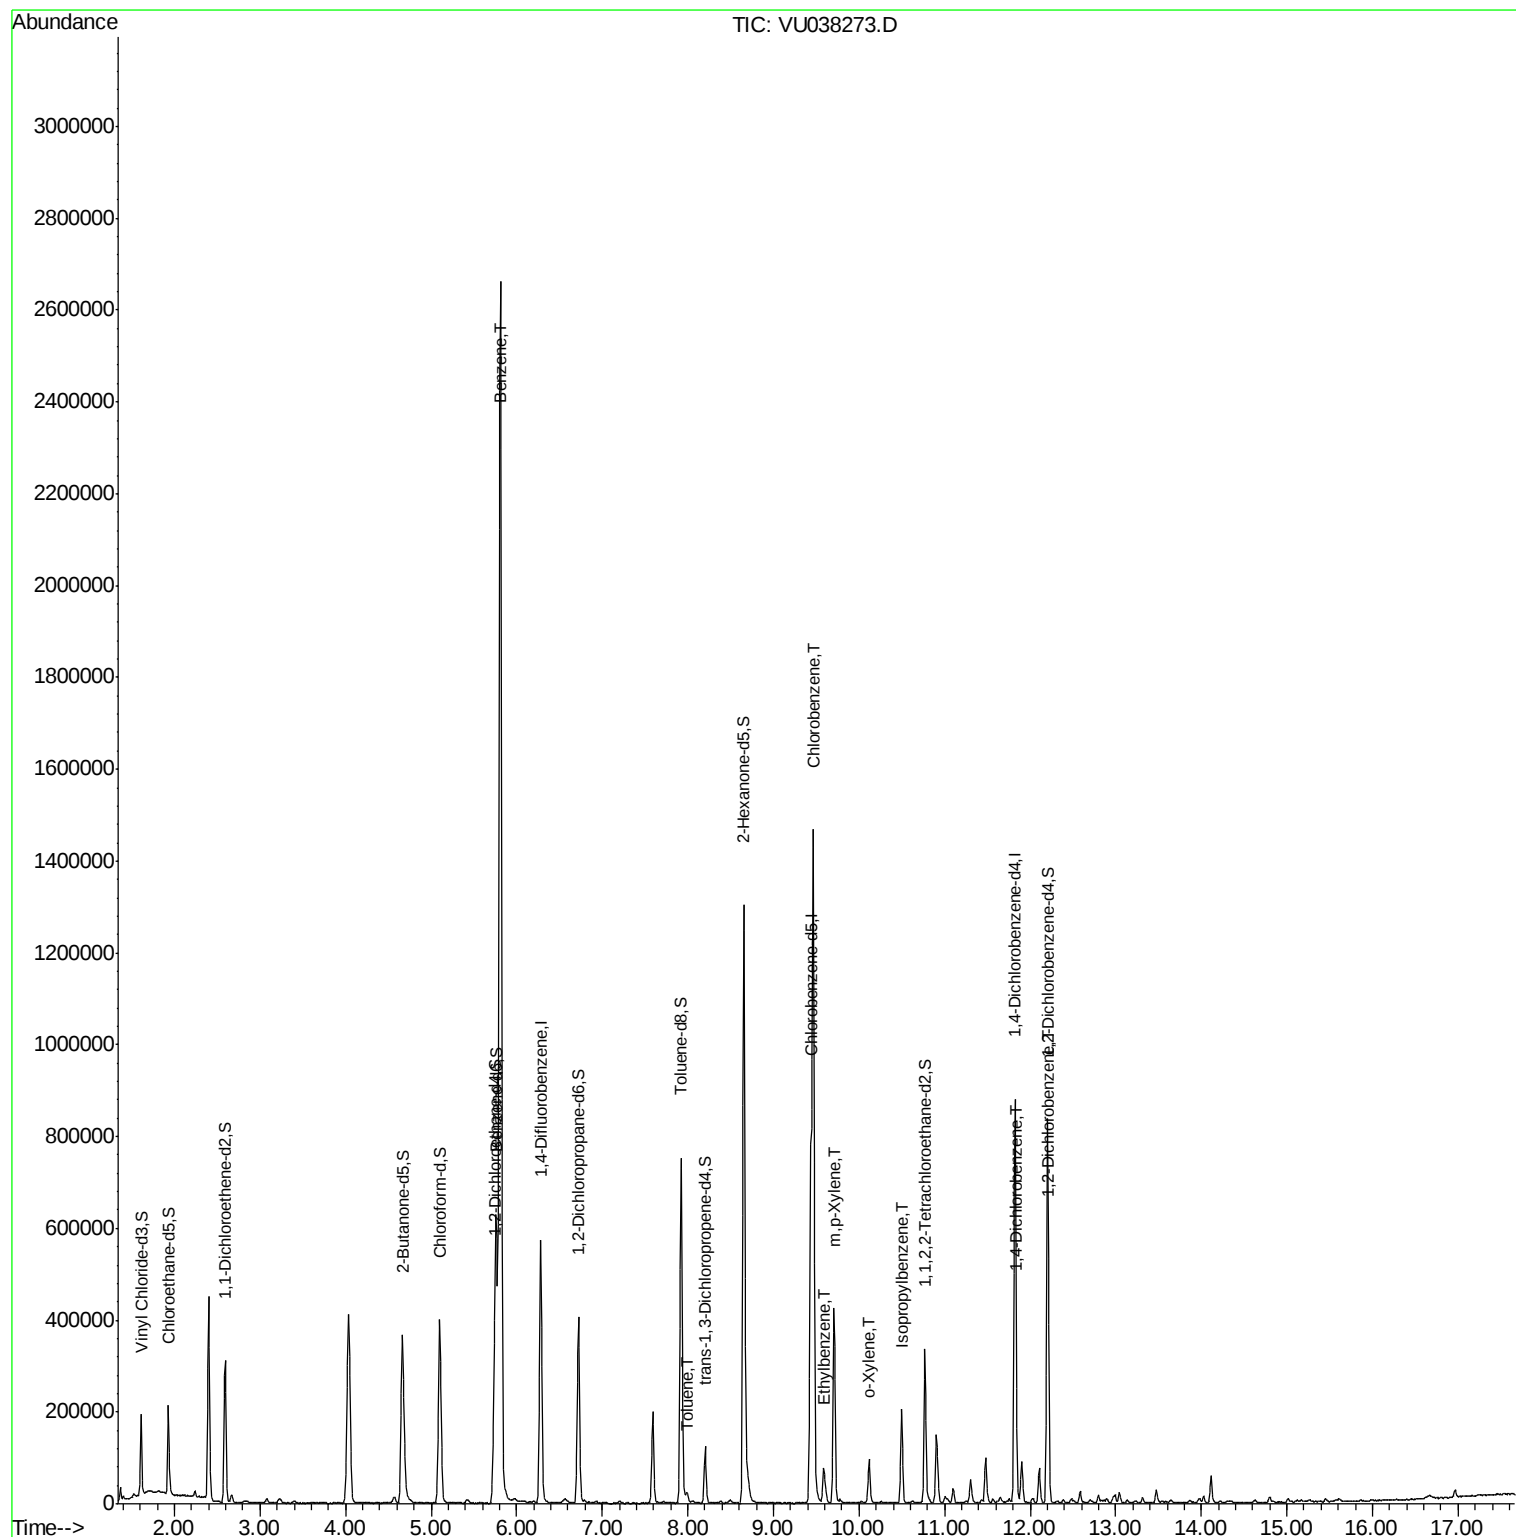

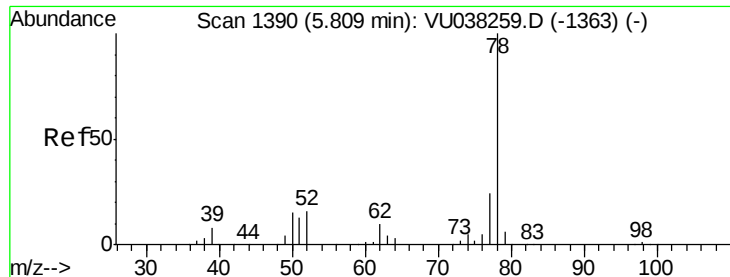

#33

Benzene

Concen: 17.491 ug/L

RT: 5.81 min Scan# 1390

Delta R.T. -0.00 min

Lab File: VU038273.D

Acq: 21 May 2020 18:58


Instrument :

MSVOA_U




ClientSampleId :

BE4T7DL

Tgt Ion: 78 Resp: 2516590

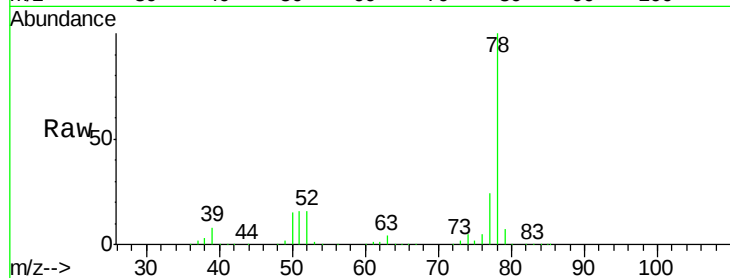

Abundance Ion 78.10 (77.80 to 78.80): VU0

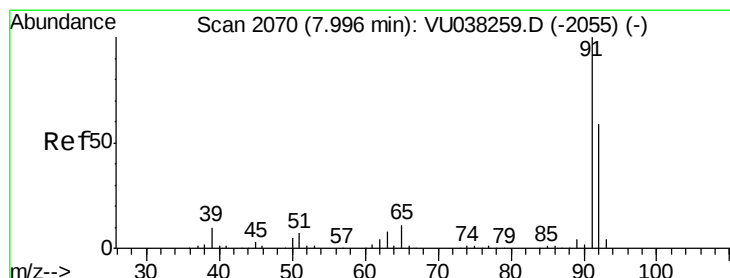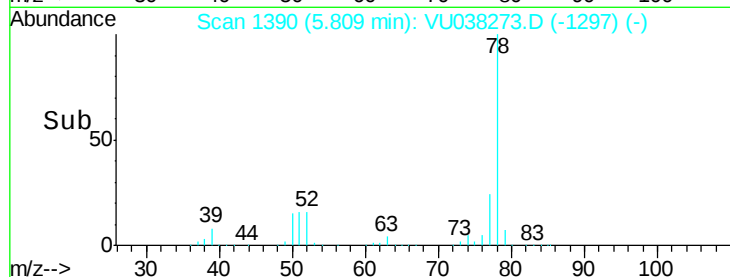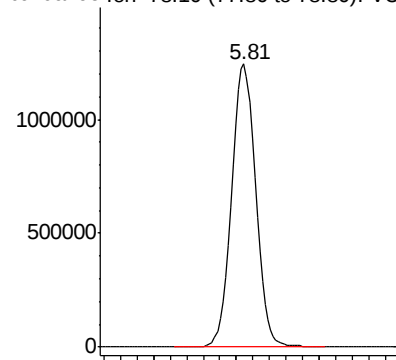

#42

Toluene

Concen: 0.081 ug/L

RT: 7.99 min Scan# 2069

Delta R.T. -0.00 min

Lab File: VU038273.D


Acq: 21 May 2020 18:58

Tgt Ion: 91 Resp: 12308

Ion Ratio Lower Upper



91 100


92 56.5 40.9 75.9

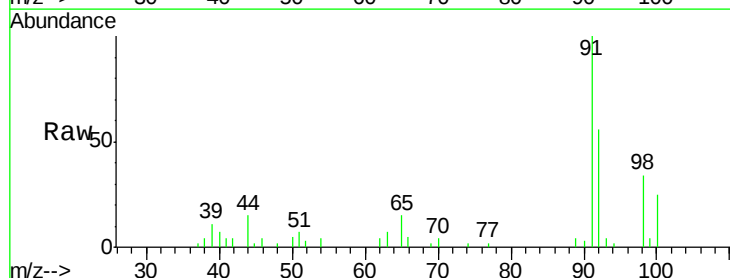

Abundance Ion 91.15 (90.85 to 91.85): VU0

Ion 92.15 (91.85 to 92.85): VU0

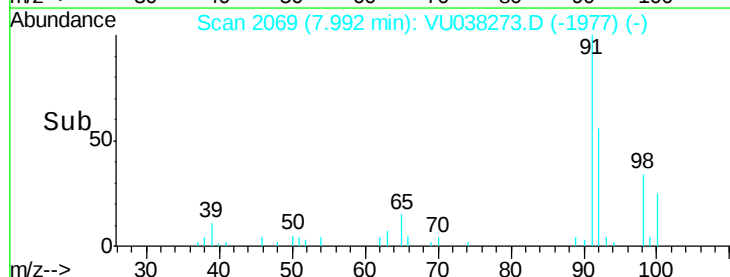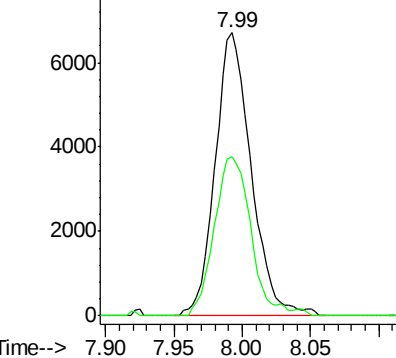


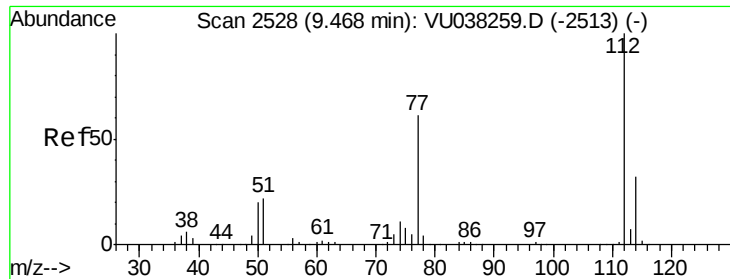




#51
Chlorobenzene
Concen: 8.137 ug/L
RT: 9.47 min Scan# 2527
Delta R.T. -0.00 min
Lab File: VU038273.D
Acq: 21 May 2020 18:58

Instrument :
MSVOA_U
ClientSampleId :
BE4T7DL

Tot Ion:112 Resp: 766993
Ion Ratio Lower Upper
112 100
114 31.3 22.5 41.7
77 60.3 49.9 74.9

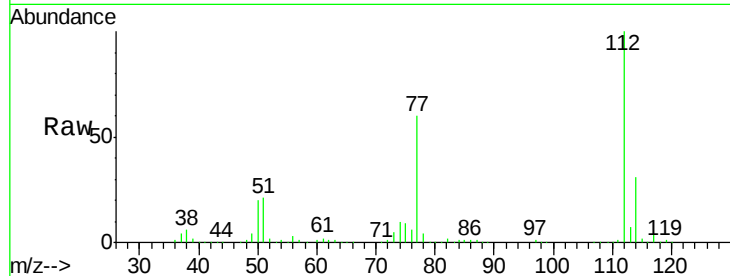


Abundance Ion 112.10 (111.80 to 112.80): V
Ion 114.05 (113.75 to 114.75): V
Ion 77.10 (76.80 to 77.80): V

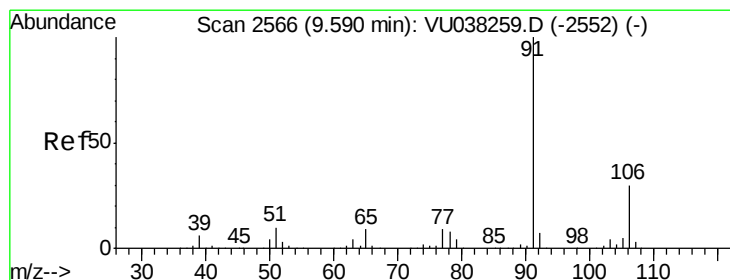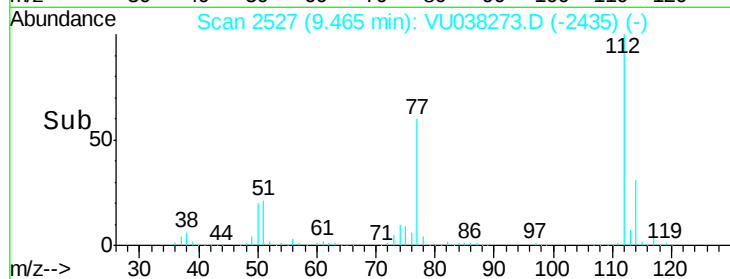
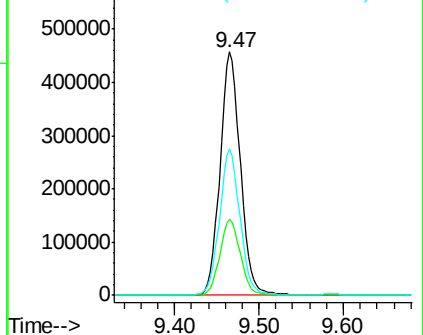



#52
Ethylbenzene
Concen: 0.313 ug/L
RT: 9.59 min Scan# 2565
Delta R.T. -0.00 min
Lab File: VU038273.D
Acq: 21 May 2020 18:58

Tgt Ion: 91 Resp: 51522
Ion Ratio Lower Upper
91 100
106 30.3 21.8 40.4

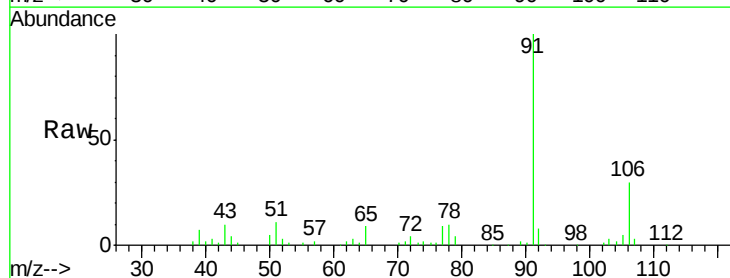

Abundance Ion 91.15 (90.85 to 91.85): V
Ion 106.15 (105.85 to 106.85): V

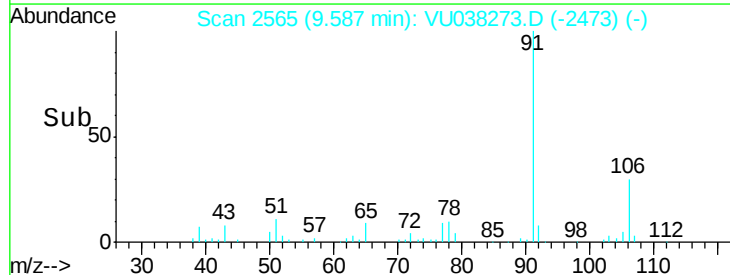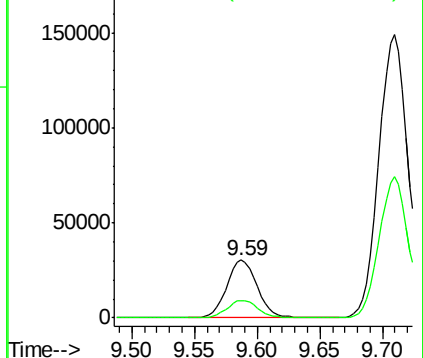


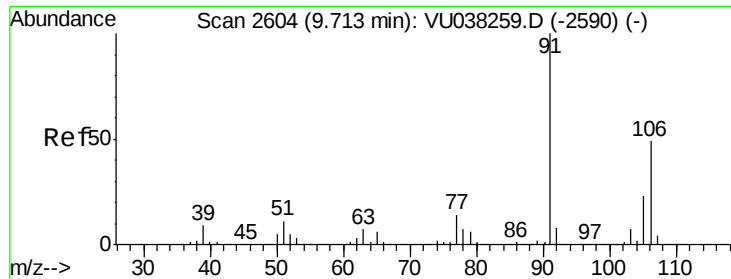




#53
m,p-Xylene
Concen: 1.957 ug/L
RT: 9.71 min Scan# 2603
Delta R.T. -0.00 min
Lab File: VU038273.D
Acq: 21 May 2020 18:58

Instrument :
MSVOA_U
ClientSampleId :
BE4T7DL

Tot Ion:106 Resp: 123484
Ion Ratio Lower Upper
106 100
91 200.8 142.1 263.9

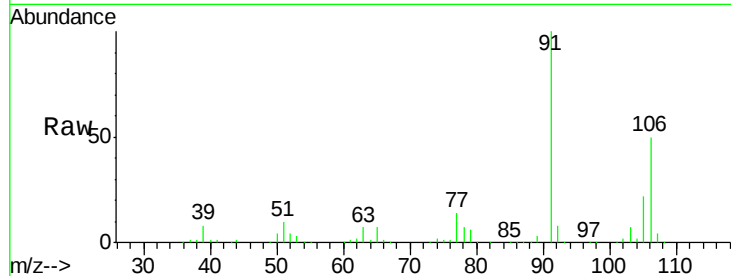


Abundance Ion 106.15 (105.85 to 106.85): V
Ion 91.15 (90.85 to 91.85): VU0

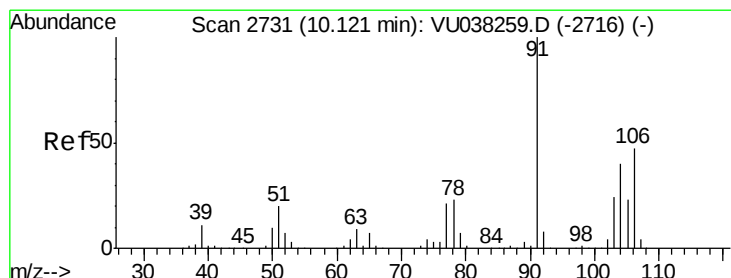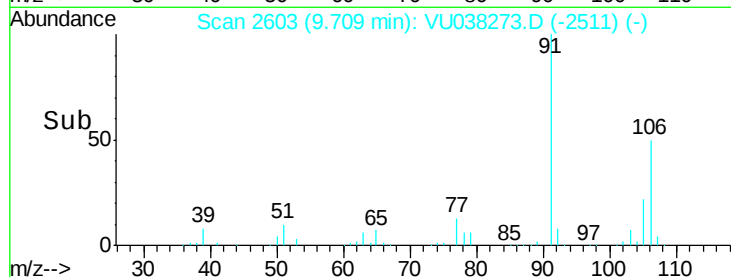
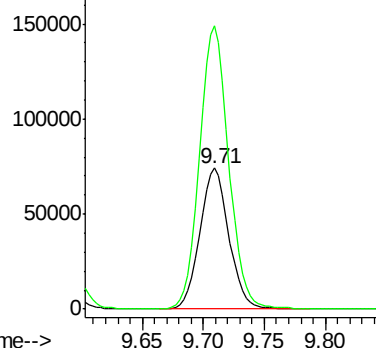



#54
o-Xylene
Concen: 0.360 ug/L
RT: 10.12 min Scan# 2730
Delta R.T. -0.00 min
Lab File: VU038273.D
Acq: 21 May 2020 18:58

Tgt Ion:106 Resp: 21952
Ion Ratio Lower Upper
106 100
91 210.7 148.5 275.9

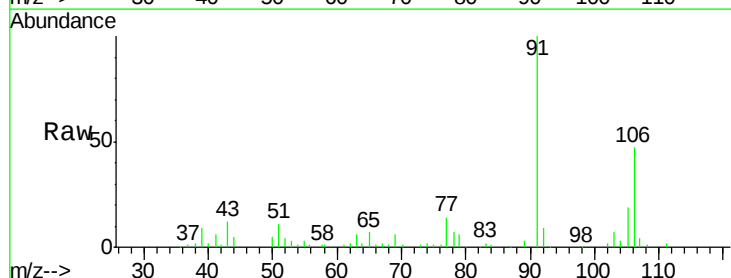

Abundance Ion 106.15 (105.85 to 106.85): V
Ion 91.15 (90.85 to 91.85): VU0

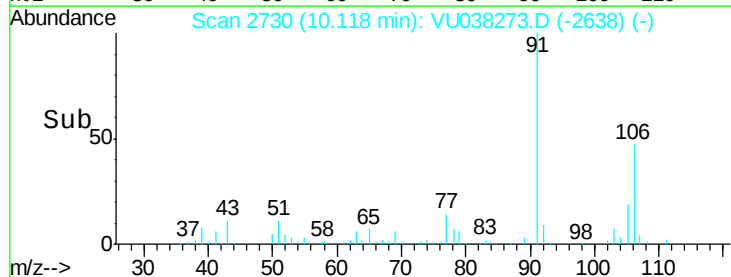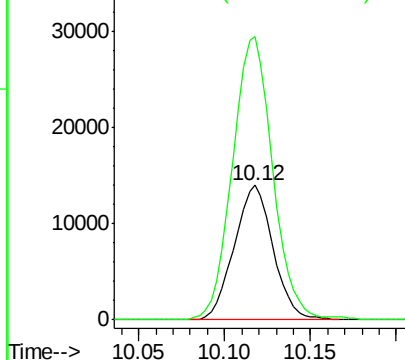

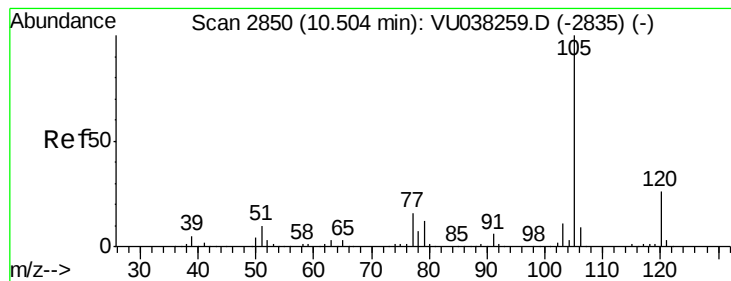

#56

Isopropylbenzene

Concen: 0.863 ug/L

RT: 10.50 min Scan# 2849

Delta R.T. -0.00 min

Lab File: VU038273.D

Acq: 21 May 2020 18:58

Instrument :

MSVOA_U

ClientSampled :

BE4T7DL


Tot Ion:105 Resp: 135232

Ion Ratio Lower Upper

105 100

120 26.3 21.0 31.6




77 15.9 13.0 19.4

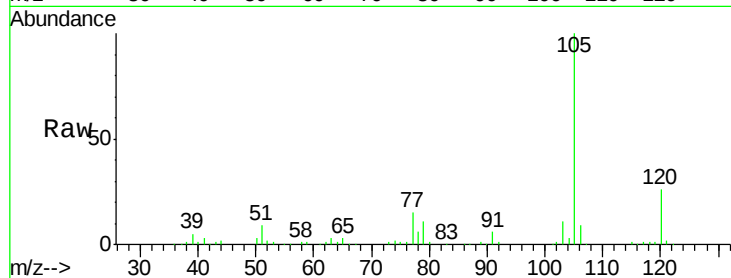

Abundance Ion 105.05 (104.75 to 105.75): V

Ion 120.10 (119.80 to 120.80): V

Ion 77.10 (76.80 to 77.80): V

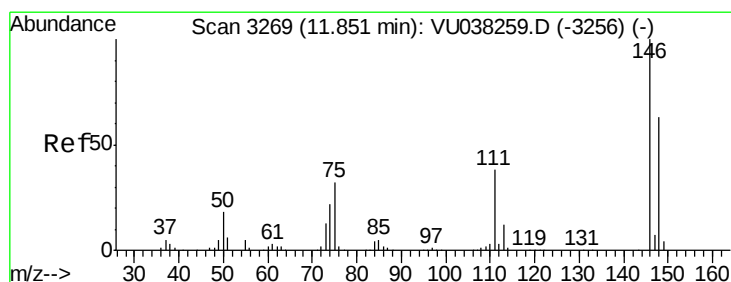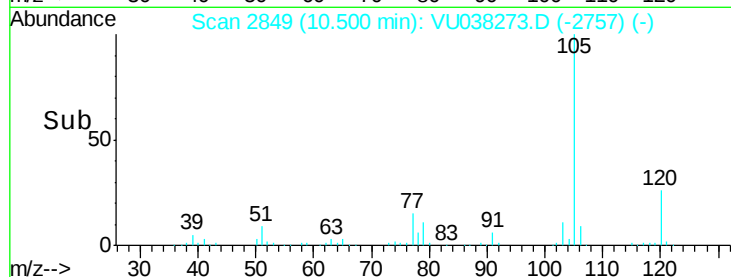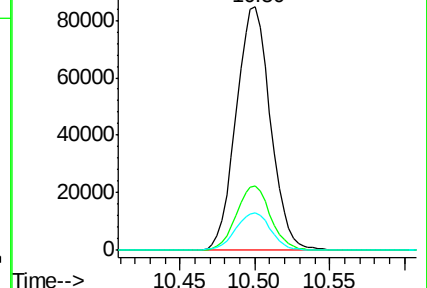

#63

1,4-Dichlorobenzene

Concen: 0.194 ug/L

RT: 11.85 min Scan# 3268

Delta R.T. -0.00 min

Lab File: VU038273.D

Acq: 21 May 2020 18:58


Tgt Ion:146 Resp: 14166

Ion Ratio Lower Upper

146 100

111 39.1 27.2 50.6



148 73.4 43.8 81.3

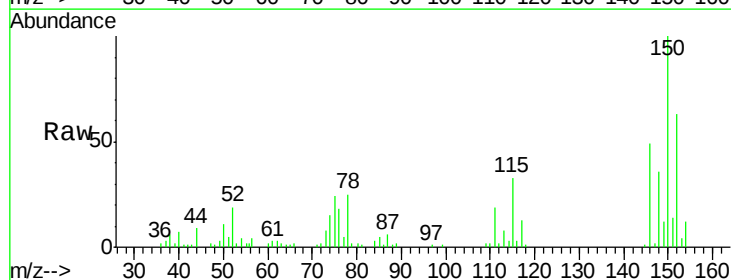


Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

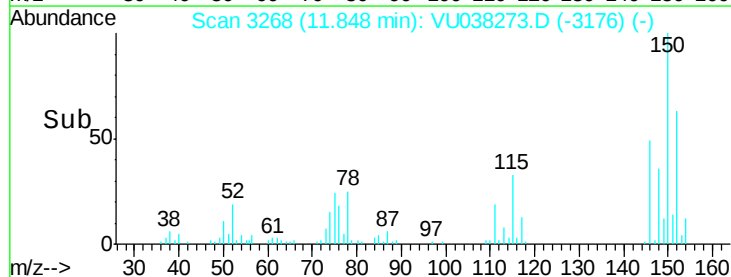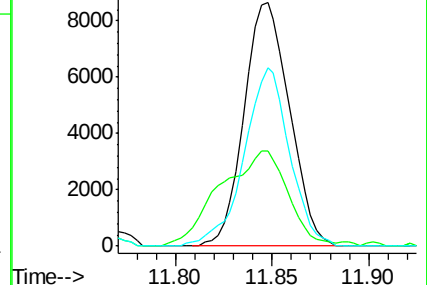

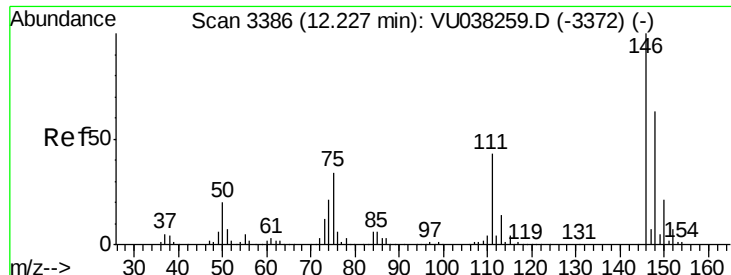

#65

1,2-Dichlorobenzene

Concen: 0.145 ug/L

RT: 12.22 min Scan# 3385

Delta R.T. -0.00 min

Lab File: VU038273.D

Acq: 21 May 2020 18:58

Instrument :

MSVOA_U

ClientSampleId :

BE4T7DL


Tot Ion:146 Resp: 10056

Ion Ratio Lower Upper

146 100

111 48.8 35.3 52.9

148 68.8 51.0 76.4

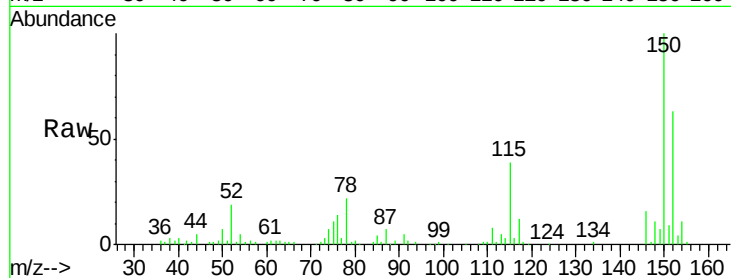

Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

