


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU052120\
Data File : VU038258.D
Acq On : 21 May 2020 10:51
Operator : JC/MD
Sample : BFB28
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB28

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri May 22 10:38:38 2020

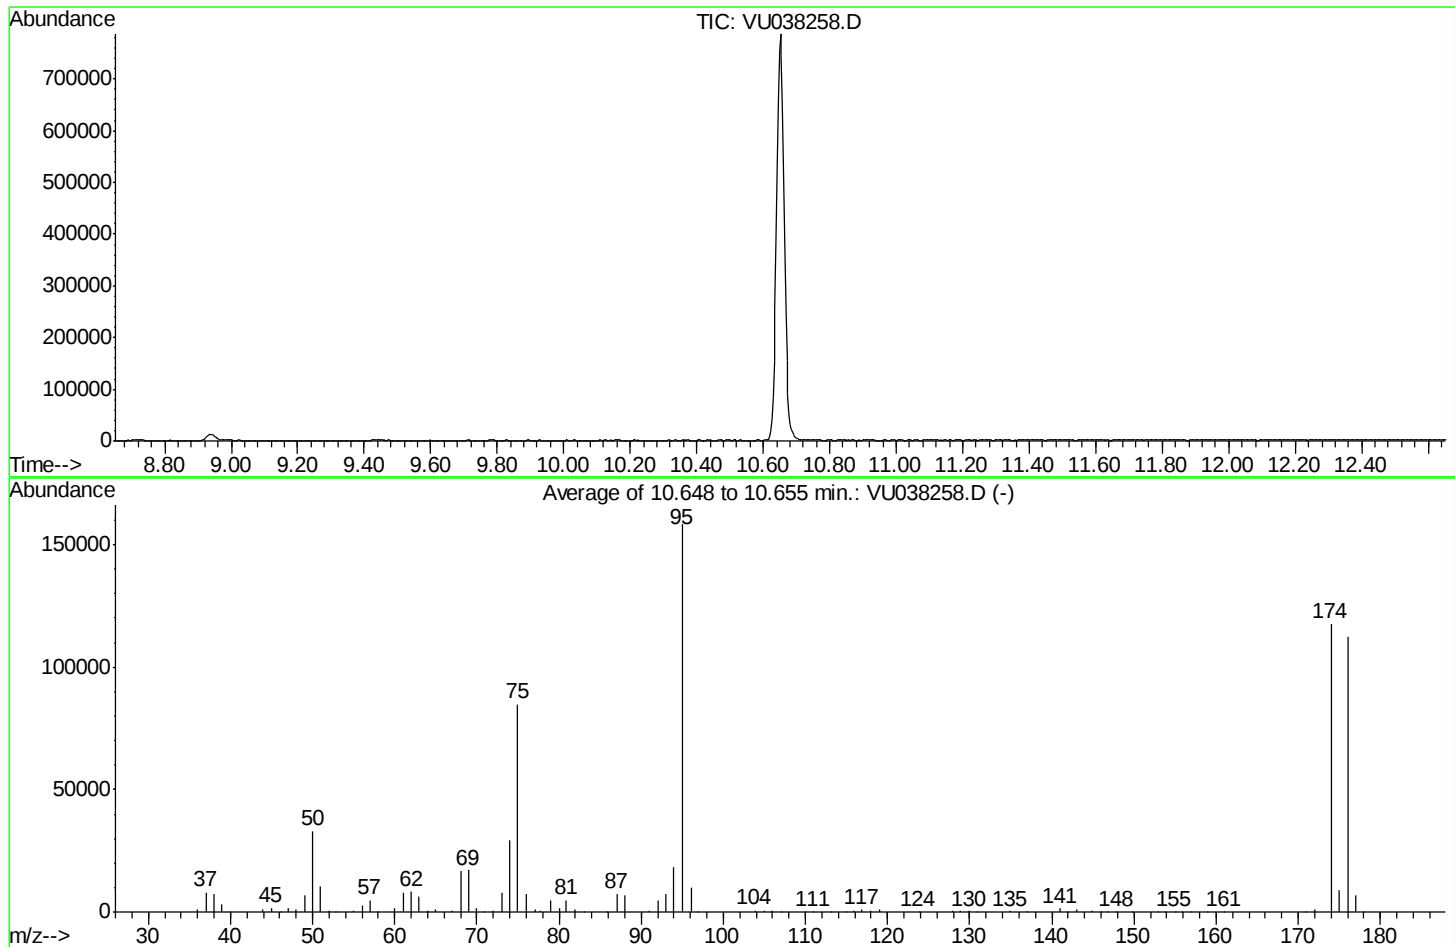

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	33074	PASS
75	95	30	80	53.5	84714	PASS
95	95	100	100	100.0	158314	PASS
96	95	5	9	6.2	9802	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.3	117632	PASS
175	174	5	9	7.4	8723	PASS
176	174	95	101	95.6	112458	PASS
177	176	5	9	6.2	7008	PASS

m/z	Abundance
36.00	1275.0
37.00	7938.0
38.00	6982.0
39.00	3063.0
39.90	334.0
44.00	2142.0
45.00	1659.0
46.10	153.0
47.00	1726.0
47.90	1147.0
49.00	6743.0
50.00	33112.0
51.00	10259.0
52.00	438.0
52.80	132.0
54.90	435.0
56.00	2717.0
57.00	4753.0
57.90	174.0
60.00	1389.0
61.00	7835.0
62.00	8209.0
63.00	6424.0
64.00	491.0
65.00	818.0
67.00	549.0
68.00	17048.0
69.00	17472.0
70.00	1199.0
71.90	731.0
73.00	7994.0
74.00	29792.0
75.00	85184.0
76.00	7086.0
77.10	1011.0
77.80	609.0
78.90	4528.0
80.00	1502.0
80.90	4585.0
82.00	1257.0
83.00	135.0
85.80	175.0
87.00	7124.0
87.90	6767.0
90.90	627.0
92.00	4582.0
93.00	7340.0
94.00	18720.0
95.00	158336.0
96.00	9891.0
96.90	284.0
103.90	739.0
104.90	266.0
105.90	536.0
110.00	128.0
110.90	161.0
113.10	212.0
115.00	178.0
115.90	586.0
116.90	946.0
117.90	612.0
118.90	765.0
123.80	113.0
127.90	530.0
128.90	289.0
129.90	499.0
130.90	117.0
135.00	278.0
137.00	250.0
141.00	1363.0
141.90	152.0
143.00	1140.0
145.00	234.0
146.00	254.0
147.90	262.0
149.70	117.0
152.90	119.0
153.80	109.0
154.90	248.0
155.80	119.0
156.90	220.0
158.80	134.0
161.00	112.0
170.90	152.0
172.00	1054.0
174.00	114024.0
175.00	8627.0
176.00	109424.0
177.00	7094.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

m/z	Abundance
36.00	1289.0
37.00	8037.0
38.00	7527.0
39.00	2992.0
39.90	373.0
44.00	2150.0
45.00	1712.0
46.00	105.0
47.00	1684.0
47.90	1222.0
49.00	6960.0
50.00	34296.0
51.00	10606.0
52.00	352.0
52.80	132.0
54.90	482.0
56.00	2683.0
57.00	4952.0
57.90	134.0
59.90	1428.0
61.00	8297.0
62.00	8459.0
63.00	6653.0
64.00	555.0
65.00	880.0
67.00	493.0
68.00	17312.0
69.00	17800.0
70.00	1410.0
70.90	165.0
71.90	755.0
73.00	8377.0
74.00	30392.0
75.00	87440.0
76.00	7439.0
77.00	1238.0
77.80	756.0
78.90	4692.0
80.00	1542.0
80.90	4910.0
82.00	1246.0
82.90	163.0
85.90	255.0
87.00	7674.0
88.00	6913.0
91.00	558.0
92.00	4707.0
93.00	7370.0
94.00	19184.0
95.00	163072.0
96.00	10013.0
96.90	288.0
103.90	768.0
105.00	313.0
105.90	609.0
107.00	124.0
110.00	141.0
111.00	136.0
113.00	221.0
115.00	155.0
115.90	529.0
116.90	965.0
117.90	637.0
119.00	867.0
127.90	557.0
128.90	292.0
130.00	545.0
130.90	130.0
134.90	295.0
136.90	193.0
141.00	1399.0
141.90	192.0
143.00	1278.0
145.00	292.0
146.00	264.0
146.70	119.0
147.90	297.0
149.70	124.0
152.90	139.0
153.80	135.0
154.90	264.0
155.90	149.0
156.90	256.0
158.90	178.0
161.00	123.0
170.90	188.0
172.00	889.0
174.00	121176.0
175.00	8906.0
176.00	115952.0
177.00	7155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

m/z	Abundance
36.00	1184.0
37.00	7653.0
38.00	7284.0
39.00	2740.0
39.90	400.0
44.00	2042.0
45.00	1492.0
47.00	1566.0
47.90	1031.0
49.00	6710.0
50.00	31816.0
51.00	9893.0
51.90	280.0
55.00	477.0
56.00	2325.0
57.00	4814.0
59.90	1429.0
61.00	8097.0
62.00	7924.0
63.00	5991.0
63.90	616.0
65.00	829.0
67.00	433.0
68.00	16424.0
69.00	16357.0
70.00	1435.0
70.90	181.0
71.90	780.0
73.00	7737.0
74.00	28008.0
75.00	81520.0
76.00	7086.0
77.00	1314.0
77.80	830.0
78.90	4373.0
80.00	1404.0
80.90	4716.0
82.00	1138.0
82.90	179.0
85.90	328.0
87.00	7372.0
88.00	6570.0
90.90	522.0
92.00	4432.0
93.00	6920.0
94.00	17784.0
95.00	153536.0
96.10	9502.0
97.00	265.0
103.90	745.0
105.00	286.0
105.90	606.0
107.00	141.0
110.00	103.0
111.00	106.0
113.00	195.0
114.90	102.0
115.90	422.0
116.90	853.0
117.90	543.0
119.00	846.0
128.00	475.0
128.90	262.0
130.00	531.0
130.90	143.0
134.90	284.0
136.90	211.0
141.00	1253.0
141.90	201.0
143.00	1322.0
144.90	317.0
146.00	256.0
146.70	123.0
147.90	277.0
152.90	126.0
153.80	127.0
155.00	315.0
155.90	145.0
157.00	279.0
158.90	177.0
170.90	173.0
172.00	719.0
174.00	117696.0
175.00	8637.0
176.00	112000.0
177.00	6776.0
177.90	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

Scan 2881 (10.603 min): VU038258.D
BFB28

m/z	Abundance
39.90	245.0
43.90	1191.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28