

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052121\
 Data File : VU043889.D
 Acq On : 21 May 2021 15:10
 Operator : SY/MD
 Sample : M2475-02DL 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB401DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043889.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	73	82	96	rVB	77504	87917	11.31%	1.350%
2	1.919	172	180	191	rVB	57953	73241	9.42%	1.124%
3	2.575	370	384	400	rBV	134719	222104	28.57%	3.409%
4	3.054	523	533	547	rBV	10764	20026	2.58%	0.307%
5	3.192	563	576	595	rBV	8513	19423	2.50%	0.298%
6	4.645	1012	1028	1053	rBV2	93817	311402	40.06%	4.780%
7	5.073	1144	1161	1186	rBV	129560	286823	36.90%	4.403%
8	5.327	1223	1240	1264	rBV	221848	501811	64.56%	7.703%
9	5.735	1341	1367	1398	rBV2	255947	668521	86.00%	10.262%
10	6.256	1511	1529	1552	rBV	243647	467260	60.11%	7.172%
11	6.700	1653	1667	1692	rBV	162214	314470	40.46%	4.827%
12	7.575	1925	1939	1956	rBV	74431	131630	16.93%	2.020%
13	7.906	2029	2042	2058	rBV	286687	503817	64.81%	7.733%
14	8.185	2115	2129	2146	rBV	47300	81980	10.55%	1.258%
15	8.558	2234	2245	2259	rBV	112830	189720	24.41%	2.912%
16	8.645	2259	2272	2316	rVV	355897	777321	100.00%	11.932%
17	9.423	2498	2514	2538	rBV	359700	602831	77.55%	9.253%
18	10.764	2919	2931	2949	rVB	137720	224188	28.84%	3.441%
19	10.899	2959	2973	2987	rVB	7707	12383	1.59%	0.190%
20	11.819	3246	3259	3278	rBV	339007	538554	69.28%	8.267%
21	12.201	3364	3378	3394	rBV	296854	479358	61.67%	7.358%




Sum of corrected areas: 6514780

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052121\
Data File : VU043889.D
Acq On : 21 May 2021 15:10
Operator : SY/MD
Sample : M2475-02DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB401DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

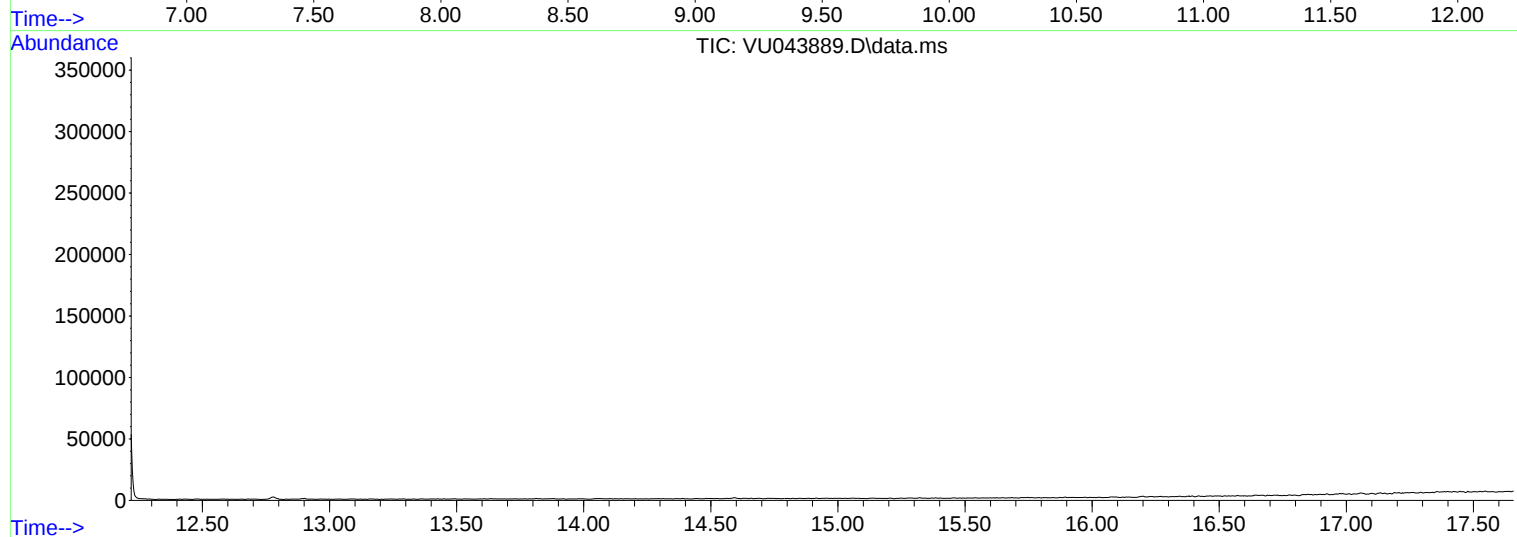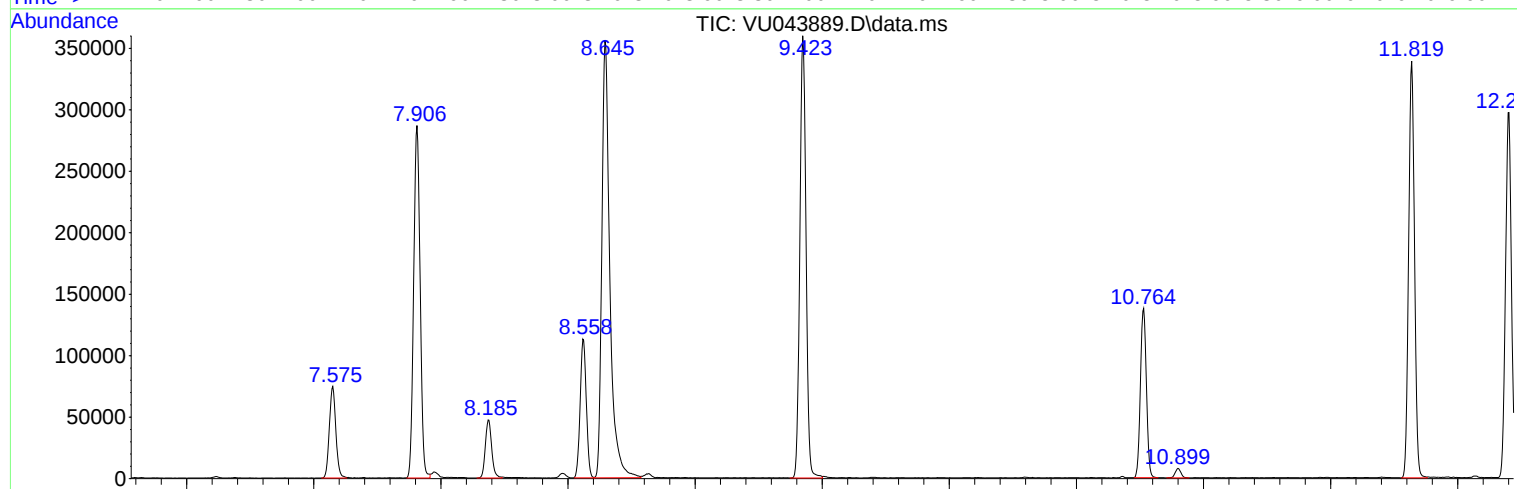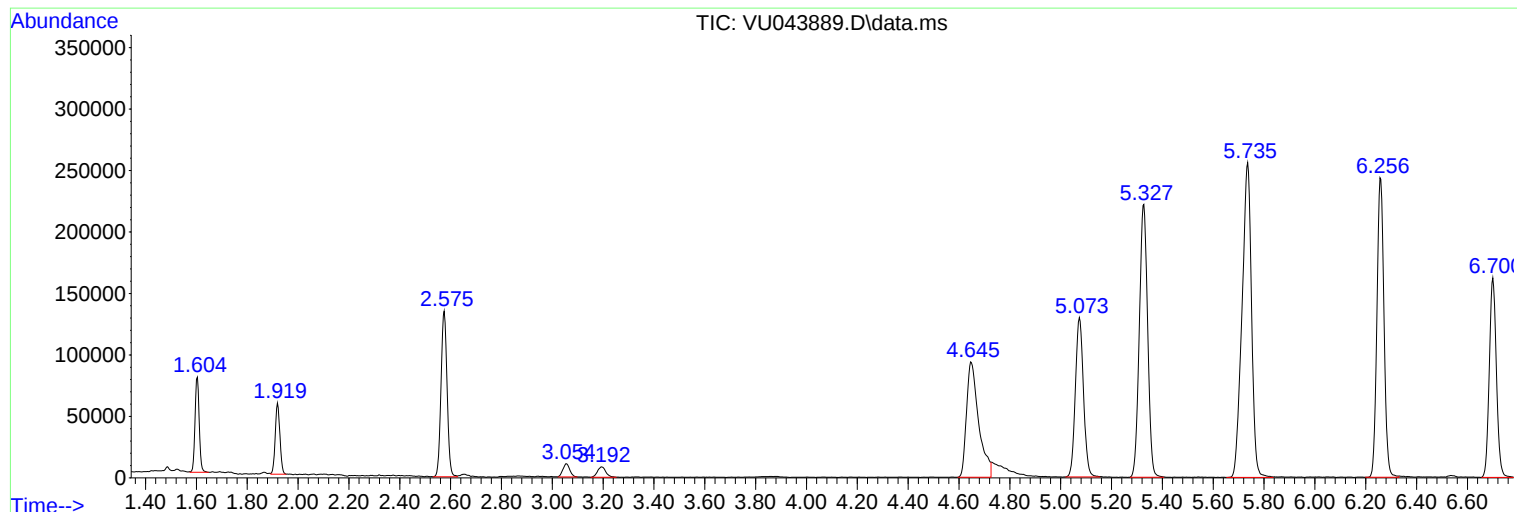

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052121\
Data File : VU043889.D
Acq On : 21 May 2021 15:10
Operator : SY/MD
Sample : M2475-02DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB401DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052121\
Data File : VU043889.D
Acq On : 21 May 2021 15:10
Operator : SY/MD
Sample : M2475-02DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB401DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
