

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052121\
 Data File : VU043901.D
 Acq On : 21 May 2021 19:58
 Operator : SY/MD
 Sample : M2459-01DL 2500X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0GJ7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043901.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	92	rBV	71756	81795	10.76%	1.283%
2	1.919	171	180	191	rBV	53778	66526	8.75%	1.044%
3	2.572	371	383	399	rBV	134247	218220	28.71%	3.423%
4	3.054	523	533	552	rVB2	8625	15871	2.09%	0.249%
5	3.192	563	576	592	rVB2	10716	23564	3.10%	0.370%
6	4.649	1009	1029	1062	rBV3	77871	278007	36.57%	4.361%
7	5.073	1145	1161	1184	rVB	124481	274971	36.17%	4.314%
8	5.735	1346	1367	1391	rBV2	244022	637503	83.87%	10.001%
9	6.256	1515	1529	1555	rBV	241396	462220	60.81%	7.251%
10	6.549	1605	1620	1640	rBV	401614	760142	100.00%	11.925%
11	6.700	1652	1667	1690	rBV	158058	304314	40.03%	4.774%
12	7.575	1925	1939	1966	rBV2	71176	127268	16.74%	1.997%
13	7.906	2028	2042	2058	rBV	280980	489384	64.38%	7.677%
14	8.186	2117	2129	2151	rBV2	44311	77972	10.26%	1.223%
15	8.645	2256	2272	2310	rBV	320277	748686	98.49%	11.745%
16	8.928	2349	2360	2378	rBV3	8216	17242	2.27%	0.270%
17	9.423	2501	2514	2551	rVB	350497	594634	78.23%	9.329%
18	10.764	2916	2931	2950	rBV	132790	216906	28.53%	3.403%
19	11.819	3244	3259	3274	rBV	329900	522280	68.71%	8.194%
20	12.198	3365	3377	3399	rBV	280029	456791	60.09%	7.166%




Sum of corrected areas: 6374296

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052121\
Data File : VU043901.D
Acq On : 21 May 2021 19:58
Operator : SY/MD
Sample : M2459-01DL 2500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GJ7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

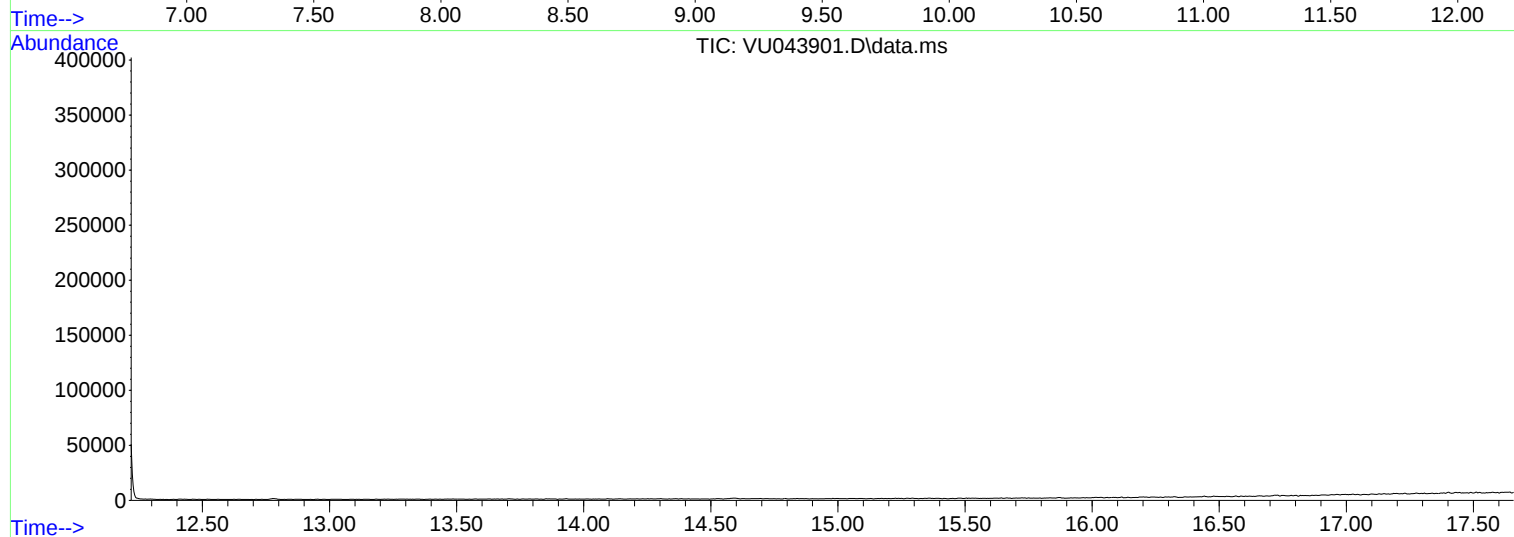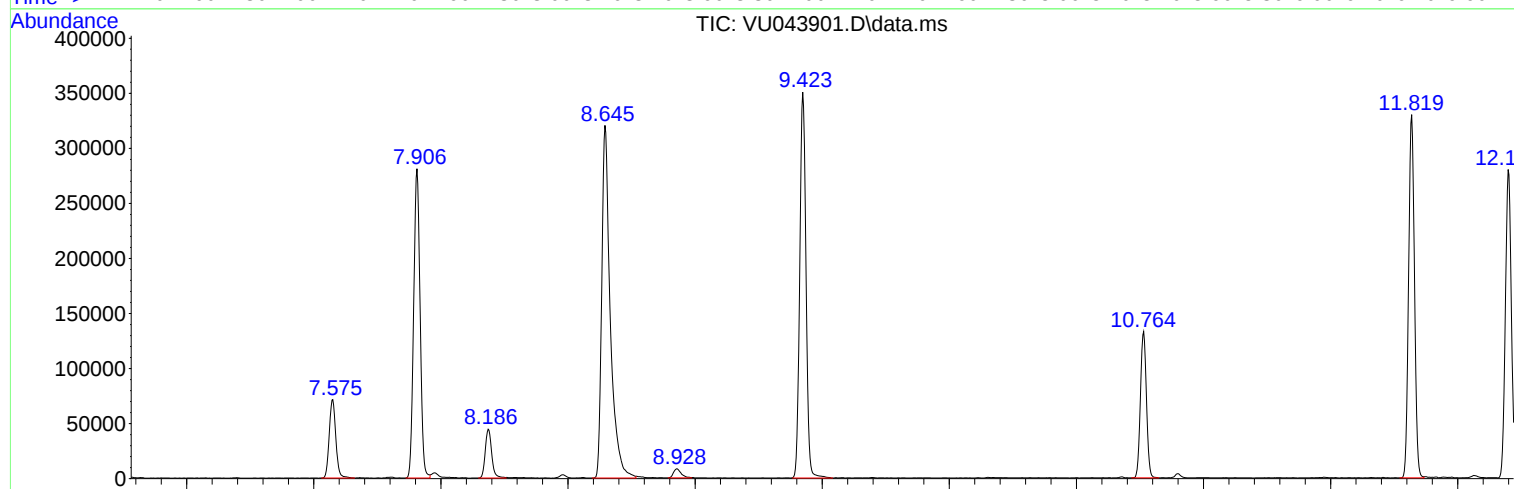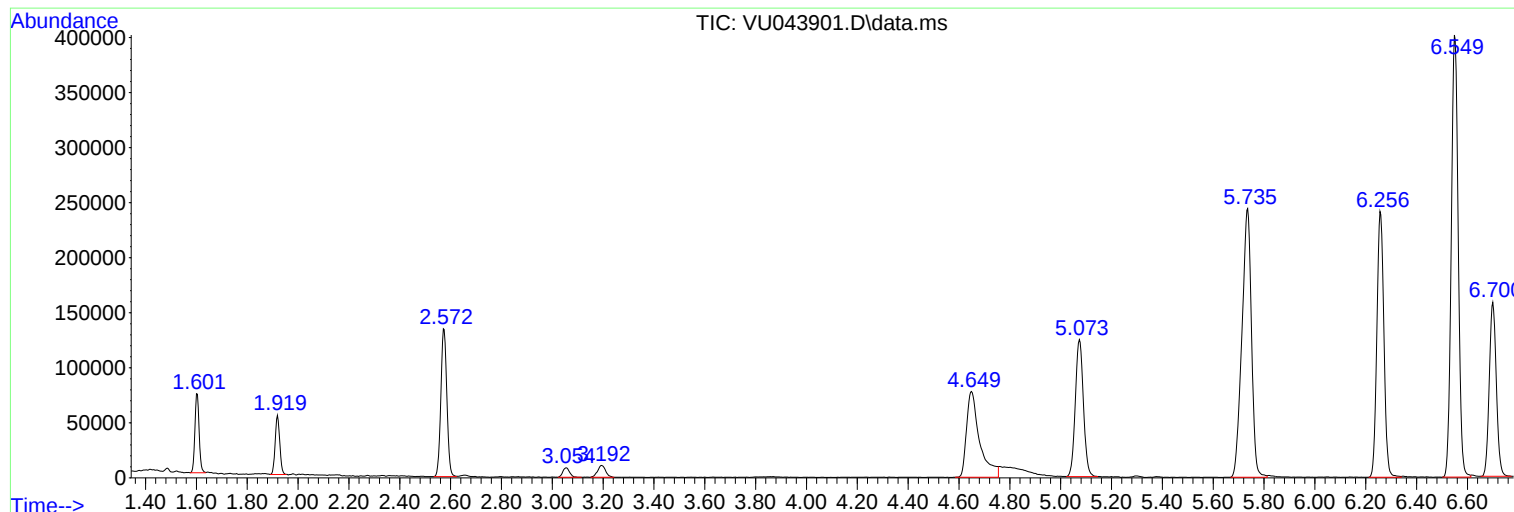

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052121\
Data File : VU043901.D
Acq On : 21 May 2021 19:58
Operator : SY/MD
Sample : M2459-01DL 2500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GJ7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052121\
Data File : VU043901.D
Acq On : 21 May 2021 19:58
Operator : SY/MD
Sample : M2459-01DL 2500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GJ7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
