
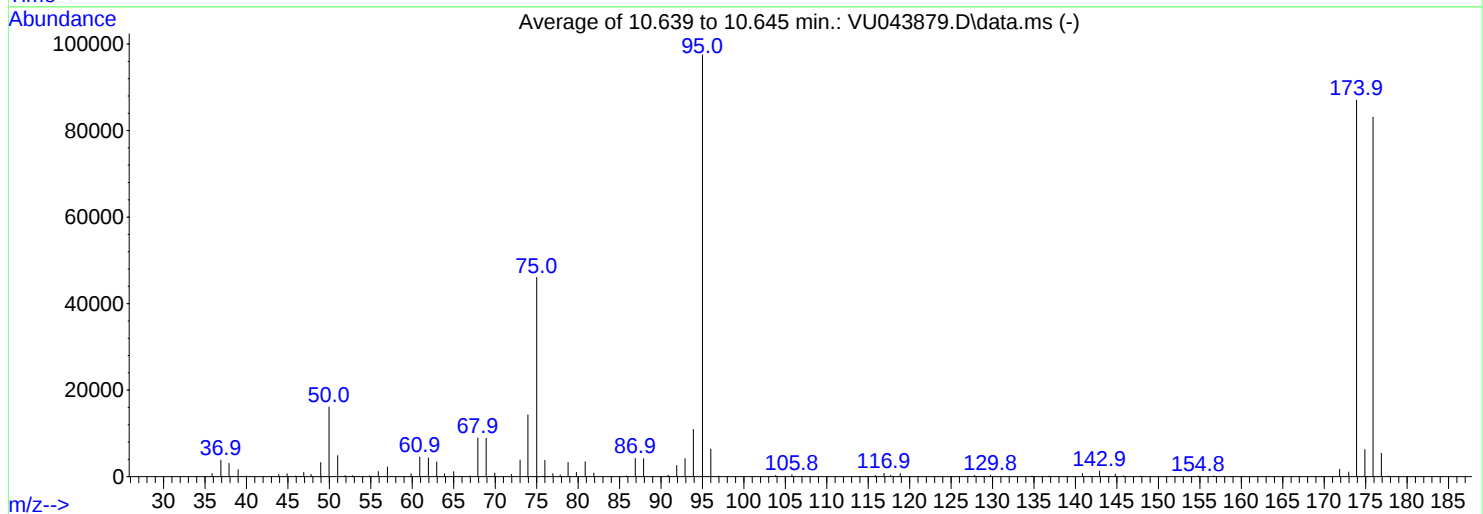


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052121\
Data File : VU043879.D
Acq On : 21 May 2021 09:27
Operator : SY/MD
Sample : BFB49
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB149

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat May 22 04:43:09 2021

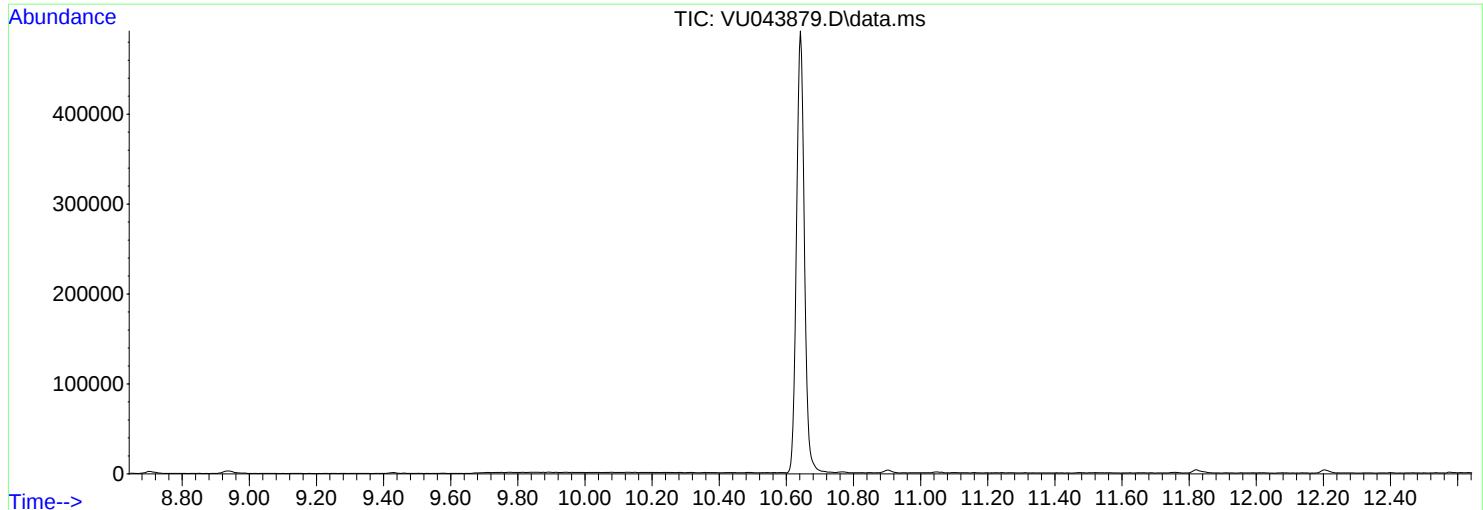

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.5	16091	PASS
75	95	30	80	47.2	46032	PASS
95	95	100	100	100.0	97507	PASS
96	95	5	9	6.5	6375	PASS
173	174	0.00	2	1.2	1083	PASS
174	95	50	120	89.2	87019	PASS
175	174	5	9	7.2	6247	PASS
176	174	95	101	95.5	83115	PASS
177	176	5	9	6.5	5384	PASS

m/z	Abundance
35.90	588.0
37.80	276.0
39.90	146.0
43.90	342.0

Instrument :
MSVOA_U
ClientSampleId :
BFB149

m/z	Abundance
35.90	1254.0
36.90	3774.0
38.00	3603.0
39.00	1630.0
39.80	212.0
43.90	726.0
44.90	660.0
45.90	148.0
46.90	1004.0
47.80	529.0
48.90	3291.0
49.90	16488.0
51.00	4869.0
51.90	305.0
52.80	203.0
54.80	235.0
55.90	1216.0
57.00	2377.0
59.80	681.0
60.90	4633.0
61.90	4340.0
62.90	3564.0
63.90	715.0
65.00	1083.0
65.90	124.0
67.00	238.0
67.90	8906.0
68.90	8921.0
70.00	826.0
72.00	450.0
73.00	4082.0
74.00	14216.0
75.00	45744.0
76.00	3852.0
76.90	652.0
77.80	403.0
78.80	3140.0
79.80	993.0
80.90	3459.0
81.90	870.0
85.90	167.0
86.90	4206.0
87.90	4304.0
90.80	321.0
91.90	2621.0
92.90	4063.0
93.90	10850.0
95.00	97152.0
96.00	6639.0
96.90	135.0
103.90	328.0
104.90	105.0
105.80	414.0
115.80	292.0
116.90	733.0
117.70	320.0
118.90	717.0
127.80	309.0
128.80	137.0
129.80	329.0
134.80	158.0
136.70	106.0
140.90	677.0
141.90	116.0
142.90	1303.0
143.80	101.0
144.80	620.0
145.80	199.0
147.80	124.0
154.80	212.0
156.70	156.0
170.80	235.0
171.90	1663.0
173.00	1031.0
173.90	84080.0
174.90	6143.0
175.90	80856.0
176.90	5264.0
177.80	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB149

m/z	Abundance
35.90	1330.0
36.90	3982.0
37.90	3426.0
39.00	1717.0
40.00	239.0
43.90	797.0
44.90	692.0
45.90	142.0
46.90	1028.0
47.80	556.0
49.00	3382.0
50.00	16512.0
51.00	4979.0
51.90	254.0
52.80	224.0
54.80	245.0
55.90	1237.0
57.00	2296.0
59.90	670.0
60.90	4674.0
62.00	4468.0
63.00	3471.0
63.90	707.0
65.00	1147.0
65.70	109.0
66.90	198.0
67.90	9319.0
68.90	9156.0
70.00	900.0
71.90	523.0
73.00	4002.0
74.00	14685.0
75.00	47520.0
76.00	3915.0
77.00	737.0
77.90	438.0
78.80	3400.0
79.80	1051.0
80.90	3568.0
81.90	864.0
85.80	177.0
86.90	4307.0
87.90	4336.0
90.90	386.0
91.90	2664.0
92.90	4350.0
93.90	11308.0
95.00	100832.0
96.00	6567.0
97.00	144.0
103.90	307.0
104.90	113.0
105.80	464.0
114.70	101.0
115.80	274.0
116.90	769.0
117.70	327.0
118.90	741.0
127.80	327.0
128.90	123.0
129.70	335.0
134.70	157.0
136.80	134.0
140.80	761.0
141.90	130.0
142.90	1325.0
144.80	632.0
145.80	246.0
147.80	165.0
154.80	212.0
156.70	198.0
171.10	242.0
171.90	1765.0
173.00	1117.0
173.90	89824.0
174.90	6484.0
175.90	85824.0
176.90	5530.0
177.80	159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB149

m/z	Abundance
35.90	1301.0
36.90	3728.0
37.90	2987.0
39.00	1549.0
40.00	274.0
43.90	898.0
44.90	611.0
45.90	141.0
46.90	947.0
47.80	510.0
49.00	3128.0
50.00	15274.0
51.00	4635.0
51.90	180.0
52.80	207.0
54.90	203.0
55.90	1141.0
57.00	2024.0
59.90	689.0
60.90	4229.0
61.90	4157.0
62.90	3215.0
63.90	628.0
65.00	1198.0
65.70	105.0
66.90	179.0
67.90	8627.0
68.90	8563.0
69.90	801.0
71.90	592.0
73.00	3485.0
73.90	13975.0
75.00	44832.0
76.00	3523.0
77.00	683.0
77.80	392.0
78.80	3304.0
79.80	946.0
80.80	3335.0
81.90	787.0
85.80	207.0
86.90	4176.0
87.90	3902.0
90.90	383.0
91.90	2446.0
92.90	4145.0
93.90	10583.0
95.00	94536.0
96.00	5919.0
97.00	154.0
103.80	293.0
105.00	136.0
105.80	477.0
115.90	286.0
116.90	719.0
117.70	318.0
118.80	671.0
127.80	305.0
129.70	298.0
134.70	117.0
136.80	147.0
140.80	773.0
141.80	107.0
142.90	1287.0
143.80	100.0
144.80	637.0
145.80	239.0
147.80	184.0
154.80	197.0
156.70	213.0
158.80	114.0
171.80	1725.0
172.90	1100.0
173.90	87152.0
174.90	6113.0
175.90	82664.0
176.90	5359.0
177.80	153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB149