

Data File : VU032250.D
Acq On : 23 May 2019 03:29
Operator : JC/SP
Sample : K3001-05MSD
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YF0

Quant Time: May 23 04:03:23 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR052219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 23 03:43:40 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	375768	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	385501	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	154755	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	113504	5.38	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.60%
7) Chloroethane-d5	1.67	69	98009	4.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.60%
11) 1,1-Dichloroethene-d2	2.27	63	227388	5.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	117.00%
20) 2-Butanone-d5	4.19	46	238979	40.15	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.30%
24) Chloroform-d	4.64	84	214629	3.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.60%
26) 1,2-Dichloroethane-d4	5.31	65	106061	3.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.20%
32) Benzene-d6	5.33	84	455006	4.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.20%
36) 1,2-Dichloropropane-d6	6.32	67	134251	3.78	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	75.60%
41) Toluene-d8	7.56	98	386842	3.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.80%
43) trans-1,3-Dichloropropene-	7.85	79	46662	3.42	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.40%
46) 2-Hexanone-d5	8.31	63	205630	40.01	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.02%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	105901	3.00	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	60.00%#
64) 1,2-Dichlorobenzene-d4	11.86	152	139423	3.27	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	65.40%#

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.30	85	3031	0.189	ug/L	96
3) Chloromethane	1.33	50	4543	0.282	ug/L	96
9) Trichlorofluoromethane	1.88	101	6290	0.298	ug/L	86
10) 1,1,2-Trichloro-1,2,2-trif	2.27	101	1922	0.144	ug/L #	19
12) 1,1-Dichloroethene	2.28	96	130164	9.734	ug/L	77
13) Acetone	2.32	43	12693	6.882	ug/L	98
15) Methyl Acetate	2.61	43	1053	0.195	ug/L #	47
18) trans-1,2-Dichloroethene	2.97	96	4825	0.336	ug/L	86
19) 1,1-Dichloroethane	3.44	63	159860	7.211	ug/L	99
22) cis-1,2-Dichloroethene	4.22	96	24196	1.727	ug/L	95
25) Chloroform	4.67	83	19593	0.818	ug/L	85
27) 1,2-Dichloroethane	5.39	62	4239	0.304	ug/L #	73
29) 1,1,1-Trichloroethane	4.91	97	128765	6.435	ug/L	99
31) Carbon tetrachloride	4.91	117	17015	0.965	ug/L	96
33) Benzene	5.38	78	502051	9.628	ug/L	100
34) Trichloroethene	6.18	95	156207	11.161	ug/L	96
35) Methylcyclohexane	6.32	83	31552	1.531	ug/L #	20

Data File : VU032250.D
Acq On : 23 May 2019 03:29
Operator : JC/SP
Sample : K3001-05MSD
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YF0

Quant Time: May 23 04:03:23 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR052219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 23 03:43:40 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1,2-Dichloropropane	6.32	63	14140	1.126	ug/L #	87
38) Bromodichloromethane	6.76	83	5313	0.326	ug/L	96
39) cis-1,3-Dichloropropene	7.22	75	3194	0.179	ug/L	84
42) Toluene	7.63	91	536168	9.677	ug/L	98
44) trans-1,3-Dichloropropene	7.85	75	1846	0.131	ug/L	94
47) Tetrachloroethene	8.22	164	8407	0.728	ug/L	96
48) 2-Hexanone	8.37	43	6876	1.413	ug/L #	74
49) Dibromochloromethane	8.48	129	901	0.082	ug/L	83
51) Chlorobenzene	9.12	112	357963	10.094	ug/L	98
52) Ethylbenzene	9.25	91	8815	0.158	ug/L	89
53) m,p-Xylene	9.37	106	15594	0.752	ug/L	97
54) o-Xylene	9.78	106	10014	0.483	ug/L	72
59) 1,2,3-Trichloropropane	11.48	75	14950	1.828	ug/L #	39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU032250.D
Acq On : 23 May 2019 03:29
Operator : JC/SP
Sample : K3001-05MSD
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YF0

Quant Time: May 23 04:03:23 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR052219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 23 03:43:40 2019
Response via : Initial Calibration

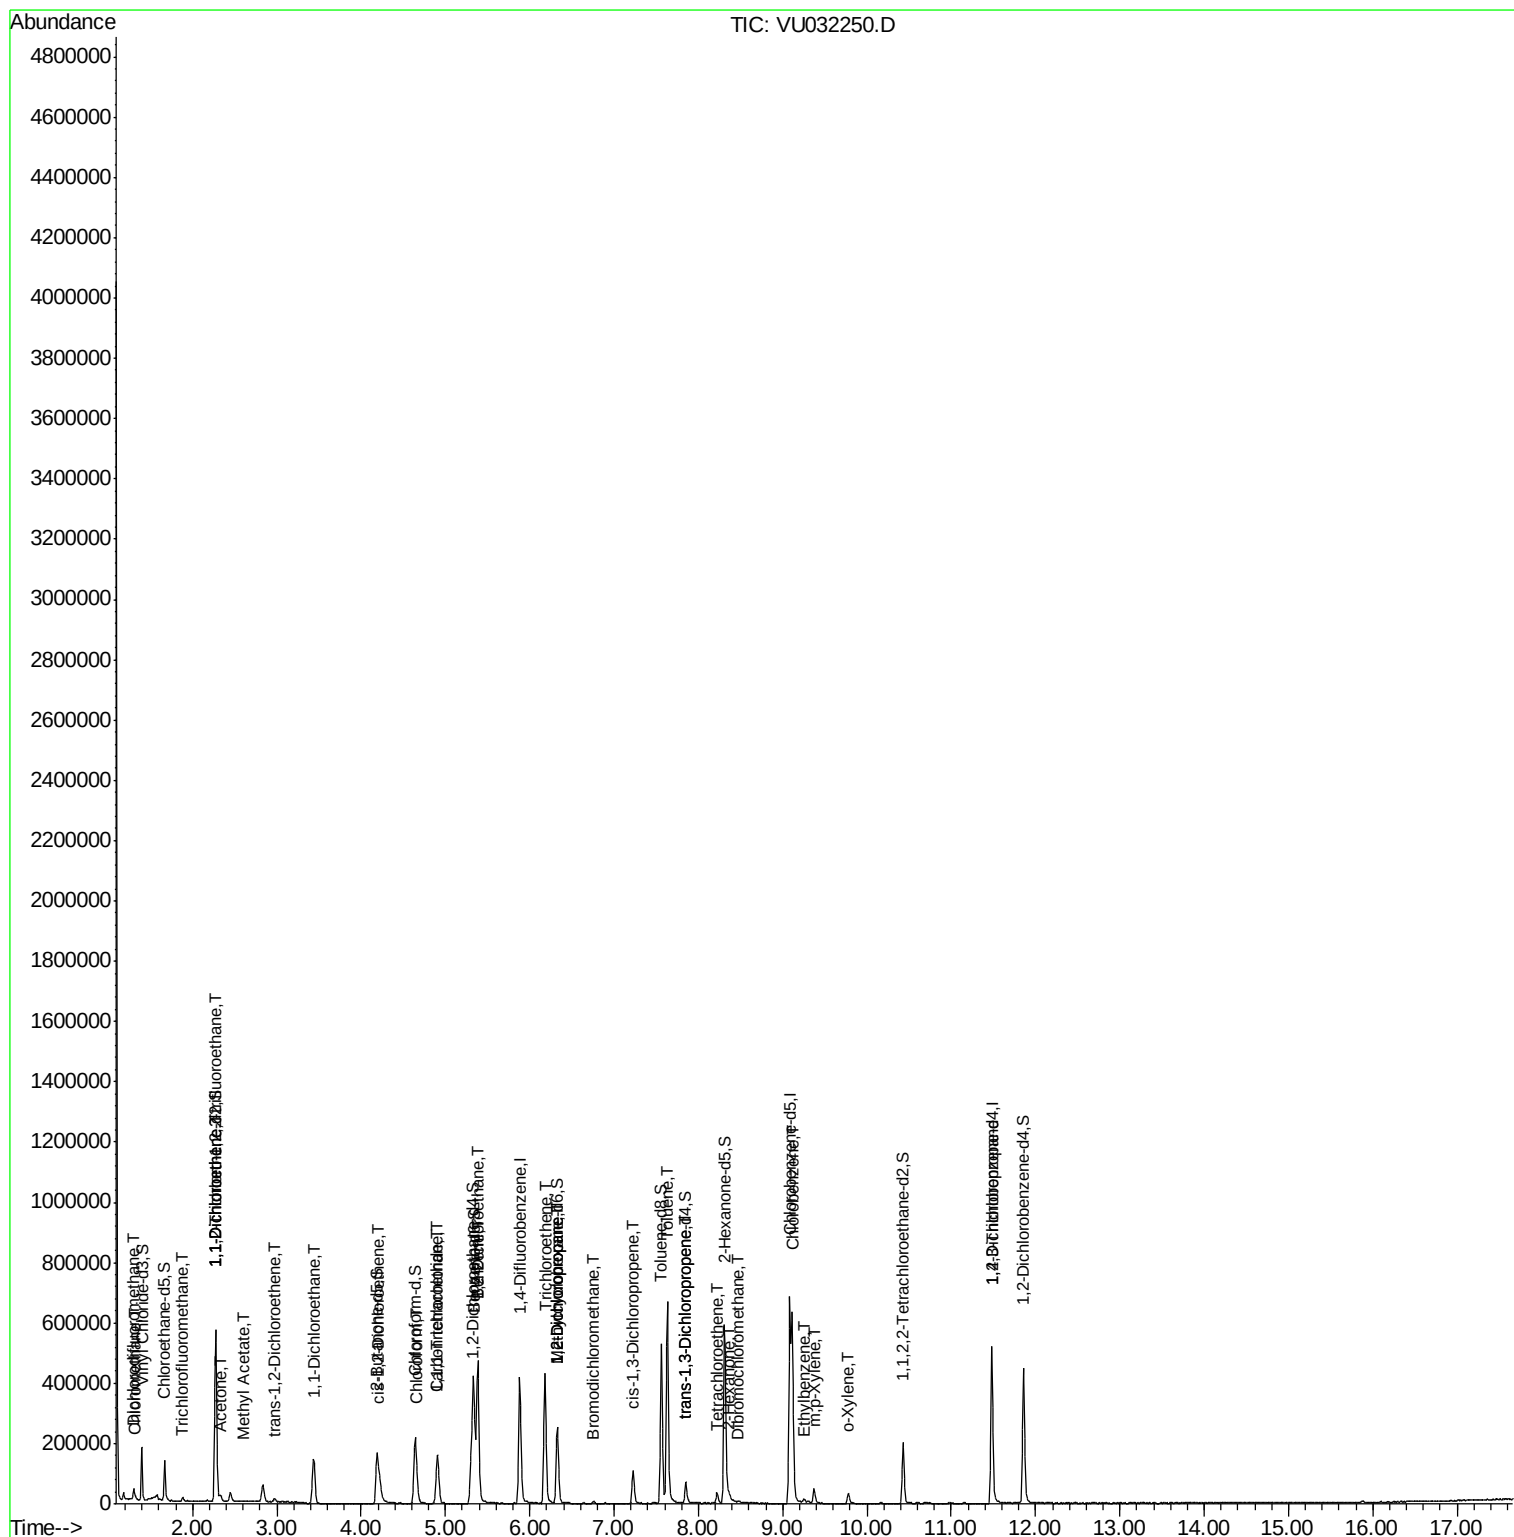

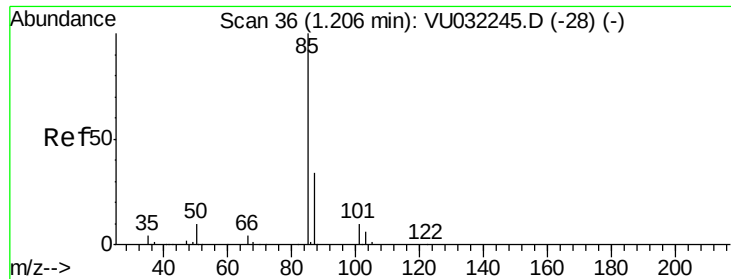

#2

Dichlorodifluoromethane

Concen: 0.189 ug/L

RT: 1.30 min Scan# 66

Delta R.T. 0.10 min

Lab File: VU032250.D

Acq: 23 May 2019 03:29

Instrument :

MSVOA_U

ClientSampleId :





E3YF0

Tgt Ion: 85 Resp: 3031

Ion Ratio Lower Upper

85 100

87 35.5 26.6 39.8

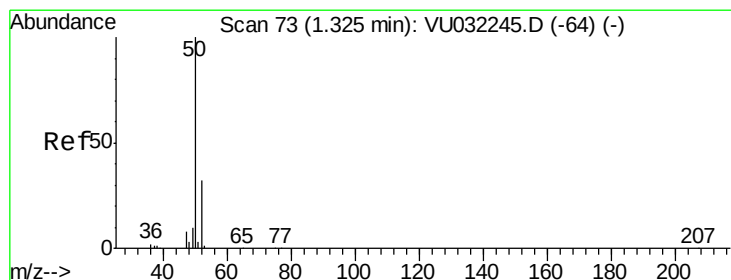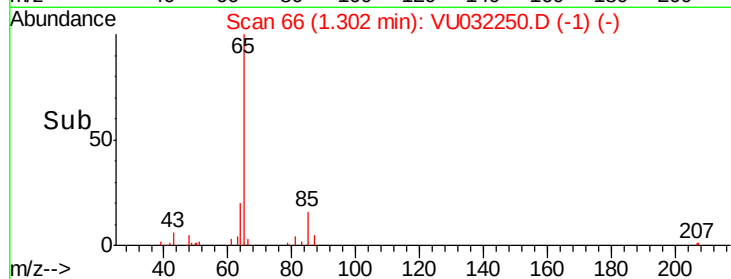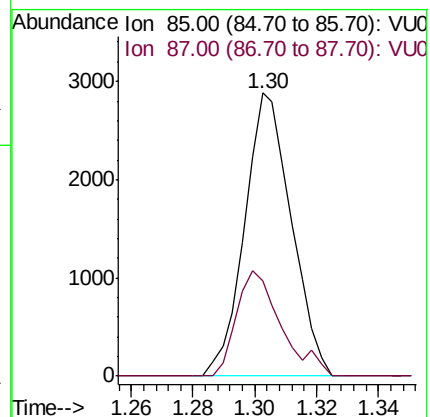

#3

Chloromethane

Concen: 0.282 ug/L

RT: 1.33 min Scan# 74

Delta R.T. 0.00 min

Lab File: VU032250.D




Acq: 23 May 2019 03:29


Tgt Ion: 50 Resp: 4543

Ion Ratio Lower Upper

50 100

52 31.0 23.3 43.3

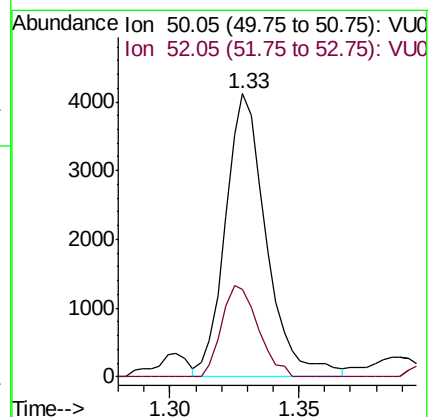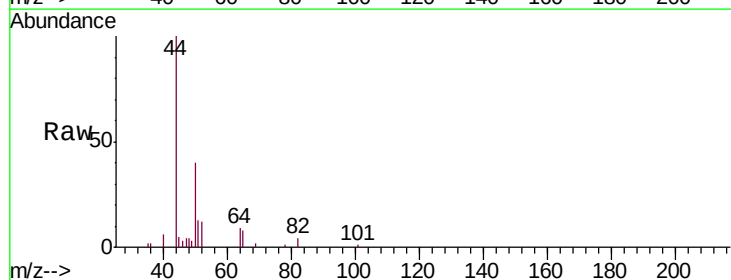



#9

Trichlorofluoromethane

Concen: 0.298 ug/L

RT: 1.88 min Scan# 246

Delta R.T. -0.00 min

Lab File: VU032250.D

Acq: 23 May 2019 03:29

Instrument :

MSVOA_U

ClientSampleId :


E3YF0

Tgt Ion:101 Resp: 6290

Ion Ratio Lower Upper




101 100

103 75.9 51.9 77.9

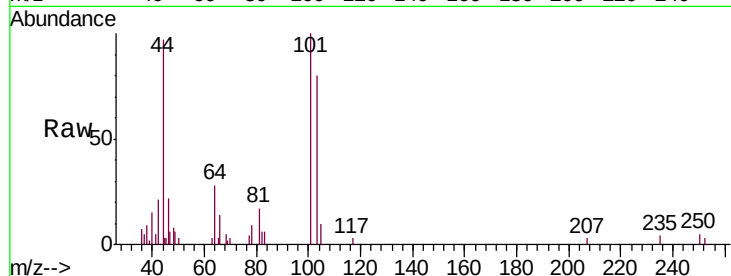

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 103.00 (102.70 to 103.70): V

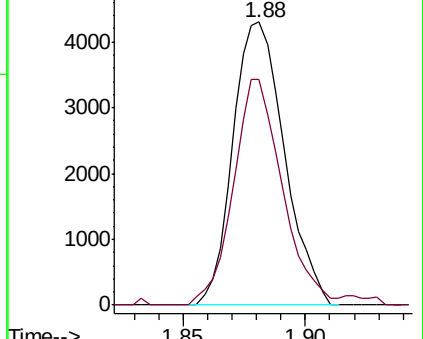

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.144 ug/L

RT: 2.27 min Scan# 367

Delta R.T. -0.02 min

Lab File: VU032250.D

Acq: 23 May 2019 03:29


Tgt Ion:101 Resp: 1922

Ion Ratio Lower Upper

101 100

85 0.0 34.2 51.4#



151 2.2 64.4 96.6#




Abundance Ion 101.00 (100.70 to 101.70): V

Ion 85.00 (84.70 to 85.70): VU0

Ion 151.00 (150.70 to 151.70): V

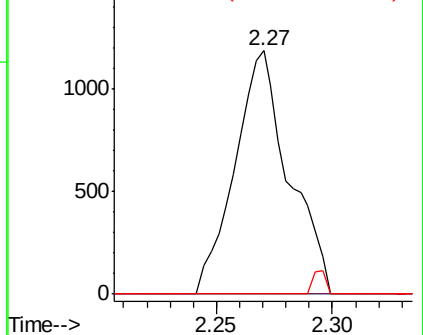



#12

1,1-Dichloroethene

Concen: 9.734 ug/L

RT: 2.28 min Scan# 370

Delta R.T. -0.00 min

Lab File: VU032250.D

Acq: 23 May 2019 03:29

Instrument :

MSVOA_U

ClientSampleId :

E3YF0


Tgt Ion: 96 Resp: 130164

Ion Ratio Lower Upper

96 100

61 148.3 113.8 211.3




63 110.1 108.8 202.2

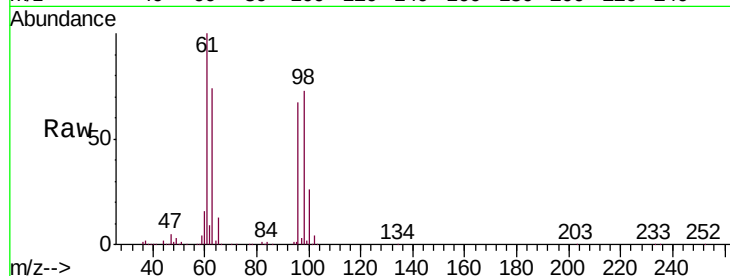

Abundance Ion 96.00 (95.70 to 96.70): VU032250.D (-278) (-)

Ion 61.05 (60.75 to 61.75): VU032250.D (-278) (-)

Ion 63.00 (62.70 to 63.70): VU032250.D (-278) (-)

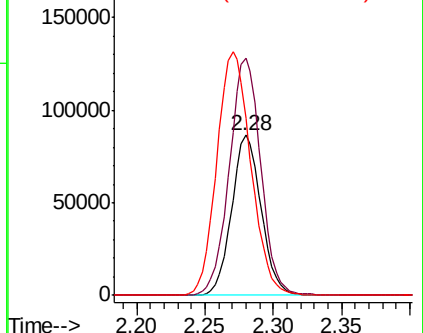

#13

Acetone

Concen: 6.882 ug/L

RT: 2.32 min Scan# 383

Delta R.T. -0.02 min

Lab File: VU032250.D


Acq: 23 May 2019 03:29

Tgt Ion: 43 Resp: 12693

Ion Ratio Lower Upper



43 100


58 37.3 0.0 72.6



Abundance Ion 43.05 (42.75 to 43.75): VU032250.D (-296) (-)

Ion 58.05 (57.75 to 58.75): VU032250.D (-296) (-)

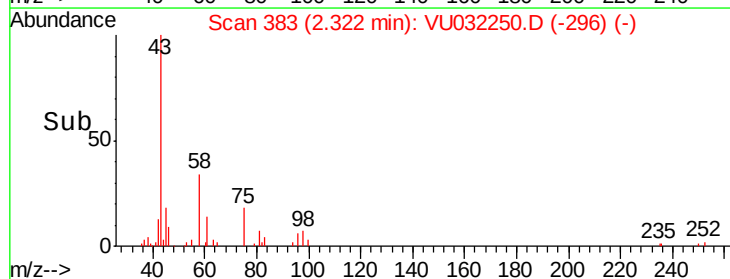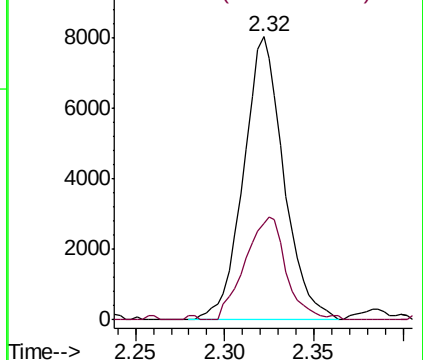



#15

Methyl Acetate

Concen: 0.195 ug/L

RT: 2.61 min Scan# 474

Delta R.T. -0.01 min

Lab File: VU032250.D

Acq: 23 May 2019 03:29

Instrument :

MSVOA_U

ClientSampleId :


E3YF0

Tgt Ion: 43 Resp: 1053




Ion Ratio Lower Upper

43 100

74 3.9 27.3 40.9#

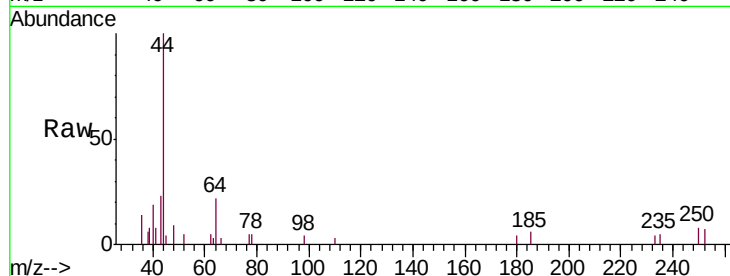

Abundance Ion 43.05 (42.75 to 43.75): VU032245.D (-460) (-)

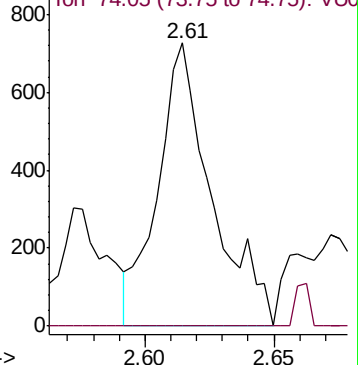

#18

trans-1,2-Dichloroethene

Concen: 0.336 ug/L

RT: 2.97 min Scan# 585

Delta R.T. -0.01 min

Lab File: VU032250.D

Acq: 23 May 2019 03:29


Tgt Ion: 96 Resp: 4825

Ion Ratio Lower Upper



96 100


61 110.4 90.6 168.3

98 63.8 49.5 91.9



Abundance Ion 96.00 (95.70 to 96.70): VU032245.D (-571) (-)




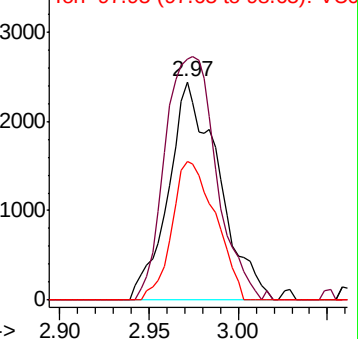


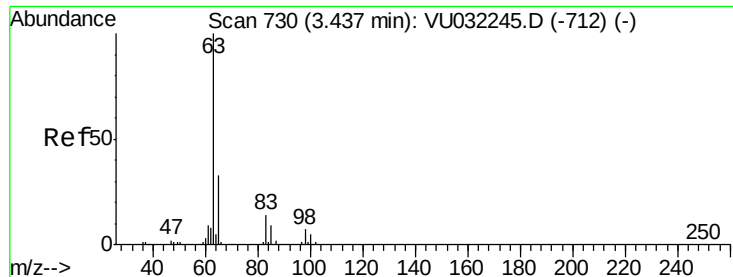

#19
 1,1-Dichloroethane
 Concen: 7.211 ug/L
 RT: 3.44 min Scan# 730
 Delta R.T. 0.00 min
 Lab File: VU032250.D
 Acq: 23 May 2019 03:29




Instrument :
 MSVOA_U
 ClientSampleId :
 E3YF0


Tgt Ion: 63 Resp: 159860
 Ion Ratio Lower Upper
 63 100
 65 33.8 23.5 43.7
 83 13.7 8.8 16.3

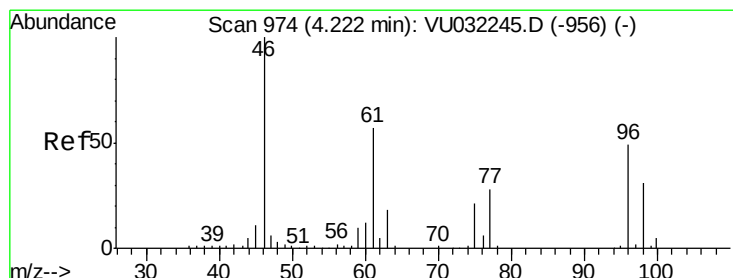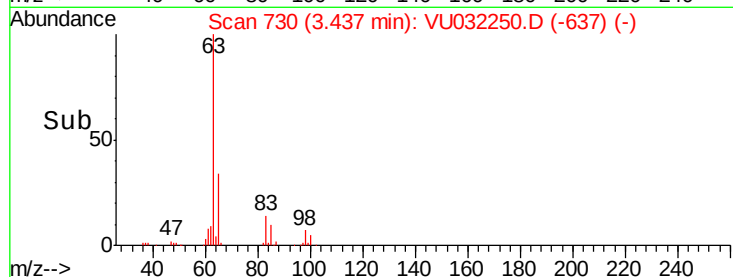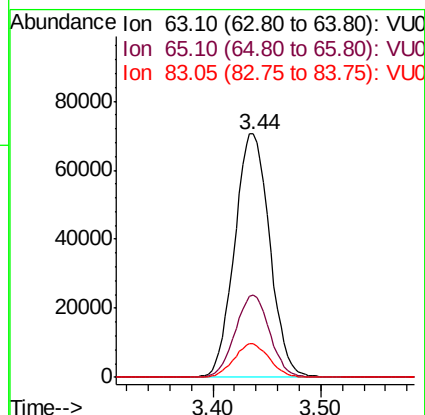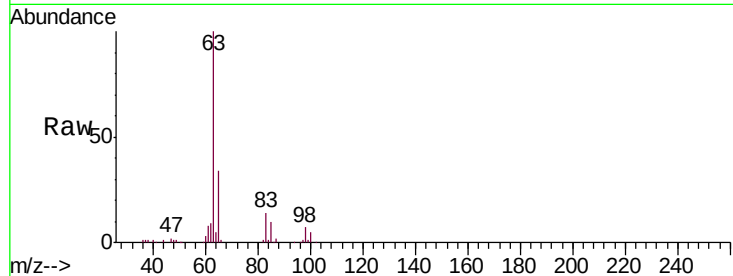

#22
 cis-1,2-Dichloroethene
 Concen: 1.727 ug/L
 RT: 4.22 min Scan# 972
 Delta R.T. -0.01 min
 Lab File: VU032250.D
 Acq: 23 May 2019 03:29

Tgt Ion: 96 Resp: 24196
 Ion Ratio Lower Upper
 96 100
 61 112.2 82.5 153.1
 68 0.0 0.0 0.0


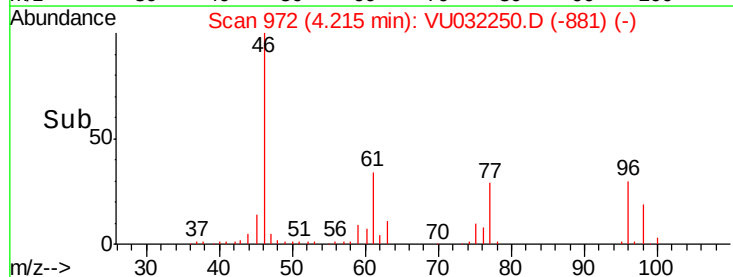
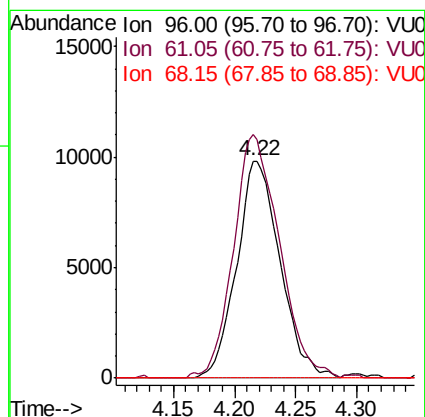
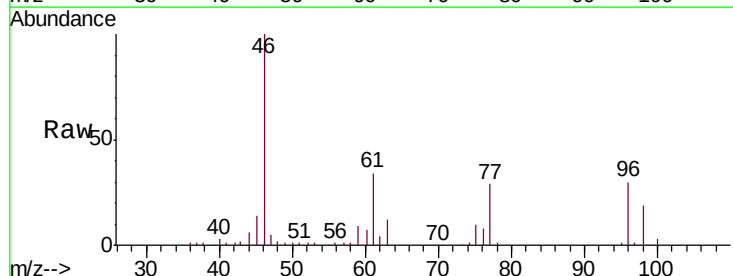


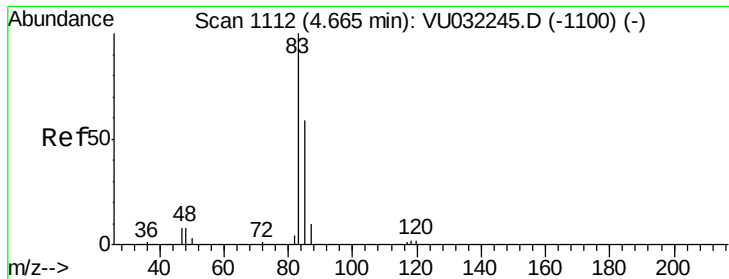

#25
Chloroform
Concen: 0.818 ug/L
RT: 4.67 min Scan# 1113
Delta R.T. 0.00 min
Lab File: VU032250.D
Acq: 23 May 2019 03:29




Instrument :
MSVOA_U
ClientSampleId :
E3YF0


Tgt Ion: 83 Resp: 19593
Ion Ratio Lower Upper
83 100
85 70.7 41.6 77.3

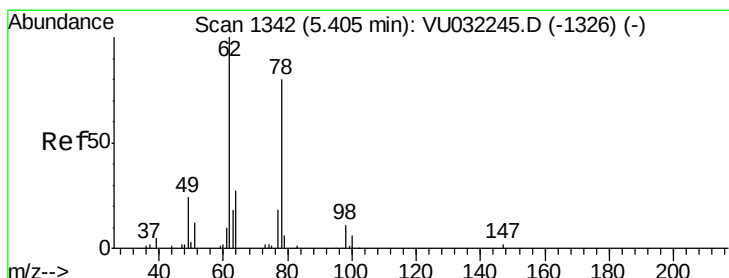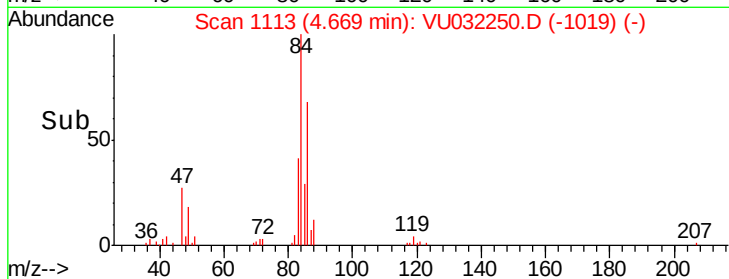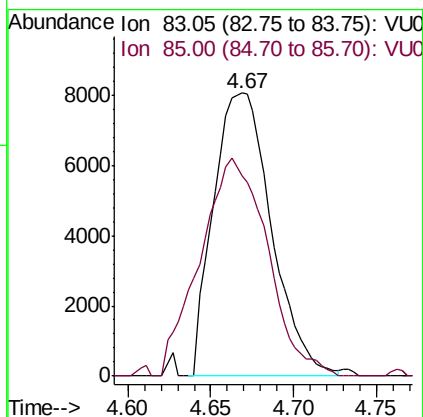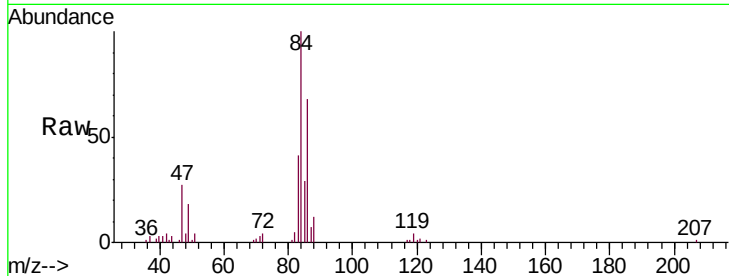

#27
1,2-Dichloroethane
Concen: 0.304 ug/L
RT: 5.39 min Scan# 1336
Delta R.T. -0.02 min
Lab File: VU032250.D
Acq: 23 May 2019 03:29

Tgt Ion: 62 Resp: 4239
Ion Ratio Lower Upper
62 100
98 0.0 8.2 12.2#

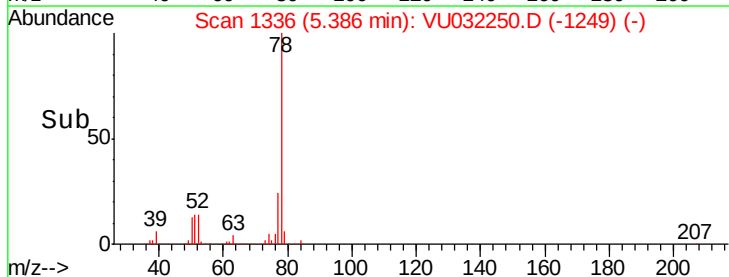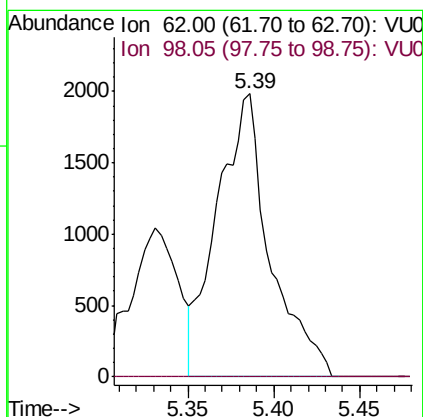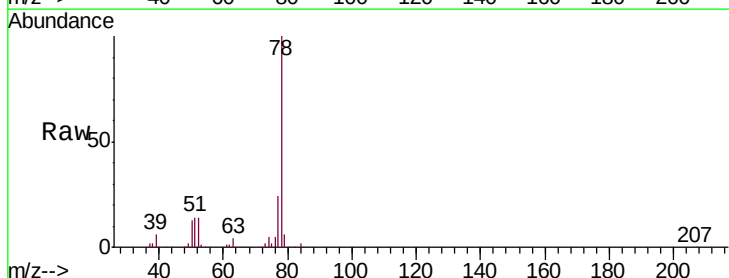

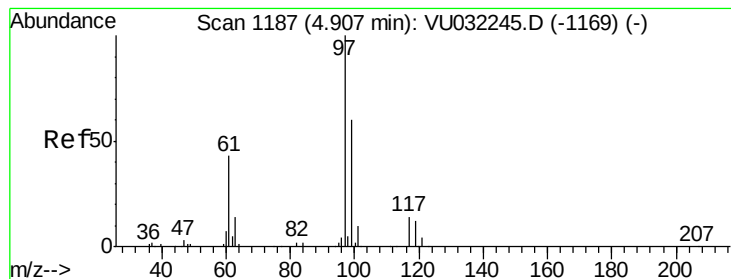

#29

1,1,1-Trichloroethane

Concen: 6.435 ug/L

RT: 4.91 min Scan# 1187

Delta R.T. 0.00 min

Lab File: VU032250.D

Acq: 23 May 2019 03:29

Instrument :

MSVOA_U

ClientSampleId :

E3YF0


Tgt Ion: 97 Resp: 128765

Ion Ratio Lower Upper

97 100

99 64.0 50.3 75.5




61 42.4 34.1 51.1



Abundance Ion 96.95 (96.65 to 97.65): VU032250.D (-1169) (-)

Ion 99.05 (98.75 to 99.75): VU032250.D (-1169) (-)

Ion 61.05 (60.75 to 61.75): VU032250.D (-1169) (-)

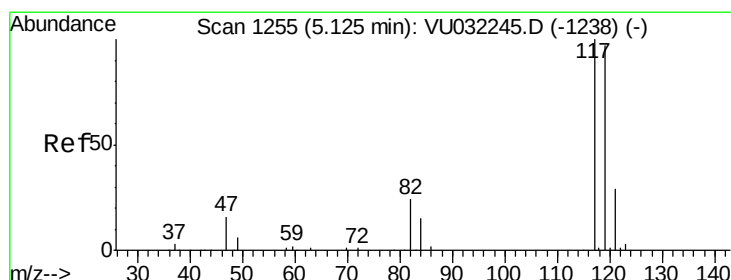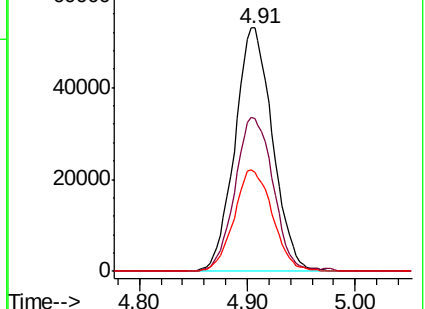

#31

Carbon tetrachloride

Concen: 0.965 ug/L

RT: 4.91 min Scan# 1187

Delta R.T. -0.22 min

Lab File: VU032250.D


Acq: 23 May 2019 03:29

Tgt Ion: 117 Resp: 17015

Ion Ratio Lower Upper



117 100


119 100.0 76.9 115.3

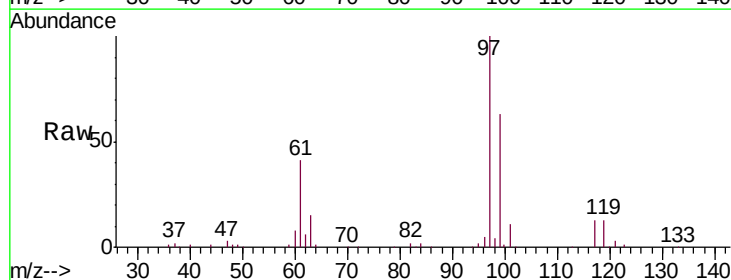

Abundance Ion 116.90 (116.60 to 117.60): VU032250.D (-1162) (-)

Ion 118.90 (118.60 to 119.60): VU032250.D (-1162) (-)

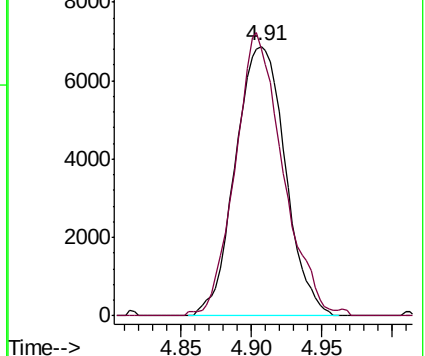



#33

Benzene

Concen: 9.628 ug/L

RT: 5.38 min Scan# 1335

Delta R.T. -0.00 min

Lab File: VU032250.D

Acq: 23 May 2019 03:29


Instrument :

MSVOA_U




ClientSampleId :

E3YF0

Tgt Ion: 78 Resp: 502051

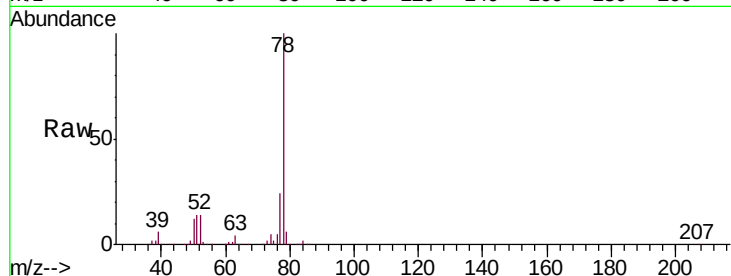

Abundance Ion 78.10 (77.80 to 78.80): VU0

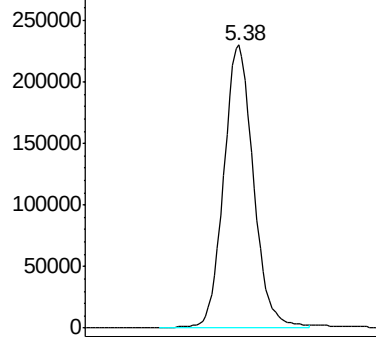

#34

Trichloroethene

Concen: 11.161 ug/L

RT: 6.18 min Scan# 1583


Delta R.T. 0.00 min

Lab File: VU032250.D

Acq: 23 May 2019 03:29

Tgt Ion: 95 Resp: 156207

Ion	Ratio	Lower	Upper
95	100		
97	63.1	39.9	74.1
132	97.8	65.9	122.5
130	99.2	70.6	131.2




Abundance Ion 95.00 (94.70 to 95.70): VU0


Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V




Time-->






#35
Methylcyclohexane
Concen: 1.531 ug/L
RT: 6.32 min Scan# 1628
Delta R.T. -0.08 min
Lab File: VU032250.D
Acq: 23 May 2019 03:29

Instrument :
MSVOA_U
ClientSampleId :
E3YF0

Tgt Ion: 83 Resp: 31552
Ion Ratio Lower Upper
83 100
55 0.1 59.7 89.5#
98 1.0 37.5 56.3#

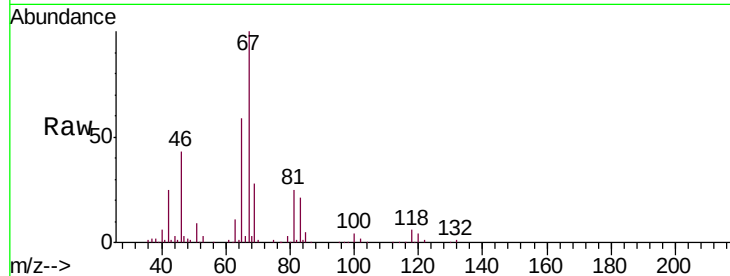


Abundance Ion 83.15 (82.85 to 83.85): VU0
Ion 55.10 (54.80 to 55.80): VU0
Ion 98.15 (97.85 to 98.85): VU0


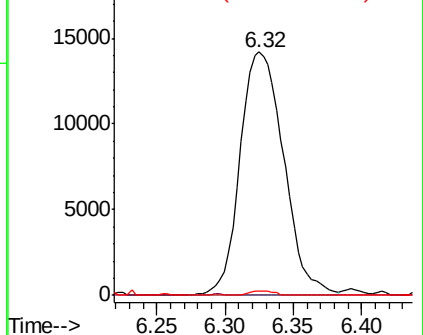



#37
1,2-Dichloropropane
Concen: 1.126 ug/L
RT: 6.32 min Scan# 1628
Delta R.T. -0.11 min
Lab File: VU032250.D
Acq: 23 May 2019 03:29

Tgt Ion: 63 Resp: 14140
Ion Ratio Lower Upper
63 100
112 0.6 3.8 5.8#



Abundance Ion 63.10 (62.80 to 63.80): VU0
Ion 112.10 (111.80 to 112.80): V

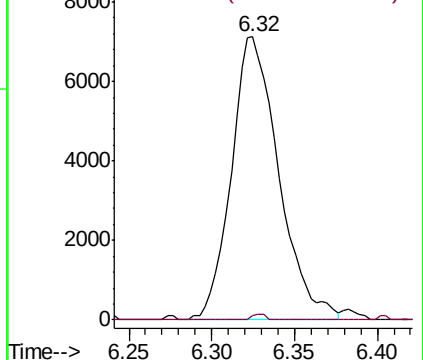

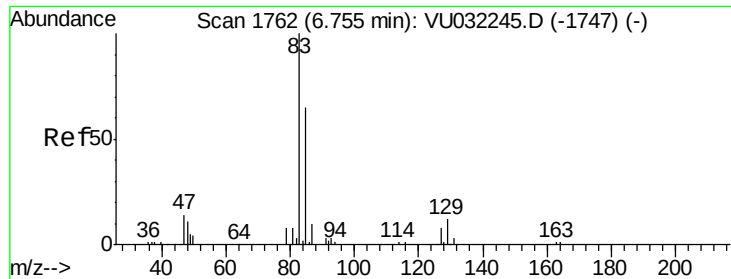

#38

Bromodichloromethane

Concen: 0.326 ug/L

RT: 6.76 min Scan# 1762

Delta R.T. 0.00 min

Lab File: VU032250.D

Acq: 23 May 2019 03:29

Instrument :

MSVOA_U

ClientSampleId :

E3YF0


Tgt Ion: 83 Resp: 5313

Ion Ratio Lower Upper

83 100

85 60.0 44.4 82.4




127 10.0 7.0 10.6

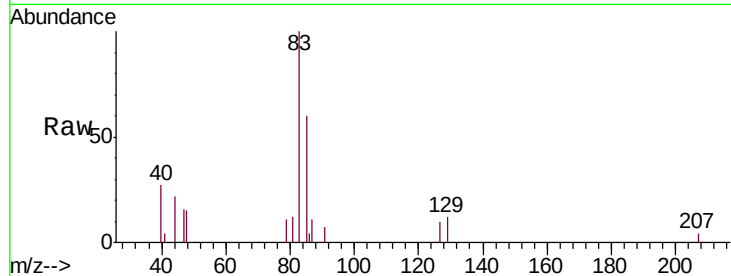

Abundance Ion 82.95 (82.65 to 83.65): VU032250.D (-1669) (-)

Ion 85.00 (84.70 to 85.70): VU032250.D (-1669) (-)

Ion 126.90 (126.60 to 127.60): VU032250.D (-1669) (-)

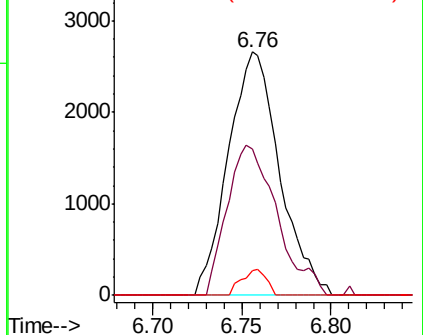

#39

cis-1,3-Dichloropropene

Concen: 0.179 ug/L

RT: 7.22 min Scan# 1907

Delta R.T. -0.04 min

Lab File: VU032250.D


Acq: 23 May 2019 03:29

Tgt Ion: 75 Resp: 3194

Ion Ratio Lower Upper



75 100


77 41.2 22.6 42.0



Abundance Ion 75.05 (74.75 to 75.75): VU032250.D (-1828) (-)

Ion 77.05 (76.75 to 77.75): VU032250.D (-1828) (-)

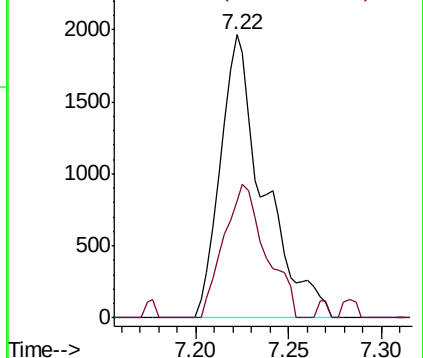

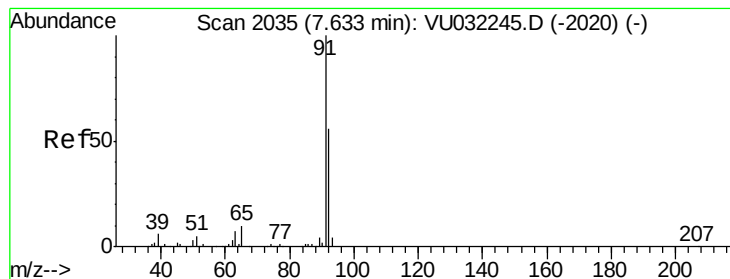

#42

Toluene

Concen: 9.677 ug/L

RT: 7.63 min Scan# 2035

Delta R.T. 0.00 min

Lab File: VU032250.D

Acq: 23 May 2019 03:29

Instrument :

MSVOA_U

ClientSampleId :


E3YF0

Tgt Ion: 91 Resp: 536168

Ion Ratio Lower Upper

91 100

92 56.1 38.5 71.5



Abundance Ion 91.15 (90.85 to 91.85): VU032245.D (-2020) (-)

Ion 92.15 (91.85 to 92.85): VU032245.D (-2020) (-)

7.63

300000



200000

100000

0

7.60 7.70

Time-->

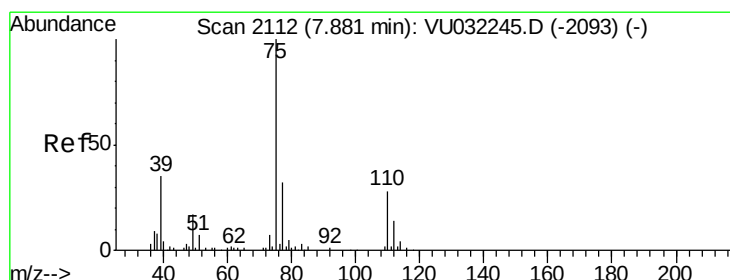

#44

trans-1,3-Dichloropropene

Concen: 0.131 ug/L

RT: 7.85 min Scan# 2101

Delta R.T. -0.04 min

Lab File: VU032250.D


Acq: 23 May 2019 03:29

Tgt Ion: 75 Resp: 1846

Ion Ratio Lower Upper

75 100

77 28.6 22.5 41.9



Abundance Ion 75.05 (74.75 to 75.75): VU032245.D (-2093) (-)

Ion 77.05 (76.75 to 77.75): VU032245.D (-2093) (-)

7.85

1000

800

600


400


200

0

7.80 7.85 7.90

Time-->





#47

Tetrachloroethene

Concen: 0.728 ug/L

RT: 8.22 min Scan# 2219

Delta R.T. 0.00 min

Lab File: VU032250.D

Acq: 23 May 2019 03:29

Instrument :

MSVOA_U

ClientSampled :

E3YF0

Tgt Ion:164 Resp: 8407


Ion Ratio Lower Upper

164 100

129 105.7 67.1 124.7

131 90.8 62.2 115.4

166 131.2 90.9 168.9






Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

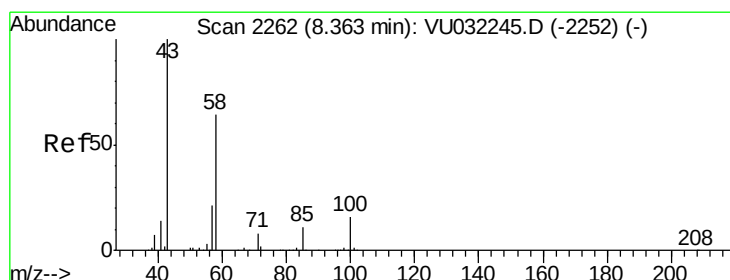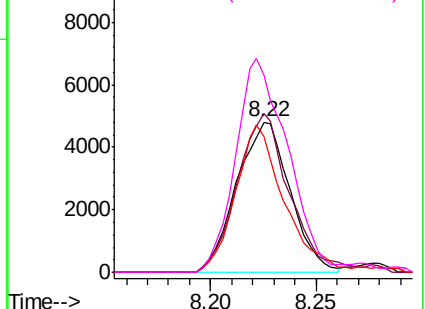

#48

2-Hexanone

Concen: 1.413 ug/L

RT: 8.37 min Scan# 2263

Delta R.T. 0.00 min

Lab File: VU032250.D

Acq: 23 May 2019 03:29

Tgt Ion: 43 Resp: 6876


Ion Ratio Lower Upper

43 100

58 44.3 49.7 74.5#

57 0.0 17.1 25.7#

100 10.3 11.6 17.4#






Abundance Ion 43.05 (42.75 to 43.75): VU0

Ion 58.05 (57.75 to 58.75): VU0

Ion 57.20 (56.90 to 57.90): VU0

Ion 100.15 (99.85 to 100.85): VU0

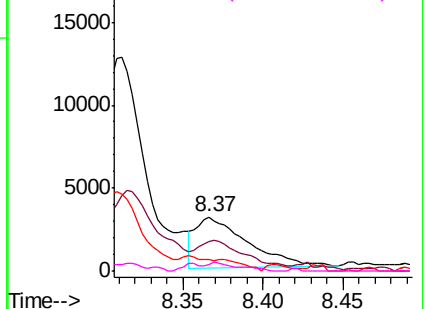



#49

Dibromochloromethane

Concen: 0.082 ug/L

RT: 8.48 min Scan# 2297

Delta R.T. 0.00 min

Lab File: VU032250.D

Acq: 23 May 2019 03:29


Instrument :
MSVOA_U
ClientSampleId :
E3YF0

Tgt Ion:129 Resp: 901




Ion Ratio Lower Upper

129 100

127 87.8 51.7 95.9

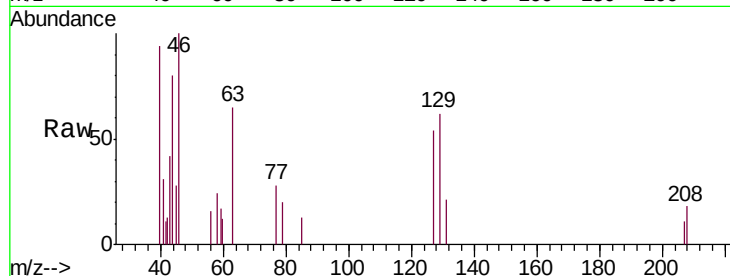

Abundance Ion 128.95 (128.65 to 129.65): V
Ion 126.90 (126.60 to 127.60): V

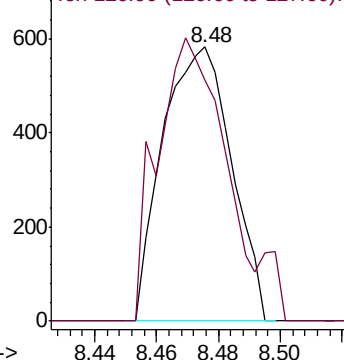

#51

Chlorobenzene

Concen: 10.094 ug/L

RT: 9.12 min Scan# 2496

Delta R.T. 0.00 min

Lab File: VU032250.D

Acq: 23 May 2019 03:29


Tgt Ion:112 Resp: 357963

Ion Ratio Lower Upper



112 100


114 30.8 22.6 42.0

77 56.9 46.8 70.2



Abundance Ion 112.10 (111.80 to 112.80): V
Ion 114.05 (113.75 to 114.75): V
Ion 77.10 (76.80 to 77.80): VU

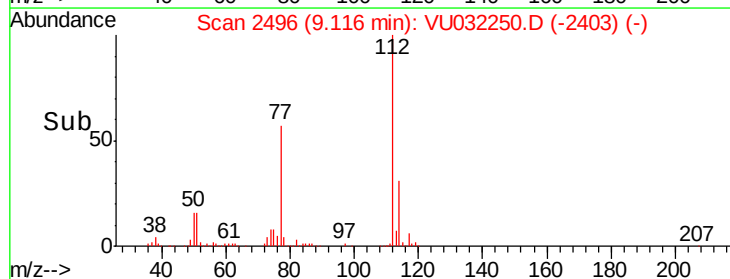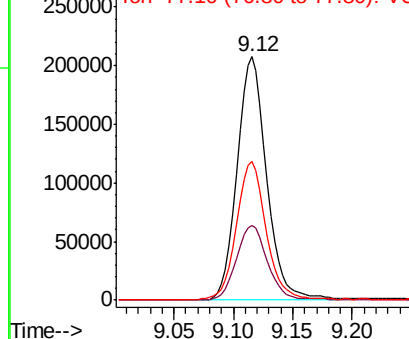

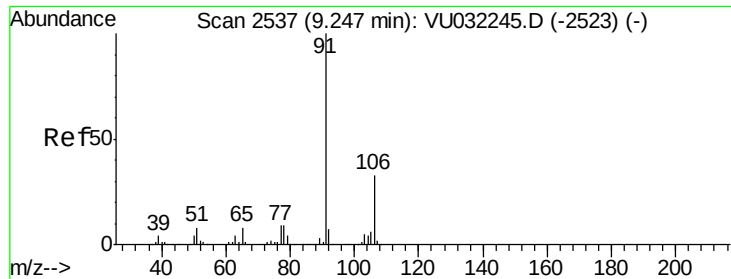

#52

Ethylbenzene

Concen: 0.158 ug/L

RT: 9.25 min Scan# 2538

Delta R.T. 0.00 min

Lab File: VU032250.D

Acq: 23 May 2019 03:29

Instrument :

MSVOA_U

ClientSampled :





E3YF0

Tgt Ion: 91 Resp: 8815

Ion Ratio Lower Upper

91 100

106 23.9 20.9 38.9

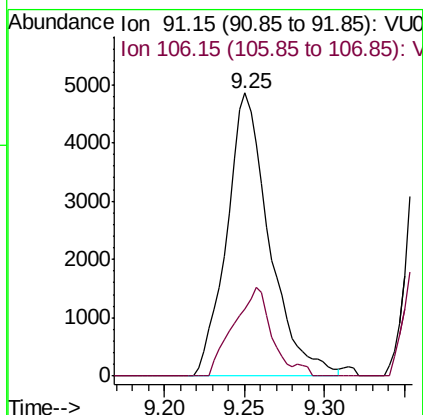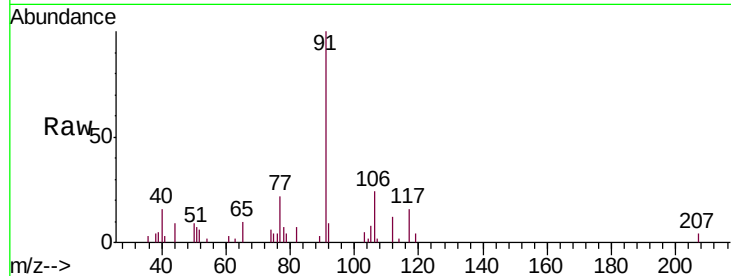

#53

m,p-Xylene

Concen: 0.752 ug/L

RT: 9.37 min Scan# 2576

Delta R.T. 0.00 min

Lab File: VU032250.D




Acq: 23 May 2019 03:29


Tgt Ion: 106 Resp: 15594

Ion Ratio Lower Upper

106 100

91 210.1 143.9 267.2


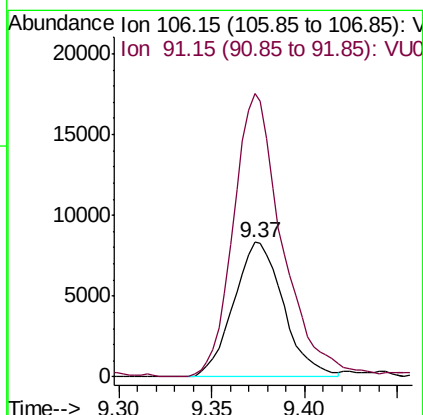




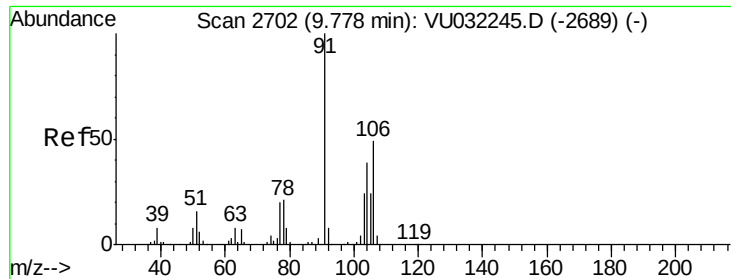

#54
o-Xylene
Concen: 0.483 ug/L
RT: 9.78 min Scan# 2702
Delta R.T. 0.00 min
Lab File: VU032250.D
Acq: 23 May 2019 03:29

Instrument :
MSVOA_U
ClientSampleId :
E3YF0

Tgt Ion: 106 Resp: 10014
Ion Ratio Lower Upper
106 100
91 167.3 147.8 274.4

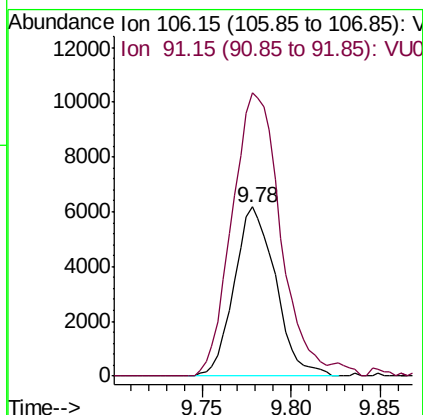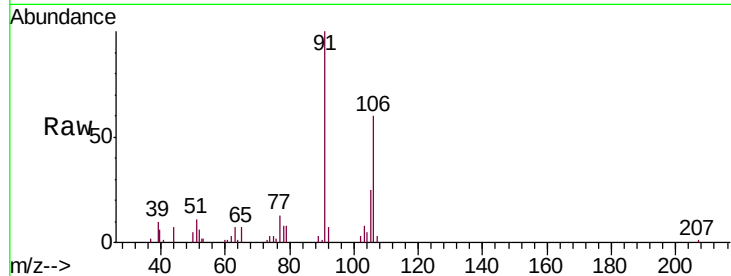

#59
1,2,3-Trichloropropane
Concen: 1.828 ug/L
RT: 11.48 min Scan# 3231
Delta R.T. 0.99 min
Lab File: VU032250.D
Acq: 23 May 2019 03:29

Tgt Ion: 75 Resp: 14950
Ion Ratio Lower Upper
75 100
77 0.0 28.2 42.4#

