

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052219\
 Data File : VU032236.D
 Acq On : 22 May 2019 20:52
 Operator : JC/SP
 Sample : K2888-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BN8

Quant Time: May 23 02:49:22 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR052219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 23 01:46:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	381738	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	390254	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	153285	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	113599	5.30	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.00%
7) Chloroethane-d5	1.68	69	97109	4.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.20%
11) 1,1-Dichloroethene-d2	2.27	63	171334	4.34	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.80%
20) 2-Butanone-d5	4.20	46	241095	39.87	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	79.74%
24) Chloroform-d	4.64	84	219260	4.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.00%
26) 1,2-Dichloroethane-d4	5.31	65	109061	3.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.20%
32) Benzene-d6	5.33	84	455029	4.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.20%
36) 1,2-Dichloropropane-d6	6.33	67	131689	3.66	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	73.20%
41) Toluene-d8	7.56	98	385290	3.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.60%
43) trans-1,3-Dichloropropene-	7.85	79	44963	3.25	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	65.00%
46) 2-Hexanone-d5	8.31	63	214389	41.20	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.40%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	104699	2.93	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	58.60%#
64) 1,2-Dichlorobenzene-d4	11.86	152	140818	3.33	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	66.60%#


Target Compounds					Ovalue
13) Acetone	2.33	43	6822	3.641 ug/L	100
47) Tetrachloroethene	8.22	164	606472	51.854 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU052219\
Data File : VU032236.D
Acq On : 22 May 2019 20:52
Operator : JC/SP
Sample : K2888-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BN8

Quant Time: May 23 02:49:22 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR052219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 23 01:46:44 2019
Response via : Initial Calibration

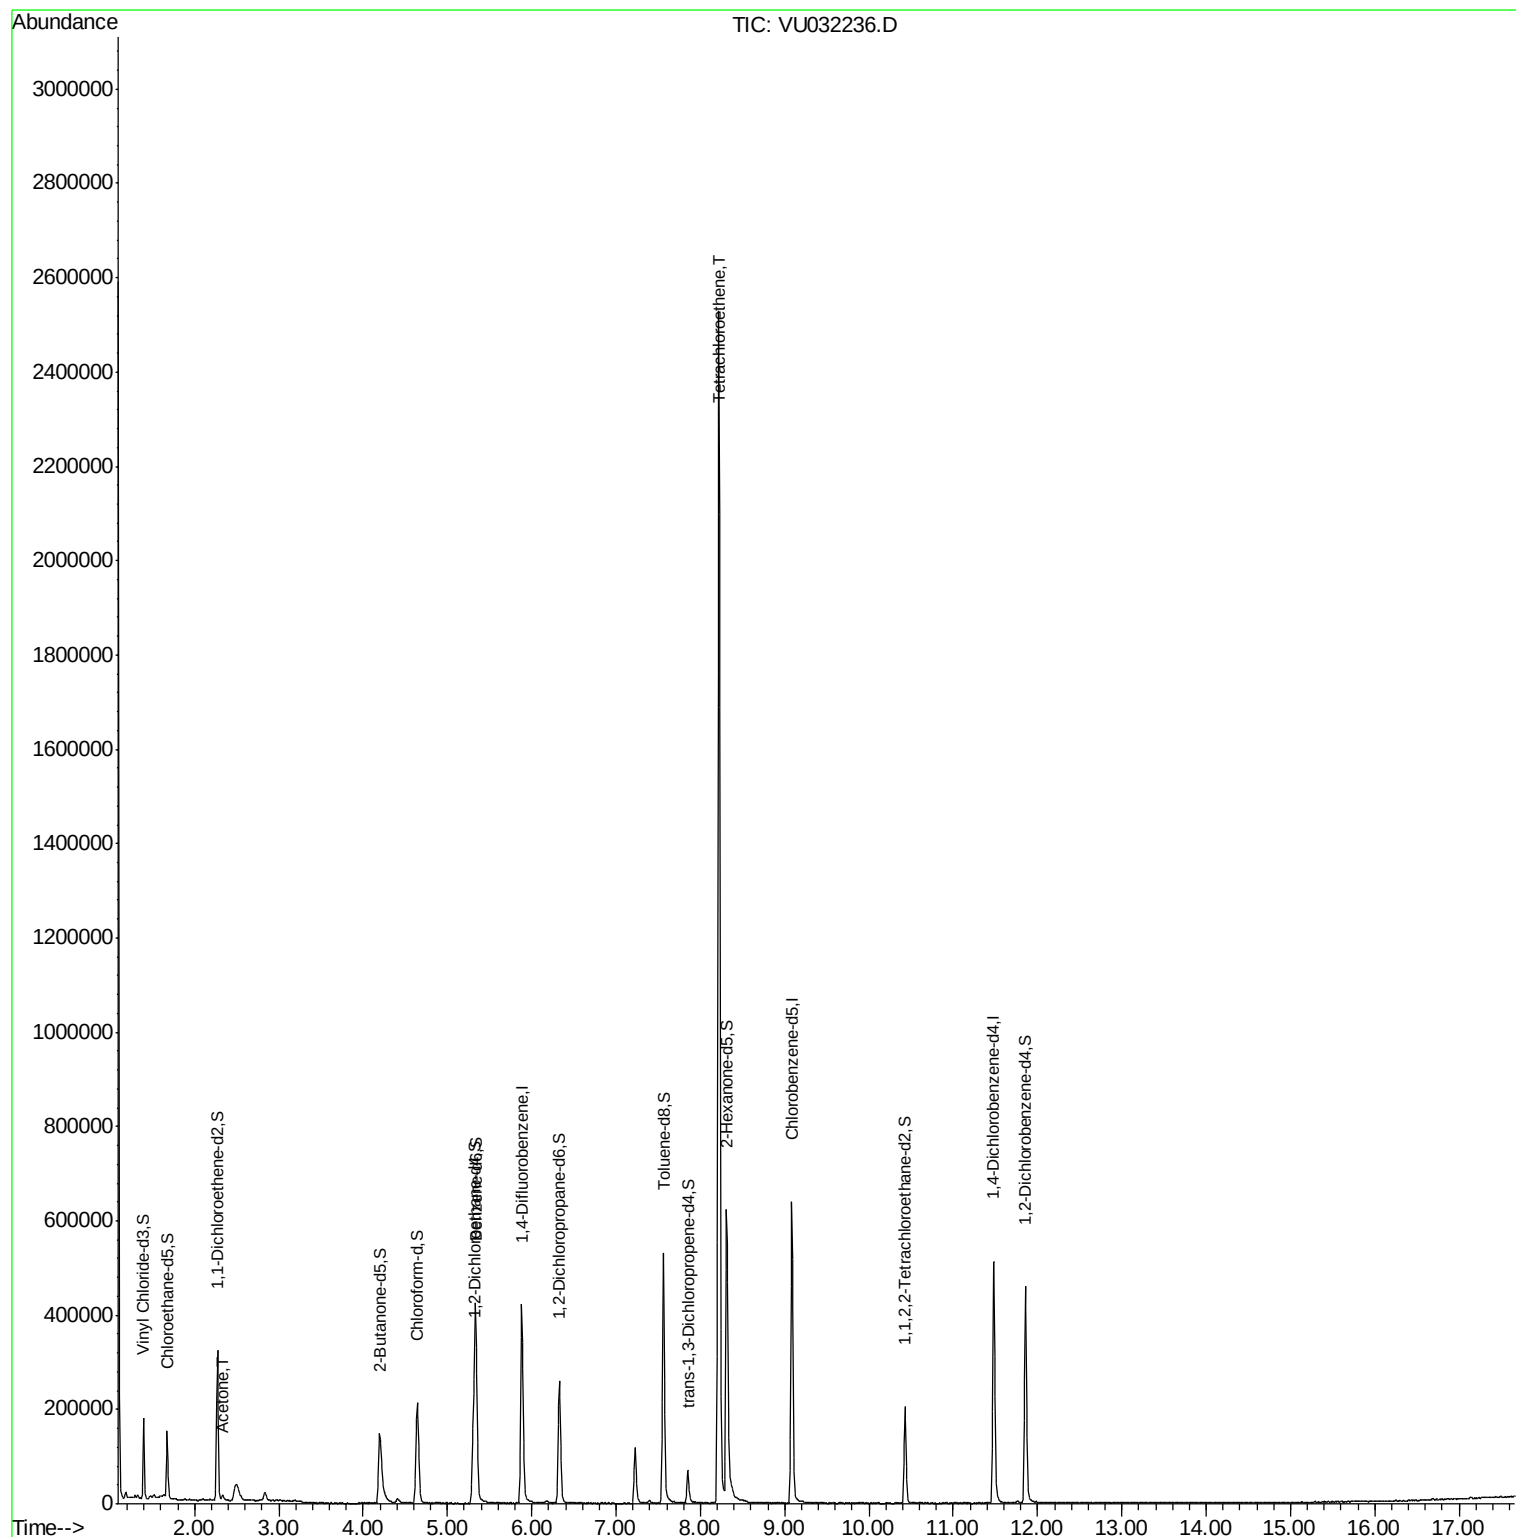

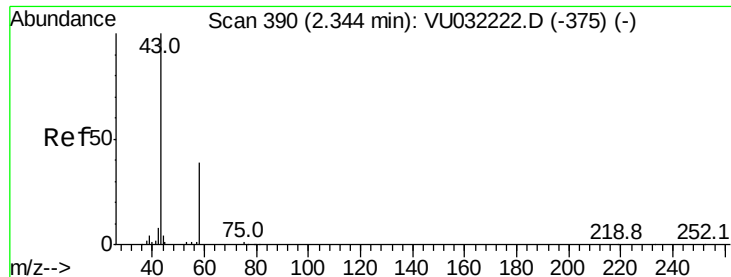

#13

Acetone

Concen: 3.641 ug/L

RT: 2.33 min Scan# 387

Delta R.T. -0.01 min

Lab File: VU032236.D

Acq: 22 May 2019 20:52

Instrument :

MSVOA_U

ClientSampleId :


C0BN8

Tot Ion: 43 Resp: 6822

Ion Ratio Lower Upper




43 100

58 36.3 0.0 72.6

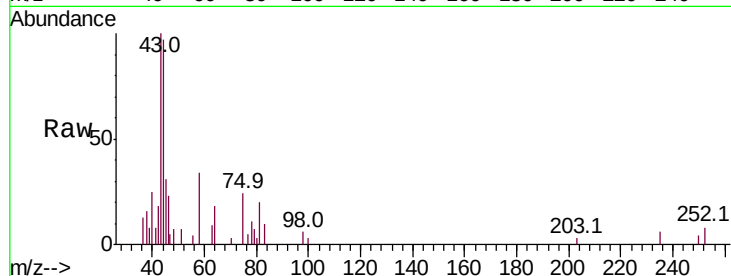

Abundance Ion 43.05 (42.75 to 43.75): VU032222.D (-375) (-)

Ion 58.05 (57.75 to 58.75): VU032222.D (-375) (-)

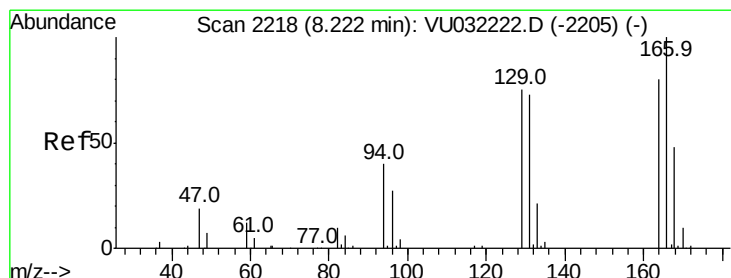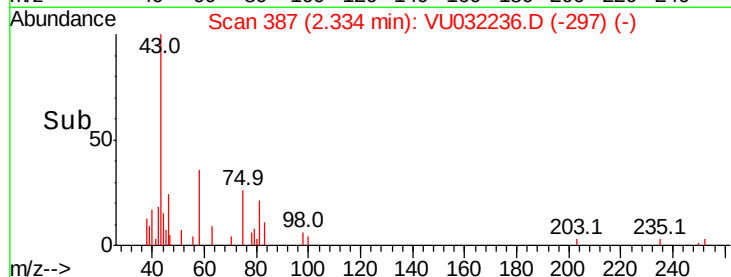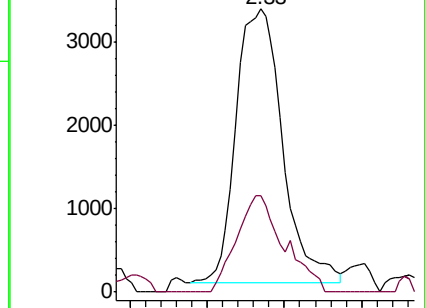

#47

Tetrachloroethene

Concen: 51.854 ug/L

RT: 8.22 min Scan# 2218

Delta R.T. 0.00 min

Lab File: VU032236.D

Acq: 22 May 2019 20:52

Tgt Ion: 164 Resp: 606472


Ion Ratio Lower Upper

164 100

129 91.8 67.1 124.7

131 89.6 62.2 115.4

166 128.1 90.9 168.9

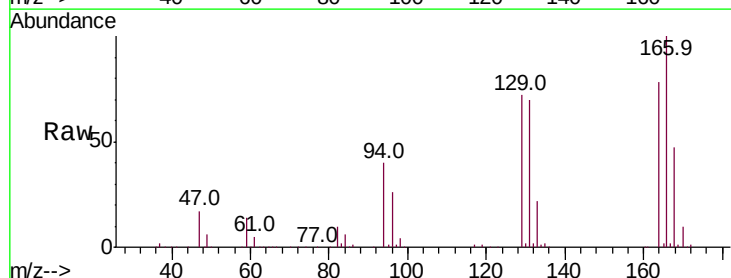

Abundance Ion 163.90 (163.60 to 164.60): VU032222.D (-2205) (-)

Ion 128.95 (128.65 to 129.65): VU032222.D (-2205) (-)

Ion 130.95 (130.65 to 131.65): VU032222.D (-2205) (-)

Ion 165.90 (165.60 to 166.60): VU032222.D (-2205) (-)

