


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052219\
Data File : VU032215.D
Acq On : 22 May 2019 11:07
Operator : JC/SP
Sample : BFB11
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB11

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR052219WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu May 23 12:27:17 2019

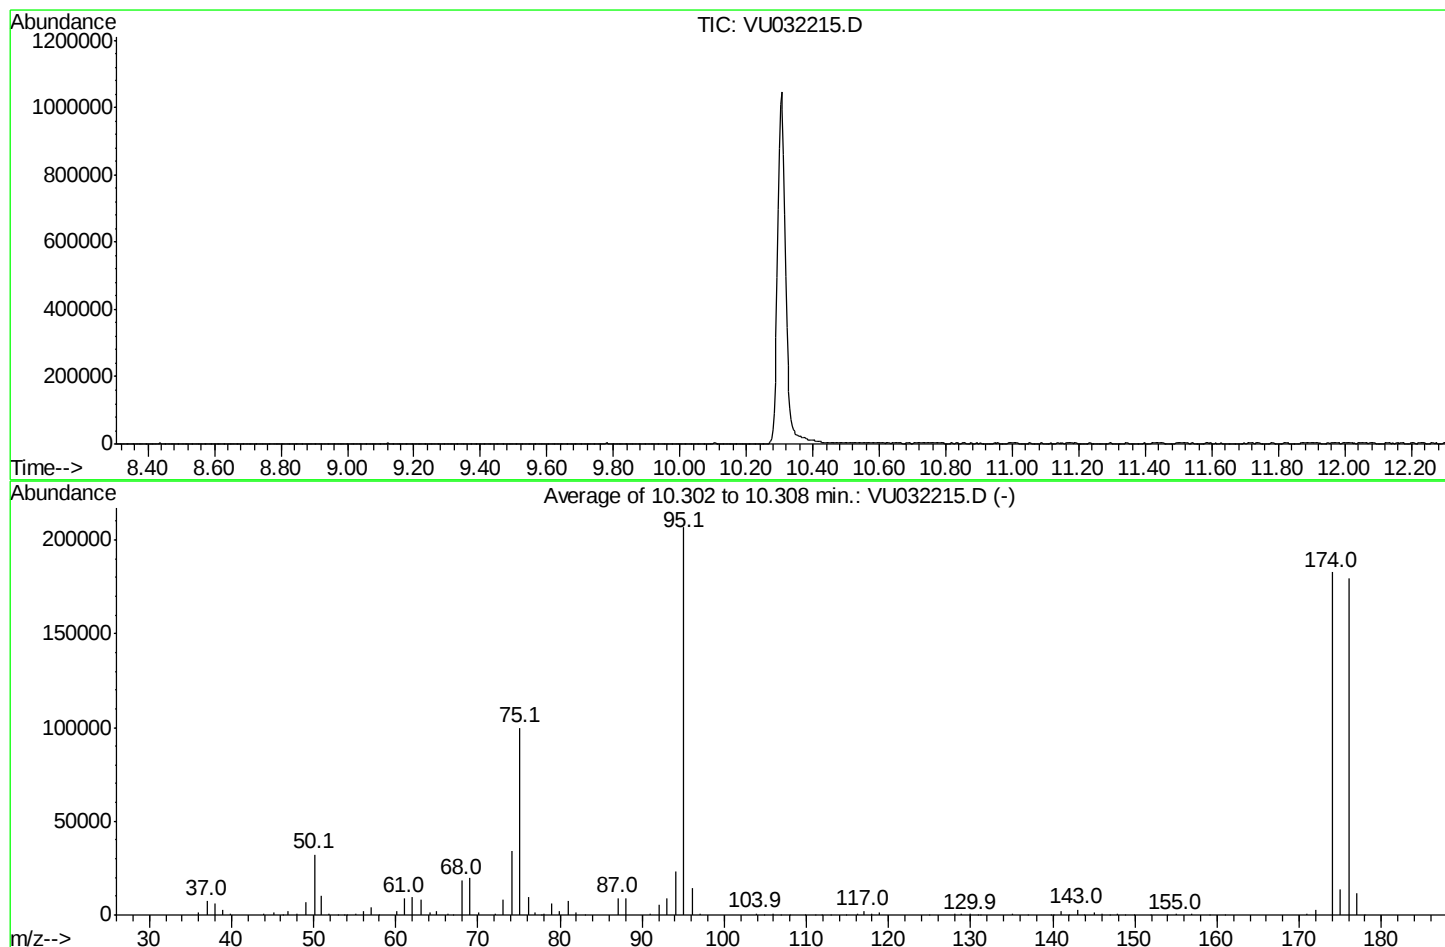

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	32234	PASS
75	95	30	80	48.3	99786	PASS
95	95	100	100	100.0	206741	PASS
96	95	5	9	6.8	14121	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.4	182805	PASS
175	174	5	9	7.6	13938	PASS
176	174	95	101	98.3	179626	PASS
177	176	5	9	6.3	11396	PASS

Scan 2851 (10.257 min): VU032215.D
BFB11

m/z	Abundance
40.00	498.0
43.90	909.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

m/z	Abundance
36.00	1361.0
37.00	7786.0
38.10	6531.0
39.00	2692.0
39.90	988.0
44.00	1471.0
45.10	1272.0
47.00	2210.0
48.00	1071.0
49.10	7545.0
50.10	32976.0
51.00	10108.0
51.90	674.0
53.00	343.0
53.70	109.0
54.10	154.0
55.10	420.0
56.10	2278.0
57.00	4292.0
58.00	193.0
60.00	2347.0
61.00	9211.0
62.00	9906.0
63.10	8558.0
64.10	1231.0
65.00	1939.0
66.30	486.0
68.00	18856.0
69.00	19856.0
70.10	1726.0
72.00	971.0
73.10	8619.0
74.10	33704.0
75.10	97864.0
76.10	9716.0
77.00	1188.0
77.70	853.0
78.20	913.0
78.90	6309.0
80.00	2007.0
81.00	7318.0
82.00	1579.0
83.10	117.0
87.00	9077.0
88.00	8924.0
91.00	588.0
92.00	5498.0
93.00	9011.0
94.10	23744.0
95.10	206848.0
96.10	14441.0
97.00	441.0
103.90	890.0
105.00	256.0
106.00	810.0
106.80	164.0
107.90	257.0
109.90	127.0
111.10	124.0
111.80	103.0
112.80	121.0
114.80	102.0
116.10	574.0
117.00	2103.0
117.90	888.0
118.90	1450.0
124.90	109.0
128.00	533.0
128.90	427.0
129.90	613.0
131.10	289.0
135.10	249.0
136.80	422.0
139.80	205.0
141.00	1707.0
142.00	242.0
143.00	3045.0
143.80	120.0
145.00	1434.0
145.90	503.0
147.90	521.0
148.80	100.0
149.80	132.0
153.90	109.0
155.00	477.0
156.90	397.0
159.10	131.0
170.80	573.0
172.00	2692.0
174.00	177536.0
175.00	13388.0
176.00	175168.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

177.0011185.0

177.90354.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

m/z	Abundance
36.00	1337.0
37.00	8103.0
38.10	6421.0
39.00	2907.0
39.90	1079.0
44.00	1610.0
45.10	1209.0
47.00	2246.0
47.90	1028.0
49.10	7389.0
50.10	33240.0
51.00	10743.0
51.90	546.0
52.90	349.0
53.80	141.0
54.00	143.0
55.10	483.0
56.10	2456.0
57.00	4398.0
57.90	189.0
60.10	2301.0
61.00	9342.0
62.10	9983.0
63.10	8669.0
64.10	1393.0
65.00	2000.0
66.30	430.0
68.00	19112.0
69.00	20312.0
70.10	1727.0
72.10	678.0
73.00	8592.0
74.10	35576.0
75.10	102736.0
76.10	9726.0
77.00	1116.0
78.10	995.0
78.90	6480.0
80.00	1966.0
81.00	7655.0
82.00	1764.0
87.00	9122.0
88.00	8772.0
91.00	571.0
92.10	5769.0
93.10	9254.0
94.10	24216.0
95.10	213248.0
96.10	14661.0
97.00	479.0
103.90	979.0
104.80	216.0
105.90	806.0
106.80	162.0
108.00	239.0
109.90	179.0
112.90	163.0
114.80	123.0
116.20	545.0
117.00	2222.0
117.90	886.0
118.90	1312.0
128.00	415.0
128.90	432.0
129.90	678.0
131.10	265.0
135.00	436.0
136.90	342.0
139.70	243.0
141.00	1844.0
142.00	226.0
143.00	3054.0
143.80	157.0
145.00	1269.0
145.90	437.0
146.90	140.0
147.90	598.0
148.70	121.0
149.80	161.0
153.80	106.0
155.00	565.0
156.90	475.0
170.90	532.0
172.00	2934.0
174.00	188160.0
175.00	14368.0
176.00	185216.0
177.00	11857.0
177.90	255.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

m/z	Abundance
36.00	1300.0
37.00	7053.0
38.00	5769.0
39.00	2806.0
39.90	1017.0
44.00	1698.0
45.10	1161.0
46.20	417.0
46.90	2050.0
47.90	956.0
49.10	6478.0
50.10	30488.0
51.00	9796.0
52.00	395.0
52.90	249.0
53.90	137.0
55.10	409.0
56.10	2324.0
57.00	4250.0
57.90	163.0
60.00	2069.0
61.00	8404.0
62.10	8943.0
63.10	7574.0
64.10	1384.0
65.00	1905.0
66.40	265.0
67.00	351.0
68.00	18352.0
69.00	18712.0
70.00	1395.0
72.10	553.0
73.00	8324.0
74.10	33552.0
75.10	98760.0
76.10	8546.0
77.00	1049.0
78.00	997.0
79.00	6094.0
79.90	1953.0
81.00	6874.0
82.00	1675.0
87.00	8723.0
88.00	8267.0
91.00	488.0
92.10	5319.0
93.10	8786.0
94.10	22688.0
95.10	200128.0
96.10	13262.0
97.00	500.0
103.90	960.0
104.80	148.0
105.90	779.0
106.80	132.0
108.00	150.0
109.90	187.0
111.20	103.0
113.00	201.0
114.90	173.0
116.20	421.0
117.00	1995.0
117.90	775.0
118.90	1052.0
128.10	399.0
128.90	358.0
130.00	702.0
130.80	229.0
135.00	594.0
137.00	259.0
139.70	255.0
140.10	137.0
140.90	1795.0
142.00	276.0
143.00	2865.0
143.80	173.0
145.00	1067.0
146.00	348.0
146.90	231.0
147.90	523.0
148.70	138.0
149.90	151.0
151.90	104.0
153.80	100.0
155.00	618.0
157.00	460.0
160.90	139.0
170.90	510.0
172.00	3057.0
174.00	182720.0
175.00	14059.0
176.00	178496.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

177.0011146.0

177.90184.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11