

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052223\
 Data File : VU054250.D
 Acq On : 22 May 2023 17:33
 Operator : JC/MD
 Sample : 02874-07DL 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0NY9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054250.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.356	3	5	17	rVB3	9412	8659	1.64%	0.198%
2	1.597	72	80	95	rVB	50877	61514	11.68%	1.405%
3	1.913	169	178	192	rBV	43134	58235	11.06%	1.330%
4	2.562	368	380	397	rBV	91724	150891	28.66%	3.446%
5	3.041	514	529	552	rBV2	47927	97680	18.55%	2.231%
6	3.179	559	572	587	rBV2	8473	19275	3.66%	0.440%
7	4.633	1009	1024	1055	rBV2	53112	202438	38.44%	4.623%
8	5.057	1142	1156	1184	rVB	83602	195834	37.19%	4.472%
9	5.719	1342	1362	1391	rBV3	156645	403610	76.65%	9.217%
10	6.244	1511	1525	1546	rBV	196011	376524	71.51%	8.598%
11	6.536	1603	1616	1643	rBV	276142	526568	100.00%	12.025%
12	6.684	1650	1662	1684	rVB3	95904	190765	36.23%	4.356%
13	7.562	1924	1935	1950	rBV2	46655	82075	15.59%	1.874%
14	7.893	2022	2038	2057	rBV	187221	329293	62.54%	7.520%
15	8.176	2115	2126	2143	rBV3	27652	47589	9.04%	1.087%
16	8.629	2256	2267	2300	rBV2	170155	335238	63.66%	7.656%
17	9.414	2498	2511	2544	rBV	271619	463423	88.01%	10.583%
18	10.751	2916	2927	2941	rBV2	68431	112012	21.27%	2.558%
19	11.806	3240	3255	3277	rBV	266731	437684	83.12%	9.995%
20	12.189	3363	3374	3395	rBV	174809	279707	53.12%	6.387%




Sum of corrected areas: 4379014

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052223\
Data File : VU054250.D
Acq On : 22 May 2023 17:33
Operator : JC/MD
Sample : 02874-07DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0NY9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

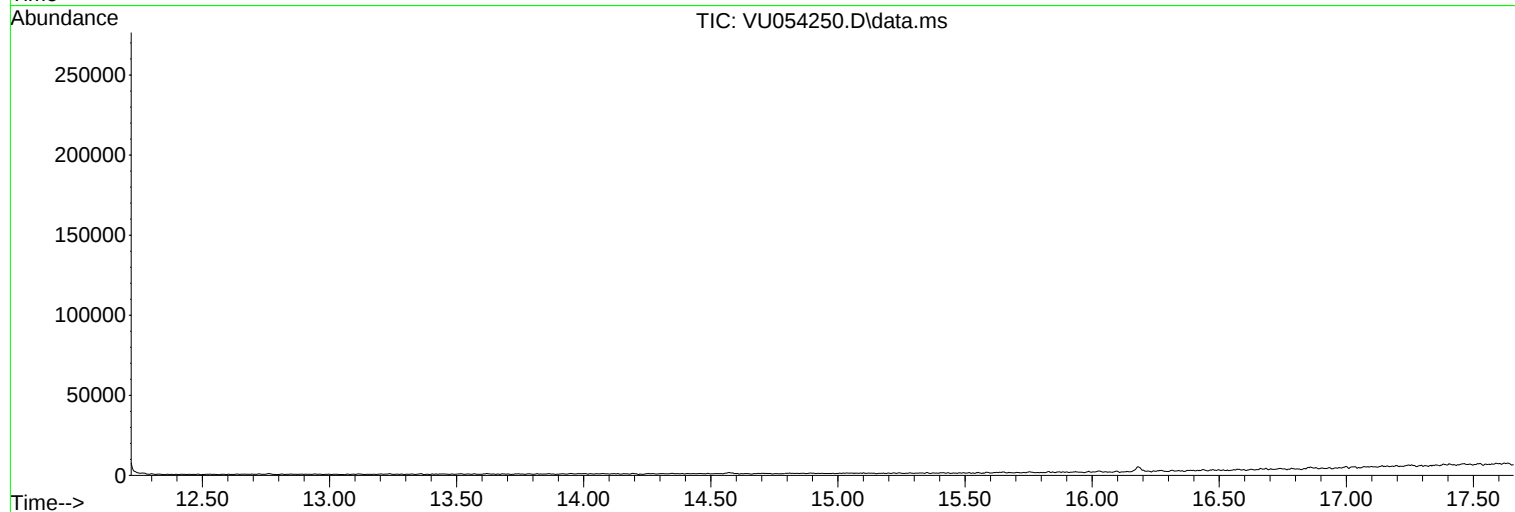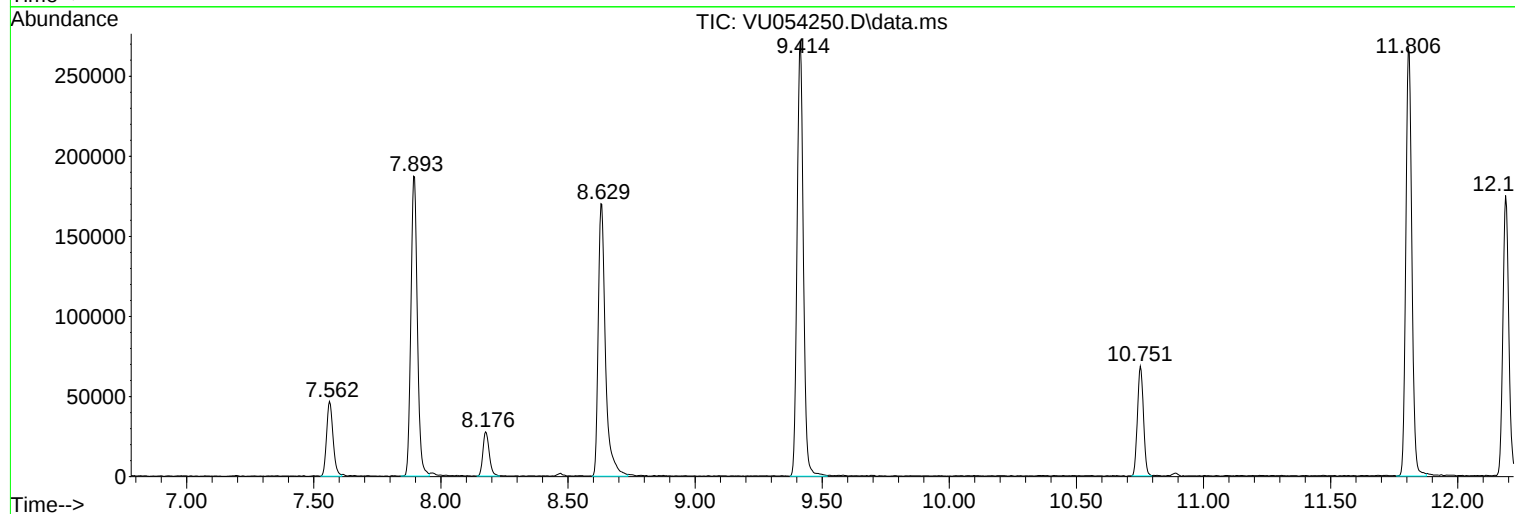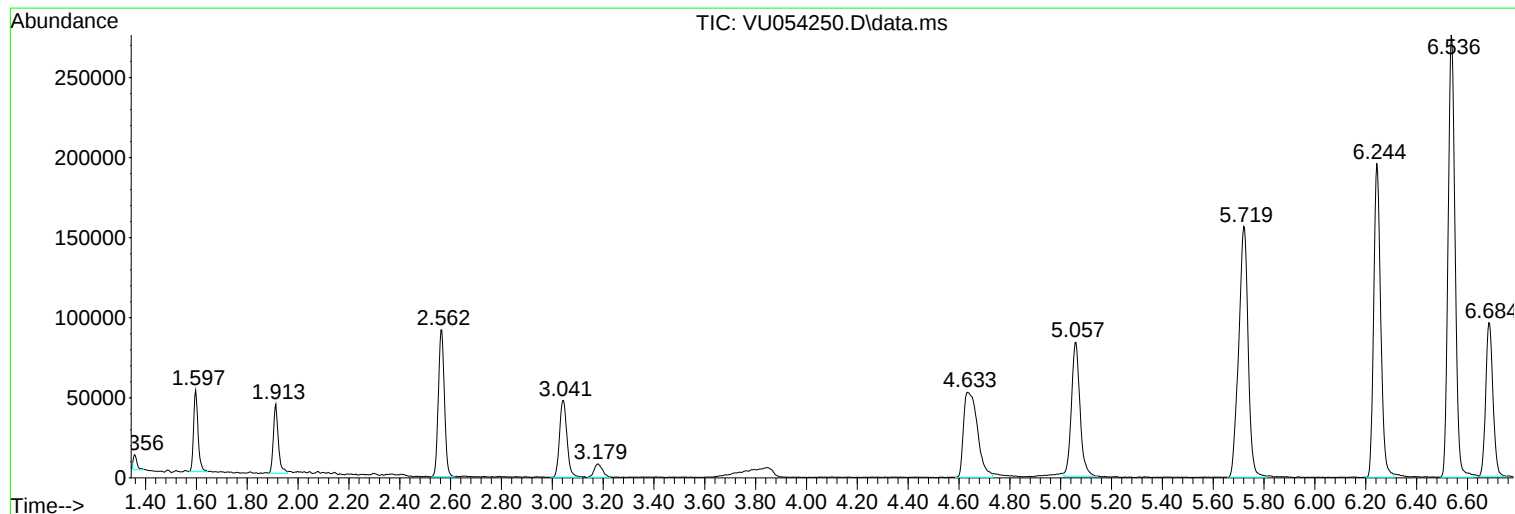

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052223\
Data File : VU054250.D
Acq On : 22 May 2023 17:33
Operator : JC/MD
Sample : 02874-07DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0NY9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052223\
Data File : VU054250.D
Acq On : 22 May 2023 17:33
Operator : JC/MD
Sample : 02874-07DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0NY9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc