

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052223\
 Data File : VU054253.D
 Acq On : 22 May 2023 18:46
 Operator : JC/MD
 Sample : 02859-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU054253.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	17	rVB2	8095	7701	1.63%	0.203%
2	1.597	71	80	93	rBV	53150	63407	13.40%	1.669%
3	1.913	169	178	198	rBV	41887	61264	12.94%	1.613%
4	2.562	369	380	398	rBV	95066	155400	32.83%	4.090%
5	3.044	515	530	548	rBV2	23536	46971	9.92%	1.236%
6	4.633	1011	1024	1057	rBV2	46655	142851	30.18%	3.760%
7	5.057	1143	1156	1177	rVB2	81882	184301	38.94%	4.851%
8	5.719	1338	1362	1381	rBV2	159388	406919	85.97%	10.711%
9	6.244	1512	1525	1547	rBV	205006	388533	82.09%	10.227%
10	6.539	1606	1617	1628	rVB5	4507	8511	1.80%	0.224%
11	6.687	1649	1663	1685	rBV2	97477	196200	41.45%	5.164%
12	7.562	1923	1935	1956	rBV2	44076	81061	17.13%	2.134%
13	7.893	2025	2038	2062	rBV	192045	337754	71.36%	8.890%
14	8.176	2112	2126	2141	rBV2	27738	47435	10.02%	1.249%
15	8.469	2205	2217	2228	rBV3	5455	9552	2.02%	0.251%
16	8.632	2255	2268	2298	rBV2	168994	335195	70.82%	8.823%
17	9.414	2499	2511	2532	rBV	280864	473306	100.00%	12.458%
18	10.751	2914	2927	2940	rBV	69657	112727	23.82%	2.967%
19	10.886	2961	2969	2980	rBV3	6994	11083	2.34%	0.292%
20	11.806	3242	3255	3286	rBV	274571	451019	95.29%	11.872%
21	12.189	3363	3374	3396	rBV	170363	277891	58.71%	7.315%




Sum of corrected areas: 3799081

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052223\
Data File : VU054253.D
Acq On : 22 May 2023 18:46
Operator : JC/MD
Sample : 02859-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

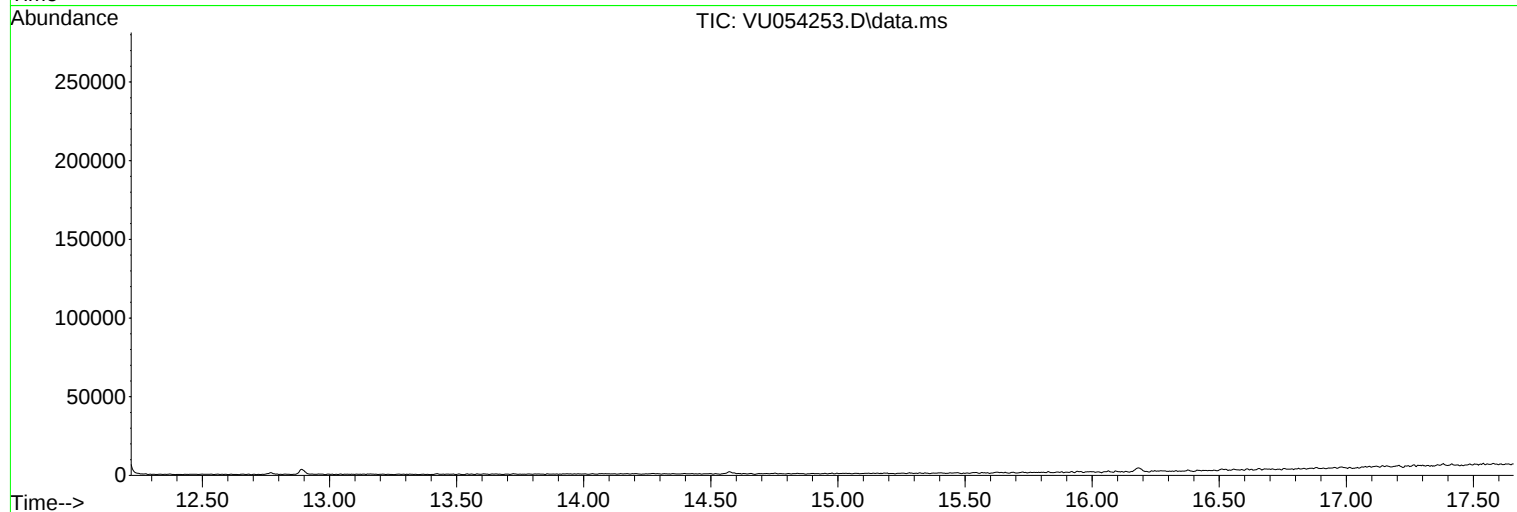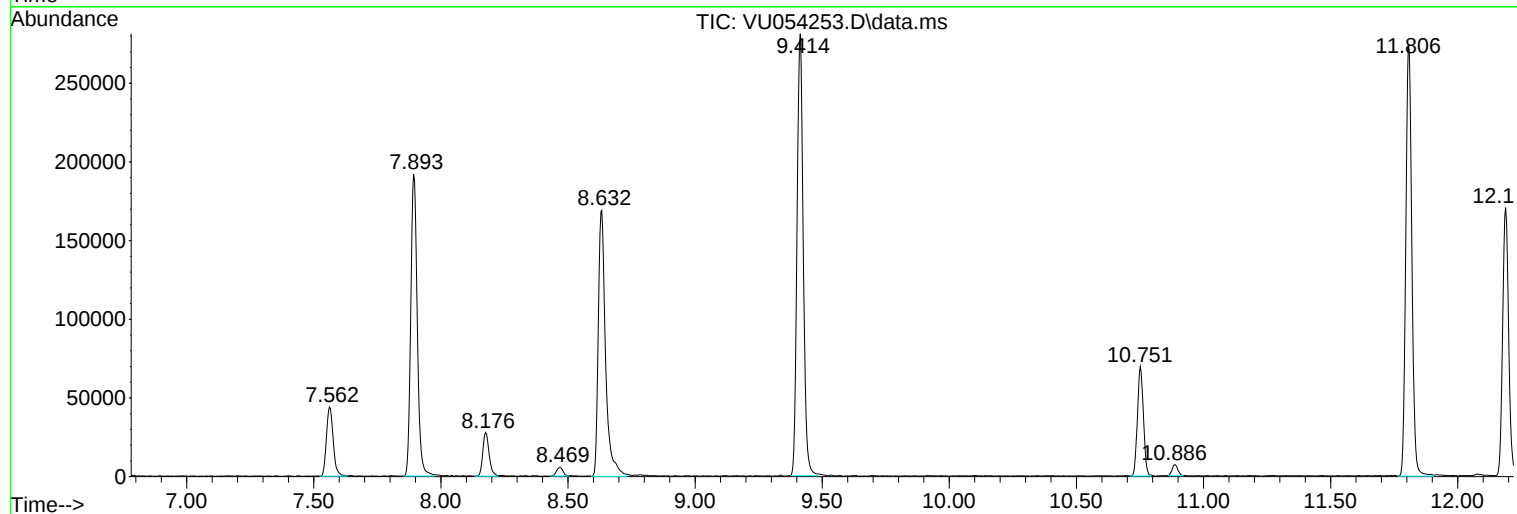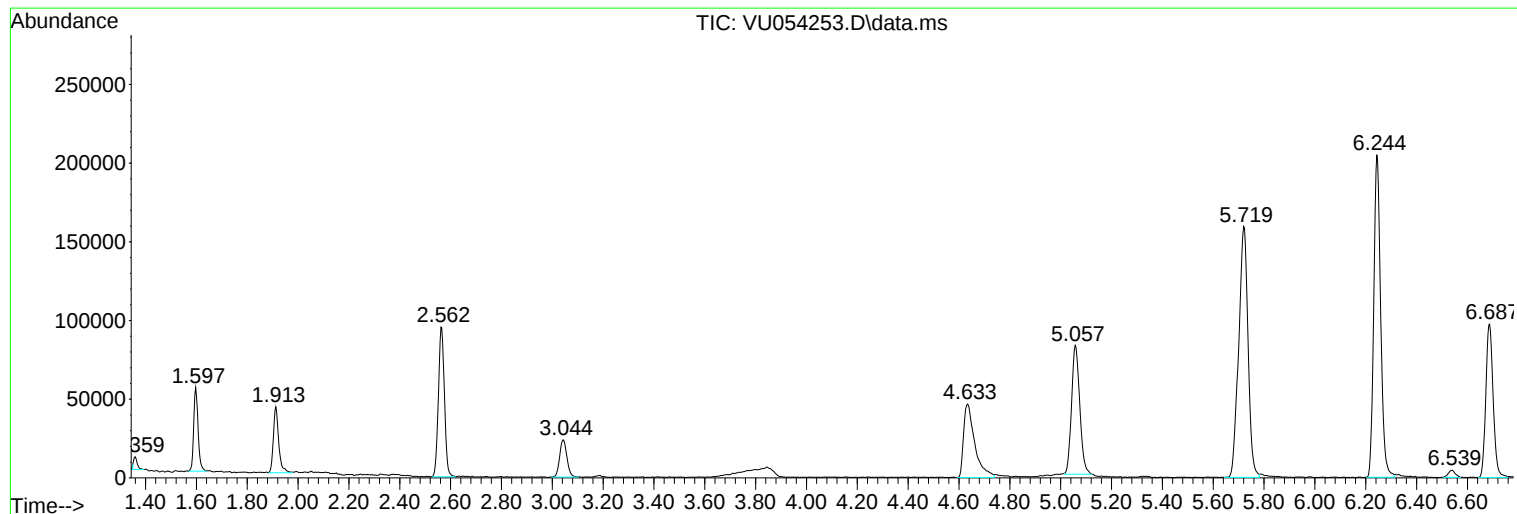

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052223\
Data File : VU054253.D
Acq On : 22 May 2023 18:46
Operator : JC/MD
Sample : 02859-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052223\
Data File : VU054253.D
Acq On : 22 May 2023 18:46
Operator : JC/MD
Sample : 02859-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc