

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU052318\
 Data File : VU024047.D
 Acq On : 23 May 2018 19:46
 Operator : MD/SY
 Sample : J3088-15 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Quant Time: May 24 05:04:47 2018
 Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM051218WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 24 04:14:38 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	274968	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	283014	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	119439	50.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.40	65	76045	29.76	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	59.52%#
7) Chloroethane-d5	1.68	69	68196	33.87	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	67.74%#
11) 1,1-Dichloroethene-d2	2.27	63	117449	25.05	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	50.10%#
21) 2-Butanone-d5	4.19	46	203595	114.50	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	114.50%
24) Chloroform-d	4.65	84	174360	44.71	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.42%
26) 1,2-Dichloroethane-d4	5.32	65	123746	48.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.46%
32) Benzene-d6	5.35	84	322164	39.00	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.00%
36) 1,2-Dichloropropane-d6	6.34	67	123995	44.43	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.86%
41) Toluene-d8	7.57	98	283511	37.25	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	74.50%#
43) trans-1,3-Dichloropropene-	7.85	79	46859	39.92	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.84%
47) 2-Hexanone-d5	8.32	63	138067	107.34	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	107.34%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	188525	47.97	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.94%
64) 1,2-Dichlorobenzene-d4	11.87	152	126842	49.17	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.34%


Target Compounds						Ovalue
20) cis-1,2-Dichloroethene	4.23	96	27199	11.50	ug/L	92
34) Trichloroethene	6.19	95	11701	4.93	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU052318\
Data File : VU024047.D
Acq On : 23 May 2018 19:46
Operator : MD/SY
Sample : J3088-15 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Quant Time: May 24 05:04:47 2018
Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM051218WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 24 04:14:38 2018
Response via : Initial Calibration

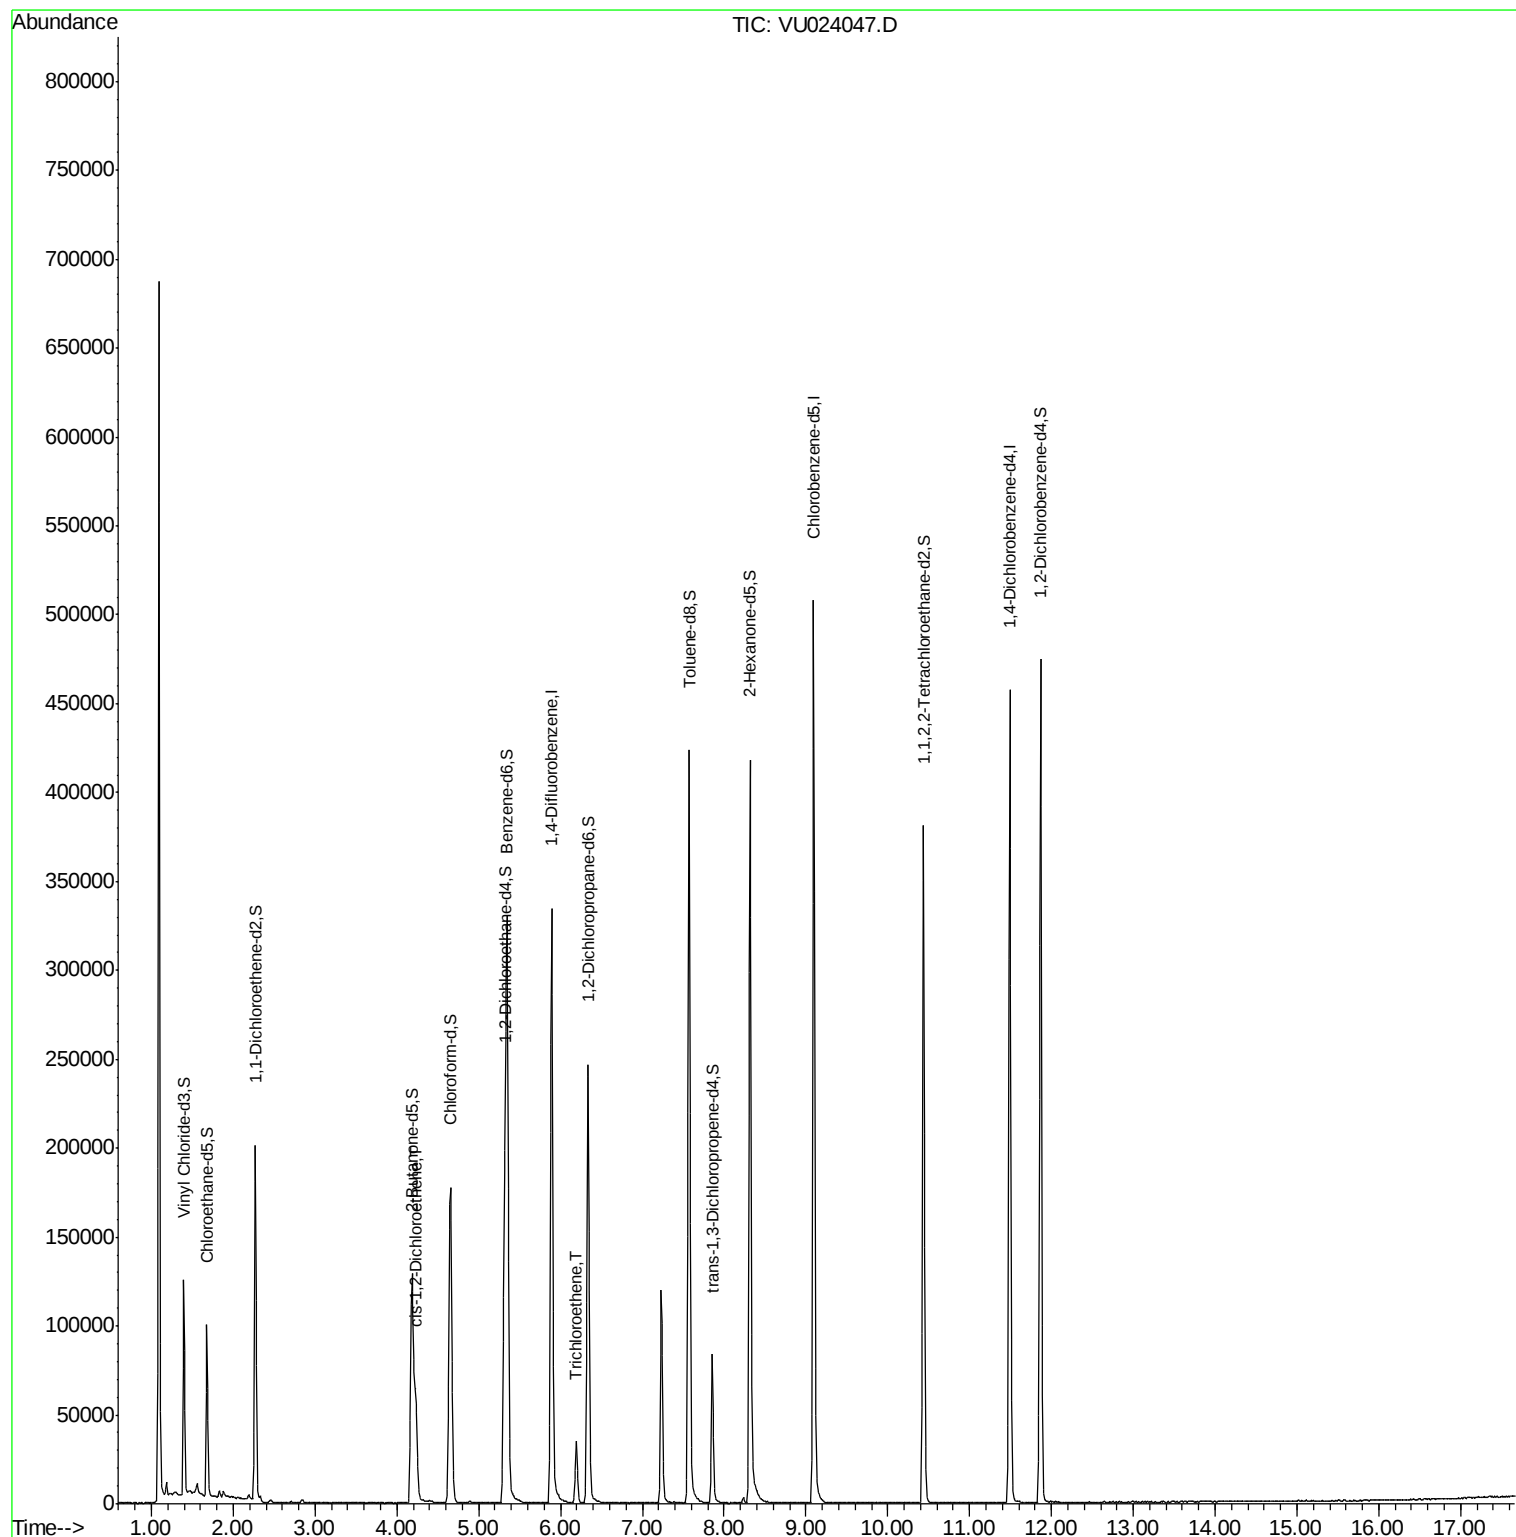

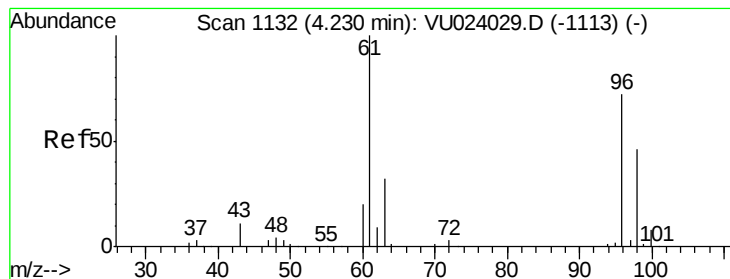

#20

cis-1,2-Dichloroethene

Concen: 11.50 ug/L

RT: 4.23 min Scan# 1132

Delta R.T. 0.00 min

Lab File: VU024047.D

Acq: 23 May 2018 19:46


Tot Ion: 96 Resp: 27199

Ion Ratio Lower Upper

96 100

61 143.1 93.3 173.3

68 0.0 0.0 0.0



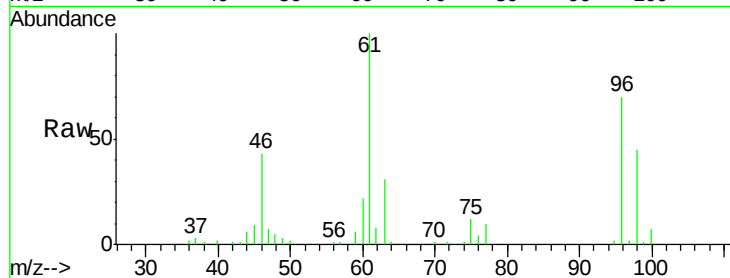


Abundance

Ion 96.00 (95.70 to 96.70): VU0

Ion 61.00 (60.70 to 61.70): VU0

Ion 68.00 (67.70 to 68.70): VU0

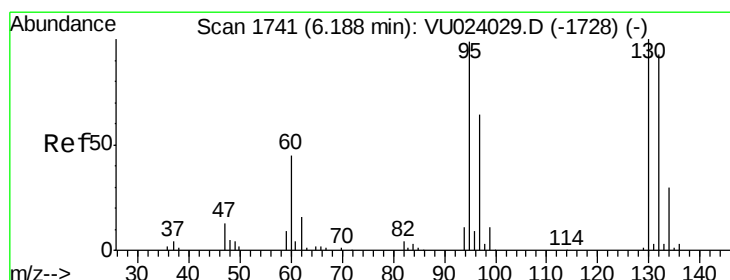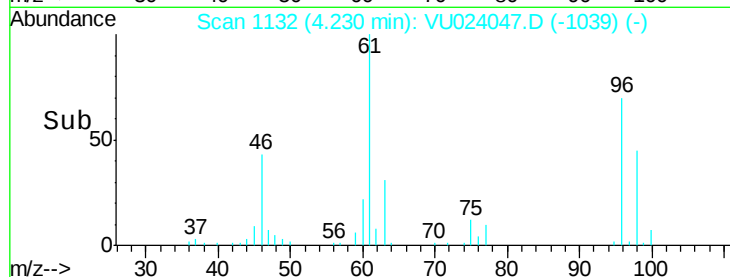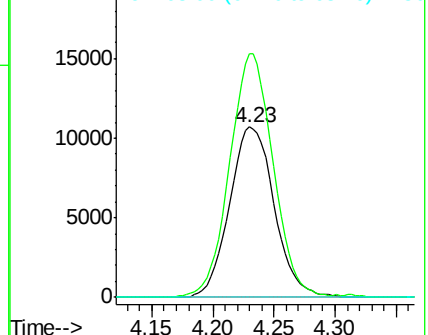

#34

Trichloroethene

Concen: 4.93 ug/L

RT: 6.19 min Scan# 1743

Delta R.T. 0.01 min

Lab File: VU024047.D

Acq: 23 May 2018 19:46

Tgt Ion: 95 Resp: 11701


Ion Ratio Lower Upper

95 100

97 66.9 45.4 84.2

132 97.2 69.0 128.1

130 95.1 71.7 133.1

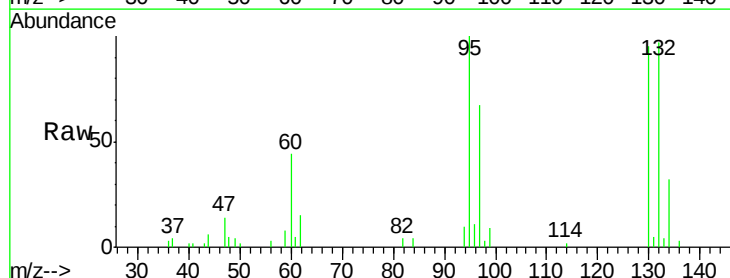

Abundance

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

Ion 132.00 (131.70 to 132.70): V

Ion 130.00 (129.70 to 130.70): V

