

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052319\
 Data File : VU032275.D
 Acq On : 23 May 2019 17:49
 Operator : JC/SP
 Sample : K3018-10
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XJ7

Quant Time: May 24 03:07:18 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR052219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 24 02:55:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	345899	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	361540	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	147551	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	79650	4.10	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.00%
7) Chloroethane-d5	1.68	69	80923	4.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.40%
11) 1,1-Dichloroethene-d2	2.27	63	130254	3.64	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.80%
20) 2-Butanone-d5	4.20	46	265777	48.50	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.00%
24) Chloroform-d	4.64	84	229989	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.60%
26) 1,2-Dichloroethane-d4	5.31	65	127266	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
32) Benzene-d6	5.33	84	438552	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.60%
36) 1,2-Dichloropropane-d6	6.33	67	147534	4.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.60%
41) Toluene-d8	7.56	98	384516	3.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.20%
43) trans-1,3-Dichloropropene-	7.85	79	52983	4.14	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.80%
46) 2-Hexanone-d5	8.31	63	220775	45.80	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.60%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	154631	4.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.40%
64) 1,2-Dichlorobenzene-d4	11.86	152	196397	4.83	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.60%


Target Compounds					Ovalue
13) Acetone	2.33	43	9111	5.367 ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU052319\
Data File : VU032275.D
Acq On : 23 May 2019 17:49
Operator : JC/SP
Sample : K3018-10
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XJ7

Quant Time: May 24 03:07:18 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR052219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 24 02:55:50 2019
Response via : Initial Calibration

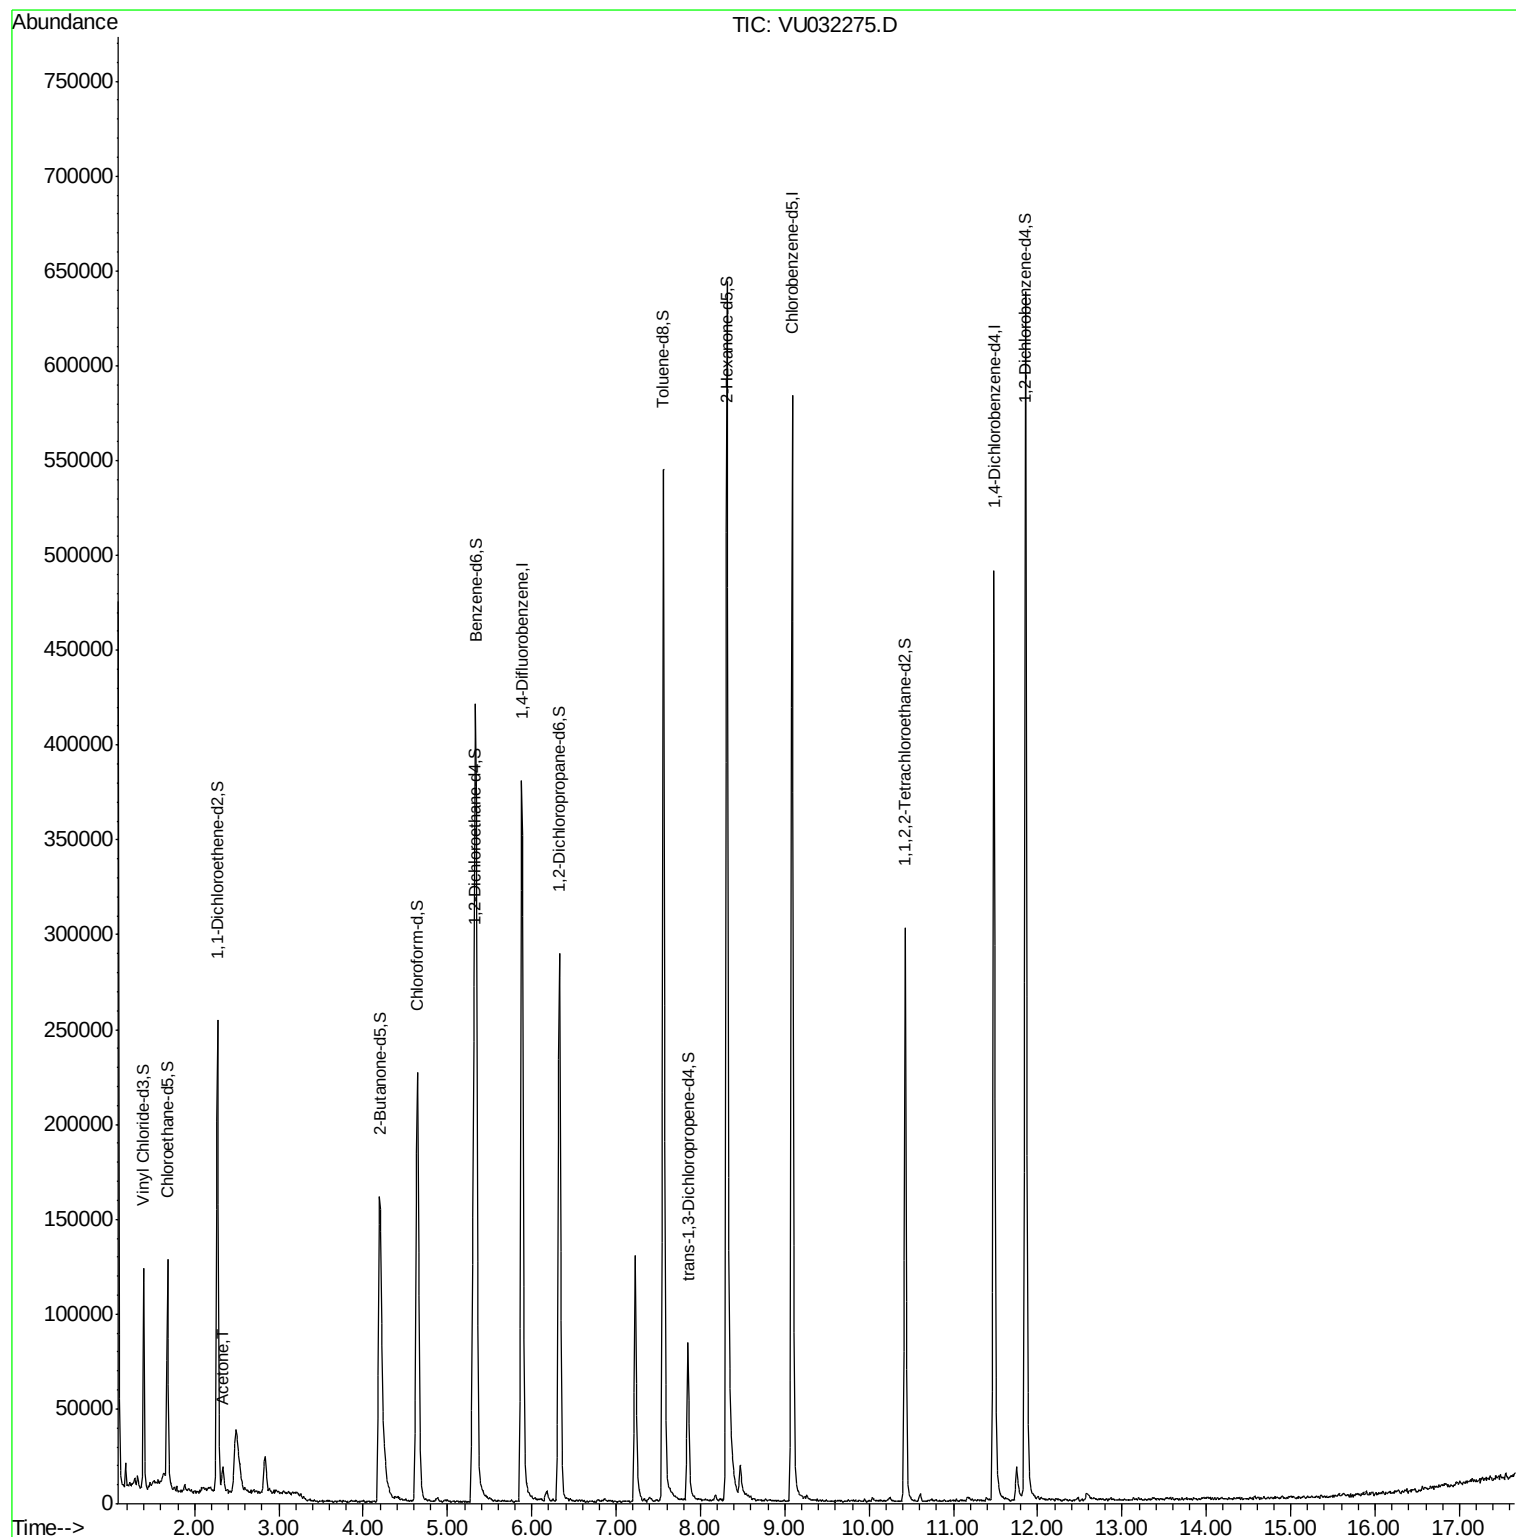

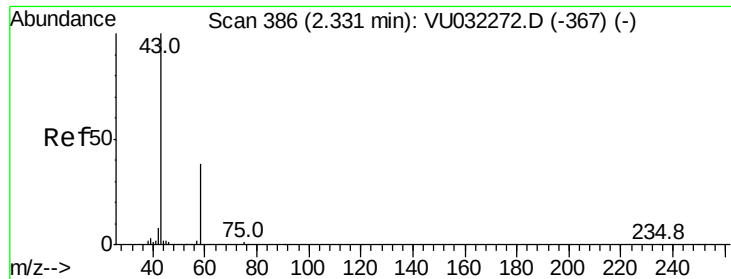

#13

Acetone

Concen: 5.367 ug/L

RT: 2.33 min Scan# 387

Delta R.T. 0.00 min

Lab File: VU032275.D

Acq: 23 May 2019 17:49

Instrument :

MSVOA_U

ClientSampleId :

C0XJ7

Tot Ion: 43 Resp: 9111

Ion Ratio Lower Upper

43 100

58 46.2 0.0 72.6

