

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052319\
 Data File : VU032279.D
 Acq On : 23 May 2019 19:28
 Operator : JC/SP
 Sample : K2888-05DL 5X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BN7DL

Quant Time: May 24 04:04:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR052219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 24 02:55:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	346613	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	354929	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	137830	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	110405	5.67	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	113.40%
7) Chloroethane-d5	1.68	69	92659	5.10	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.00%
11) 1,1-Dichloroethene-d2	2.27	63	163028	4.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.80%
20) 2-Butanone-d5	4.20	46	237127	43.19	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.38%
24) Chloroform-d	4.64	84	218164	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.80%
26) 1,2-Dichloroethane-d4	5.31	65	107709	4.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.80%
32) Benzene-d6	5.33	84	443439	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.00%
36) 1,2-Dichloropropane-d6	6.33	67	127916	3.91	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	78.20%
41) Toluene-d8	7.56	98	360545	3.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.60%
43) trans-1,3-Dichloropropene-	7.85	79	41161	3.27	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	65.40%
46) 2-Hexanone-d5	8.31	63	199004	42.05	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.10%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	102553	3.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	63.20%#
64) 1,2-Dichlorobenzene-d4	11.86	152	130993	3.45	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	69.00%#


Target Compounds					Ovalue
47) Tetrachloroethene	8.22	164	101277	9.521 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU052319\
Data File : VU032279.D
Acq On : 23 May 2019 19:28
Operator : JC/SP
Sample : K2888-05DL 5X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BN7DL

Quant Time: May 24 04:04:09 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR052219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 24 02:55:50 2019
Response via : Initial Calibration

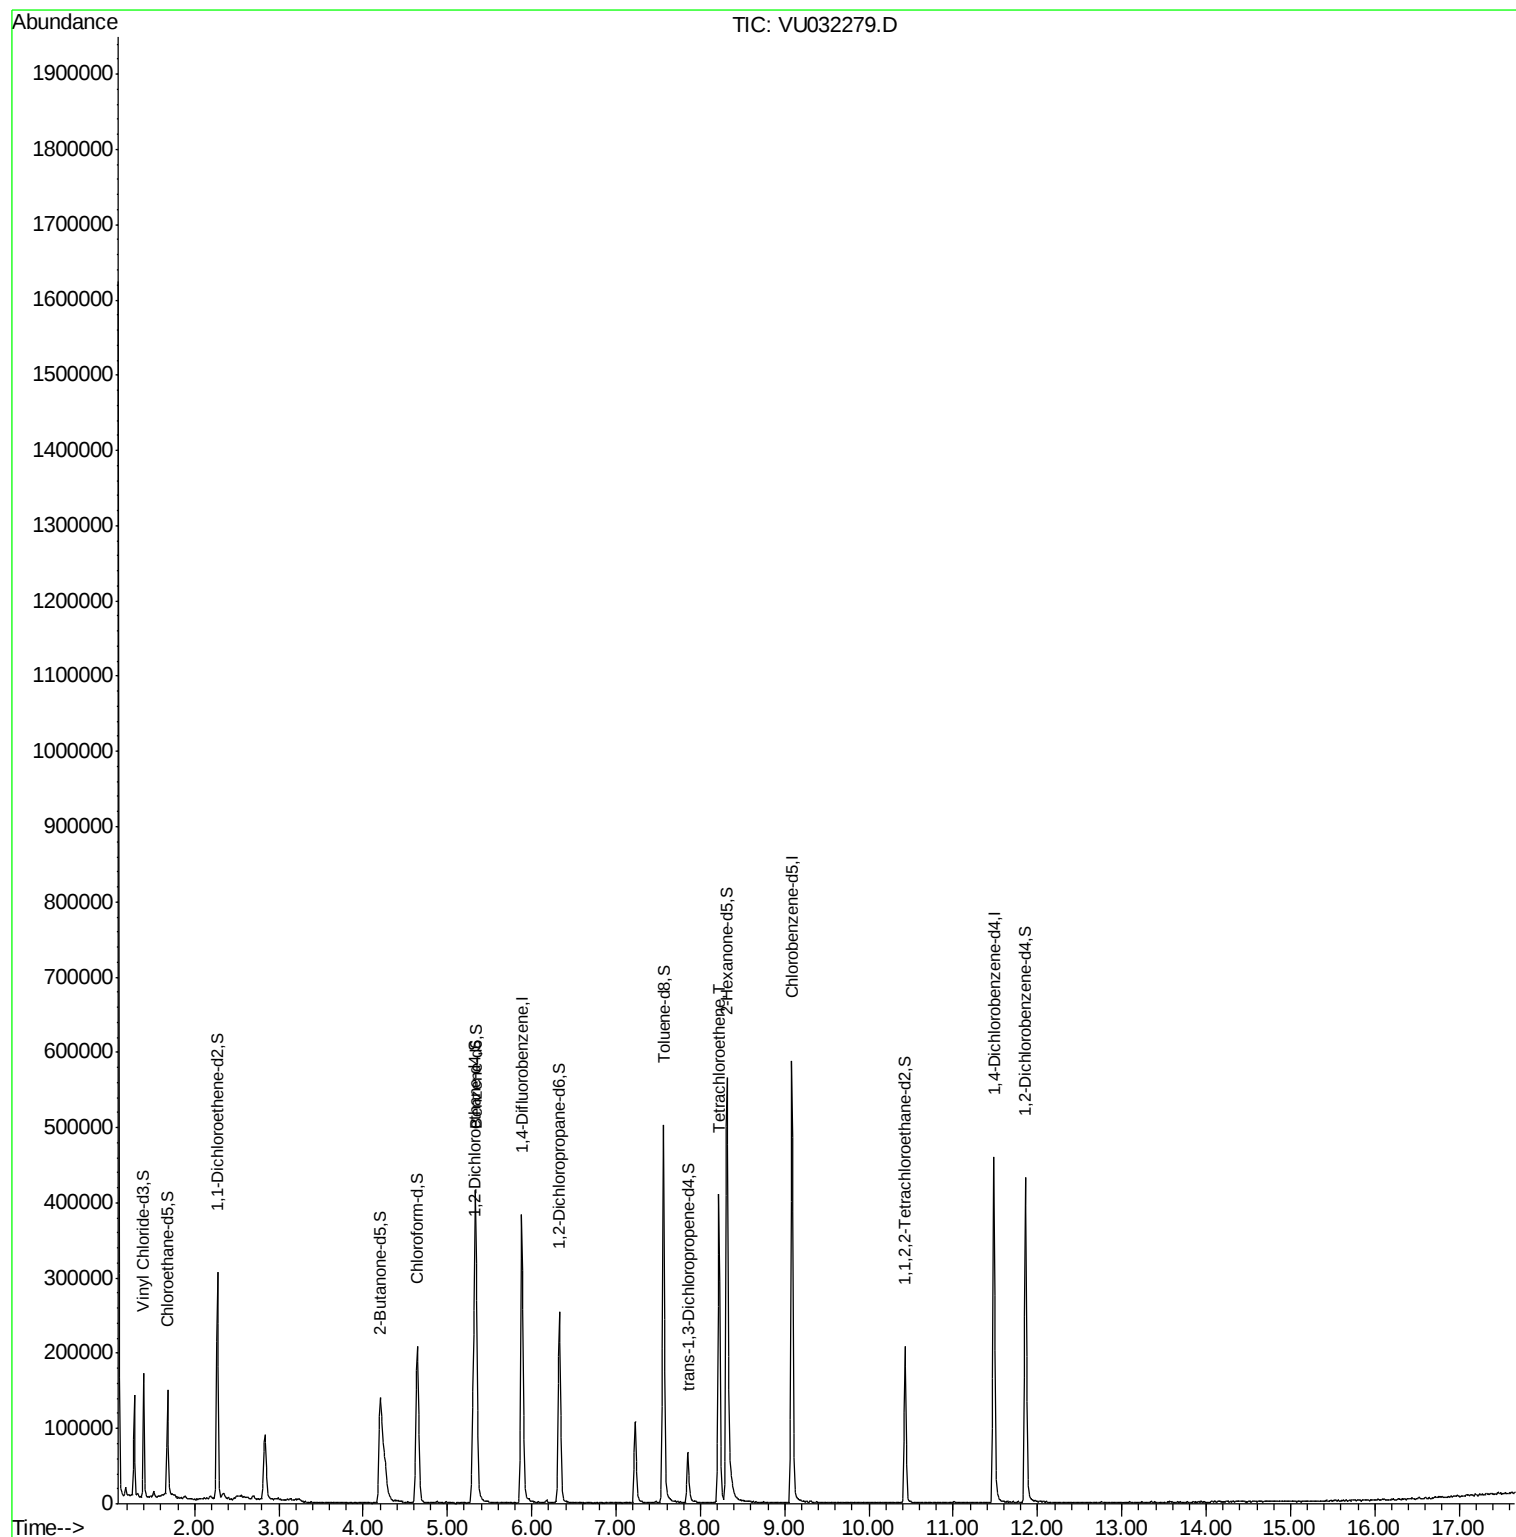

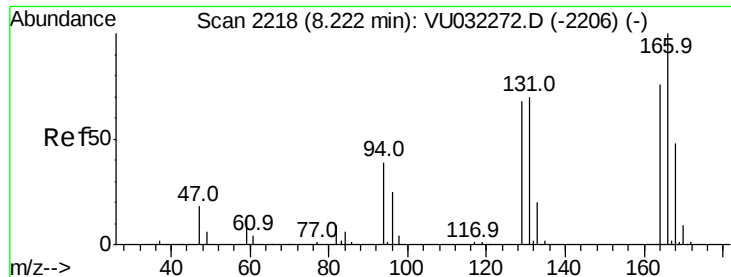

#47

Tetrachloroethene

Concen: 9.521 ug/L

RT: 8.22 min Scan# 2218

Delta R.T. 0.00 min

Lab File: VU032279.D


Acq: 23 May 2019 19:28

Instrument :

MSVOA_U

ClientSampleId :

C0BN7DL

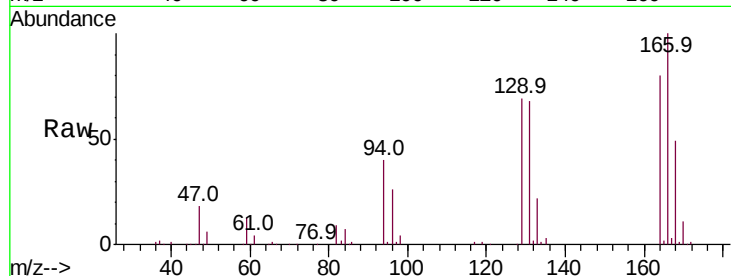

Tot Ion:164 Resp: 101277

Ion Ratio Lower Upper

164 100

129 85.6 67.1 124.7

131 84.8 62.2 115.4

166 124.6 90.9 168.9

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

