


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052319\
 Data File : VU032256.D
 Acq On : 23 May 2019 08:25
 Operator : JC/SP
 Sample : BFB12
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB12

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR052219WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri May 24 13:57:06 2019

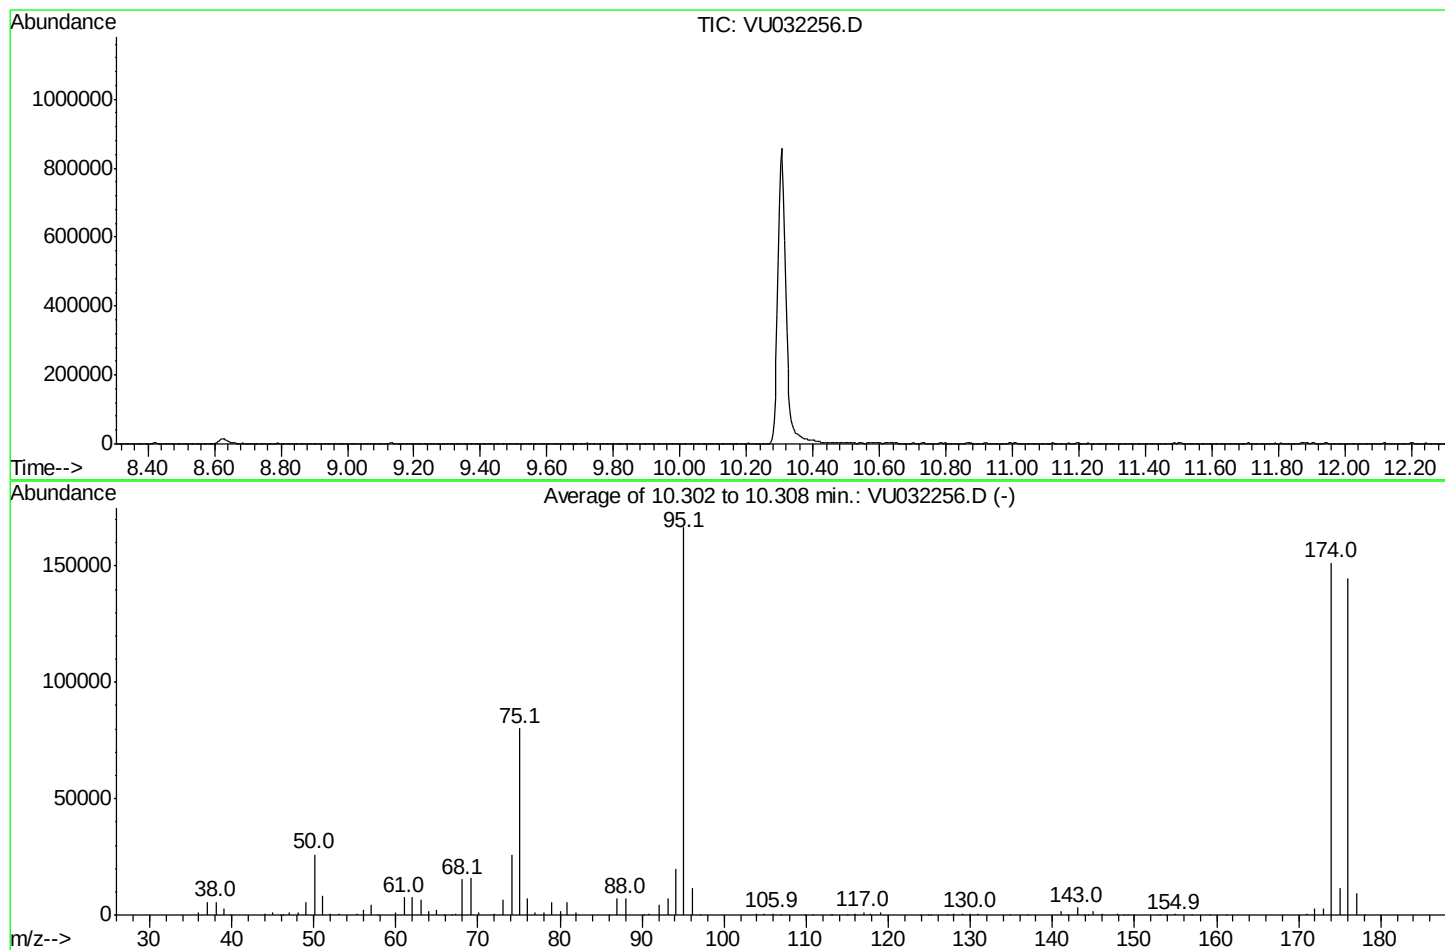

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	26157	PASS
75	95	30	80	48.1	80200	PASS
95	95	100	100	100.0	166677	PASS
96	95	5	9	7.0	11609	PASS
173	174	0.00	2	1.9	2939	PASS
174	95	50	120	91.0	151616	PASS
175	174	5	9	7.6	11554	PASS
176	174	95	101	95.4	144682	PASS
177	176	5	9	6.5	9383	PASS

Scan 2852 (10.260 min): VU032256.D
BFB12

m/z	Abundance
39.90	679.0
44.00	568.0
64.10	203.0
77.10	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
35.90	919.0
37.00	5352.0
38.00	5147.0
39.10	2863.0
39.90	748.0
44.00	1092.0
45.00	1126.0
45.90	155.0
47.00	1434.0
48.20	851.0
49.10	5466.0
50.00	26304.0
51.10	8206.0
52.00	415.0
53.00	304.0
55.30	357.0
56.00	2237.0
57.10	4127.0
60.00	1388.0
61.00	7109.0
62.00	7695.0
63.00	6294.0
64.00	1813.0
65.00	1909.0
65.90	247.0
66.80	240.0
67.20	315.0
68.10	15366.0
69.10	15689.0
70.10	1259.0
72.00	934.0
73.00	6474.0
74.10	25944.0
75.10	79240.0
76.10	7229.0
77.00	1081.0
78.00	885.0
79.00	5870.0
80.00	1437.0
80.90	5720.0
82.00	1235.0
86.00	318.0
87.00	6887.0
88.00	6599.0
90.90	539.0
92.00	4195.0
93.10	6760.0
94.10	20056.0
95.10	163520.0
96.10	11758.0
97.20	254.0
104.00	560.0
104.90	413.0
106.00	676.0
107.00	224.0
110.80	168.0
112.90	117.0
115.00	283.0
115.90	491.0
117.00	1286.0
117.80	450.0
119.00	1161.0
127.20	104.0
128.00	638.0
129.10	398.0
130.00	632.0
131.00	296.0
137.00	269.0
141.10	1416.0
141.90	145.0
143.00	3345.0
143.90	139.0
145.00	1495.0
146.00	294.0
147.90	289.0
148.70	130.0
149.20	195.0
149.90	254.0
154.90	587.0
156.90	167.0
161.10	159.0
171.10	826.0
172.00	2950.0
173.10	2734.0
174.00	145984.0
175.00	10968.0
176.00	139072.0
177.00	9561.0
178.00	257.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
36.00	919.0
37.10	5266.0
38.10	5899.0
39.10	3245.0
39.90	725.0
44.00	1132.0
45.00	1000.0
46.10	203.0
47.00	1325.0
48.10	849.0
49.10	5704.0
50.10	27000.0
51.10	8459.0
52.00	349.0
53.10	357.0
55.20	372.0
56.00	2381.0
57.10	4424.0
59.90	1431.0
61.00	7889.0
62.00	8235.0
63.10	6527.0
64.10	1683.0
65.00	2138.0
65.90	269.0
67.20	360.0
68.10	15724.0
69.10	16440.0
70.10	1345.0
72.00	841.0
73.00	7096.0
74.10	26672.0
75.10	82432.0
76.10	7347.0
77.00	1194.0
78.00	962.0
79.00	5860.0
80.00	1825.0
80.90	5631.0
81.90	1363.0
86.10	369.0
87.00	7060.0
88.00	7199.0
90.90	605.0
92.00	4643.0
93.10	7204.0
94.10	20904.0
95.10	172096.0
96.10	12208.0
97.00	257.0
104.00	588.0
104.90	488.0
105.90	828.0
106.90	176.0
110.90	218.0
113.10	116.0
115.00	296.0
115.90	511.0
117.00	1345.0
117.80	504.0
119.00	979.0
124.90	108.0
125.10	106.0
128.00	564.0
129.10	429.0
130.00	680.0
130.90	365.0
137.00	250.0
141.10	1455.0
141.90	220.0
143.00	3362.0
144.20	174.0
145.00	1434.0
146.10	369.0
147.90	336.0
149.10	200.0
150.00	252.0
153.10	154.0
154.90	546.0
156.90	182.0
159.10	115.0
161.10	127.0
171.10	844.0
172.00	3130.0
173.10	3130.0
174.00	156160.0
175.00	11887.0
176.00	148544.0
177.00	9691.0
178.00	273.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
36.00	980.0
37.10	5232.0
38.10	5653.0
39.00	2861.0
40.00	707.0
44.00	1163.0
45.00	894.0
46.20	295.0
47.00	1181.0
48.00	880.0
49.10	5382.0
50.10	25168.0
51.10	8052.0
52.00	287.0
53.10	351.0
55.20	384.0
56.00	2073.0
57.00	4331.0
57.80	108.0
59.90	1380.0
61.00	7867.0
62.00	7874.0
63.10	6411.0
64.10	1450.0
65.00	2209.0
65.90	235.0
67.20	346.0
68.10	14769.0
69.10	15312.0
70.10	1196.0
71.90	645.0
73.00	7079.0
74.10	25336.0
75.10	78928.0
76.00	6684.0
77.00	1205.0
78.00	840.0
79.00	5505.0
80.00	1854.0
80.90	5149.0
81.90	1278.0
87.00	7017.0
88.00	7219.0
90.20	117.0
90.90	592.0
92.00	4325.0
93.10	6991.0
94.10	19000.0
95.10	164416.0
96.10	10862.0
96.90	214.0
103.90	631.0
104.90	445.0
105.80	786.0
106.80	182.0
109.90	132.0
110.90	253.0
113.10	160.0
114.90	251.0
115.90	508.0
117.00	1177.0
117.90	529.0
119.00	781.0
123.90	106.0
125.20	132.0
128.00	439.0
129.10	364.0
130.00	638.0
130.90	347.0
134.80	114.0
137.00	244.0
141.00	1439.0
141.90	371.0
143.00	3119.0
144.30	254.0
144.90	1512.0
146.10	389.0
147.90	285.0
149.00	210.0
150.00	208.0
153.10	147.0
153.90	113.0
154.90	459.0
157.00	251.0
159.10	150.0
171.00	796.0
172.00	2862.0
173.10	2953.0
174.00	152704.0
175.00	11809.0
176.00	146432.0
177.00	8899.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

178.00

213.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12