

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052322\
 Data File : VU048651.D
 Acq On : 23 May 2022 11:45
 Operator : SY/MD
 Sample : VU0523MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK136

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048651.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	104	rVB	57311	67196	8.33%	1.008%
2	1.916	170	179	191	rVB	55950	69958	8.67%	1.049%
3	2.568	370	382	400	rBV	148803	243408	30.17%	3.650%
4	2.745	433	437	439	rBV	184	186	0.02%	0.003%
5	3.018	519	522	525	rBV	213	184	0.02%	0.003%
6	3.044	525	530	538	rVB3	1002	1406	0.17%	0.021%
7	3.182	569	573	576	rBV3	651	665	0.08%	0.010%
8	3.420	643	647	651	rBB	185	201	0.02%	0.003%
9	3.552	684	688	691	rBB	186	161	0.02%	0.002%
10	3.742	744	747	750	rBB	182	143	0.02%	0.002%
11	3.790	759	762	765	rBV	295	215	0.03%	0.003%
12	3.819	768	771	774	rBB	186	139	0.02%	0.002%
13	4.166	875	879	882	rBB	213	178	0.02%	0.003%
14	4.581	1005	1008	1010	rBV	341	247	0.03%	0.004%
15	4.629	1010	1023	1047	rBV	86138	223096	27.66%	3.346%
16	4.880	1095	1101	1104	rVB3	554	564	0.07%	0.008%
17	4.906	1105	1109	1110	rBV	366	231	0.03%	0.003%
18	5.067	1143	1159	1182	rBV2	162527	361221	44.78%	5.417%
19	5.301	1229	1232	1234	rVB	286	179	0.02%	0.003%
20	5.378	1253	1256	1258	rBB	268	149	0.02%	0.002%
21	5.539	1302	1306	1308	rBB	244	147	0.02%	0.002%
22	5.729	1343	1365	1386	rBV3	288624	806709	100.00%	12.098%
23	5.883	1411	1413	1416	rVB2	405	205	0.03%	0.003%
24	5.938	1428	1430	1433	rVB	340	176	0.02%	0.003%
25	6.041	1459	1462	1464	rBV	264	225	0.03%	0.003%
26	6.066	1468	1470	1473	rBB	282	153	0.02%	0.002%
27	6.111	1481	1484	1488	rBB2	298	231	0.03%	0.003%
28	6.250	1513	1527	1547	rBV	253326	483013	59.87%	7.244%
29	6.372	1562	1565	1567	rBV2	241	159	0.02%	0.002%
30	6.433	1581	1584	1588	rBB	231	198	0.02%	0.003%
31	6.533	1603	1615	1625	rBB5	5162	9866	1.22%	0.148%
32	6.571	1626	1627	1631	rBV	223	154	0.02%	0.002%
33	6.693	1651	1665	1690	rBB2	184243	363050	45.00%	5.445%
34	6.787	1691	1694	1696	rBV2	301	209	0.03%	0.003%
35	6.803	1696	1699	1701	rBV	446	265	0.03%	0.004%
36	6.854	1711	1715	1717	rBB	278	179	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052322\
 Data File : VU048651.D
 Acq On : 23 May 2022 11:45
 Operator : SY/MD
 Sample : VU0523MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK136

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	6.893	1724	1727	1730	rBB2	265	151	0.02%	0.002%
38	7.108	1790	1794	1797	rBB	151	156	0.02%	0.002%
39	7.189	1810	1819	1827	rBV6	1652	2434	0.30%	0.037%
40	7.250	1834	1838	1841	rBB	144	149	0.02%	0.002%
41	7.568	1925	1937	1956	rBV	112843	198769	24.64%	2.981%
42	7.697	1966	1977	1988	rBB5	1309	2499	0.31%	0.037%
43	7.751	1991	1994	1996	rBV	249	169	0.02%	0.003%
44	7.793	2003	2007	2009	rBV	569	485	0.06%	0.007%
45	7.899	2027	2040	2057	rBV	370787	638601	79.16%	9.577%
46	8.182	2115	2128	2144	rBV	81662	143136	17.74%	2.147%
47	8.539	2236	2239	2244	rBB2	281	234	0.03%	0.004%
48	8.635	2257	2269	2298	rBV	271185	501163	62.12%	7.516%
49	8.841	2331	2333	2339	rBB	251	235	0.03%	0.004%
50	8.867	2339	2341	2343	rBB	284	148	0.02%	0.002%
51	8.928	2358	2360	2363	rVB2	299	163	0.02%	0.002%
52	8.999	2379	2382	2385	rBV	219	162	0.02%	0.002%
53	9.070	2400	2404	2407	rBB	278	232	0.03%	0.003%
54	9.121	2418	2420	2424	rBB	299	191	0.02%	0.003%
55	9.189	2436	2441	2444	rBB	195	196	0.02%	0.003%
56	9.288	2468	2472	2480	rVB	305	468	0.06%	0.007%
57	9.420	2500	2513	2528	rBV	374676	617712	76.57%	9.264%
58	9.562	2550	2557	2558	rBV2	370	342	0.04%	0.005%
59	9.635	2576	2580	2583	rBB2	342	248	0.03%	0.004%
60	9.664	2584	2589	2594	rBV	181	296	0.04%	0.004%
61	9.697	2594	2599	2601	rBV	565	466	0.06%	0.007%
62	9.787	2624	2627	2630	rBB	300	197	0.02%	0.003%
63	9.854	2645	2648	2650	rBV	174	140	0.02%	0.002%
64	9.912	2661	2666	2669	rBV	322	249	0.03%	0.004%
65	9.951	2676	2678	2681	rBV	278	179	0.02%	0.003%
66	10.002	2690	2694	2698	rBB	178	185	0.02%	0.003%
67	10.105	2722	2726	2728	rBV2	606	377	0.05%	0.006%
68	10.147	2736	2739	2744	rBV	156	198	0.02%	0.003%
69	10.491	2840	2846	2851	rVB4	708	751	0.09%	0.011%
70	10.552	2861	2865	2868	rBV	198	215	0.03%	0.003%
71	10.635	2885	2891	2899	rBV3	1000	1623	0.20%	0.024%
72	10.758	2916	2929	2948	rBV	300487	489095	60.63%	7.335%
73	10.835	2948	2953	2956	rBV2	234	239	0.03%	0.004%
74	10.989	2991	3001	3003	rBV	327	549	0.07%	0.008%
75	11.018	3007	3010	3014	rVB	358	263	0.03%	0.004%
76	11.044	3014	3018	3022	rBB	267	251	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052322\
 Data File : VU048651.D
 Acq On : 23 May 2022 11:45
 Operator : SY/MD
 Sample : VU0523MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK136

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	11.082	3026	3030	3031	rBV	346	262	0.03%	0.004%
78	11.475	3144	3152	3162	rVB3	988	1618	0.20%	0.024%
79	11.552	3173	3176	3177	rBV3	311	158	0.02%	0.002%
80	11.748	3232	3237	3245	rVB4	1341	1618	0.20%	0.024%
81	11.812	3245	3257	3275	rBV	429120	679508	84.23%	10.191%
82	12.195	3363	3376	3392	rBV	442094	719600	89.20%	10.792%
83	12.362	3425	3428	3432	rVB2	261	178	0.02%	0.003%
84	12.388	3432	3436	3438	rBV2	356	205	0.03%	0.003%
85	12.587	3495	3498	3500	rVV2	293	205	0.03%	0.003%
86	12.680	3524	3527	3532	rBV	161	200	0.02%	0.003%
87	12.938	3604	3607	3611	rBV	373	211	0.03%	0.003%
88	13.121	3661	3664	3666	rBV	260	138	0.02%	0.002%
89	13.188	3682	3685	3688	rBV2	244	193	0.02%	0.003%
90	13.224	3690	3696	3704	rVV4	1188	1386	0.17%	0.021%
91	13.256	3704	3706	3710	rVB	335	182	0.02%	0.003%
92	13.291	3715	3717	3719	rBV	220	147	0.02%	0.002%
93	13.516	3784	3787	3793	rVB2	340	308	0.04%	0.005%
94	13.745	3856	3858	3861	rBV	372	241	0.03%	0.004%
95	13.848	3881	3890	3896	rBV5	2539	3828	0.47%	0.057%
96	14.053	3951	3954	3956	rBV2	406	232	0.03%	0.003%
97	14.092	3956	3966	3978	rVV	9864	15484	1.92%	0.232%
98	14.188	3994	3996	4000	rBV2	340	223	0.03%	0.003%
99	14.333	4036	4041	4049	rVB5	2811	3337	0.41%	0.050%
100	15.510	4406	4407	4412	rVB	894	406	0.05%	0.006%




Sum of corrected areas: 6667850

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052322\
Data File : VU048651.D
Acq On : 23 May 2022 11:45
Operator : SY/MD
Sample : VU0523MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK136

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

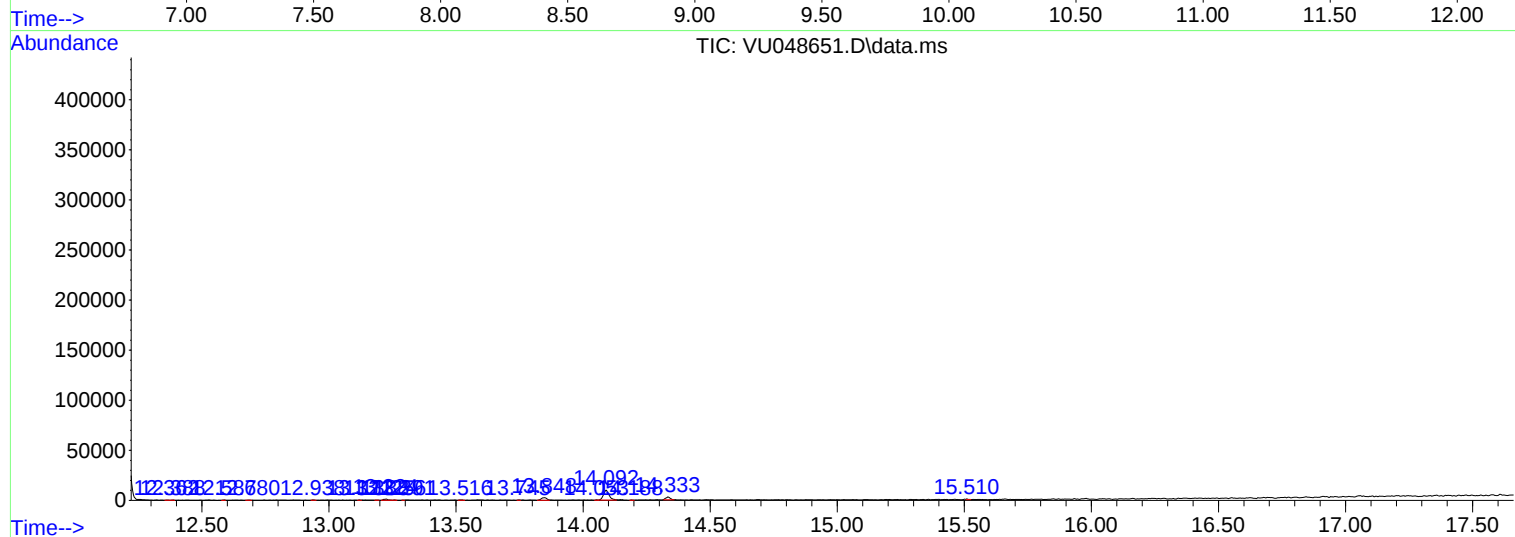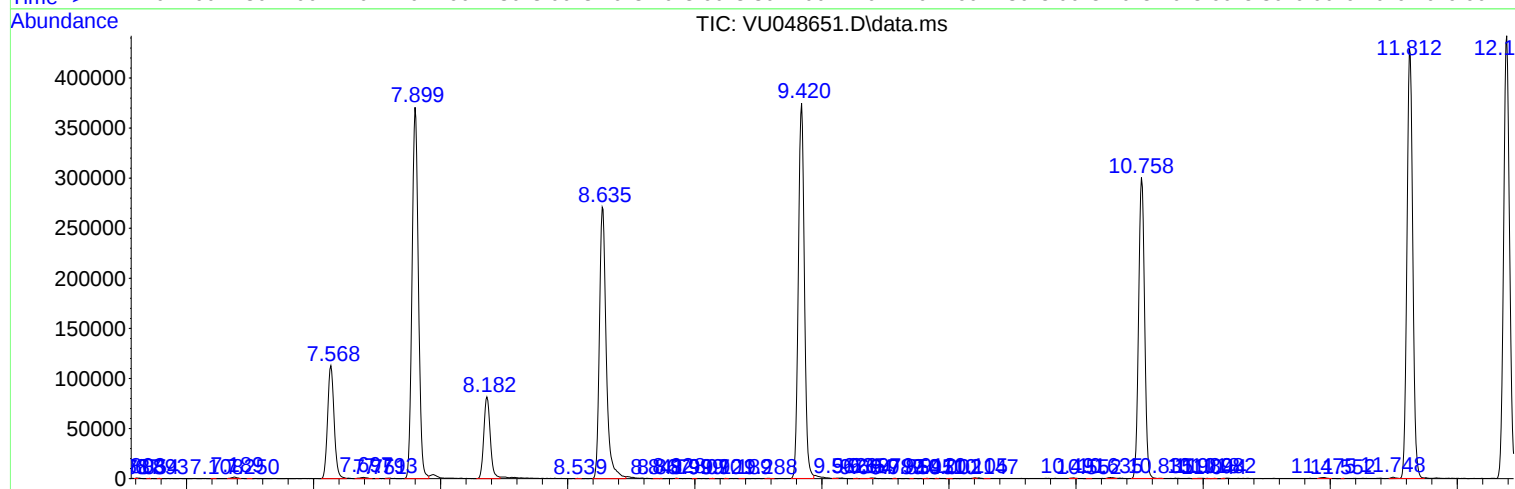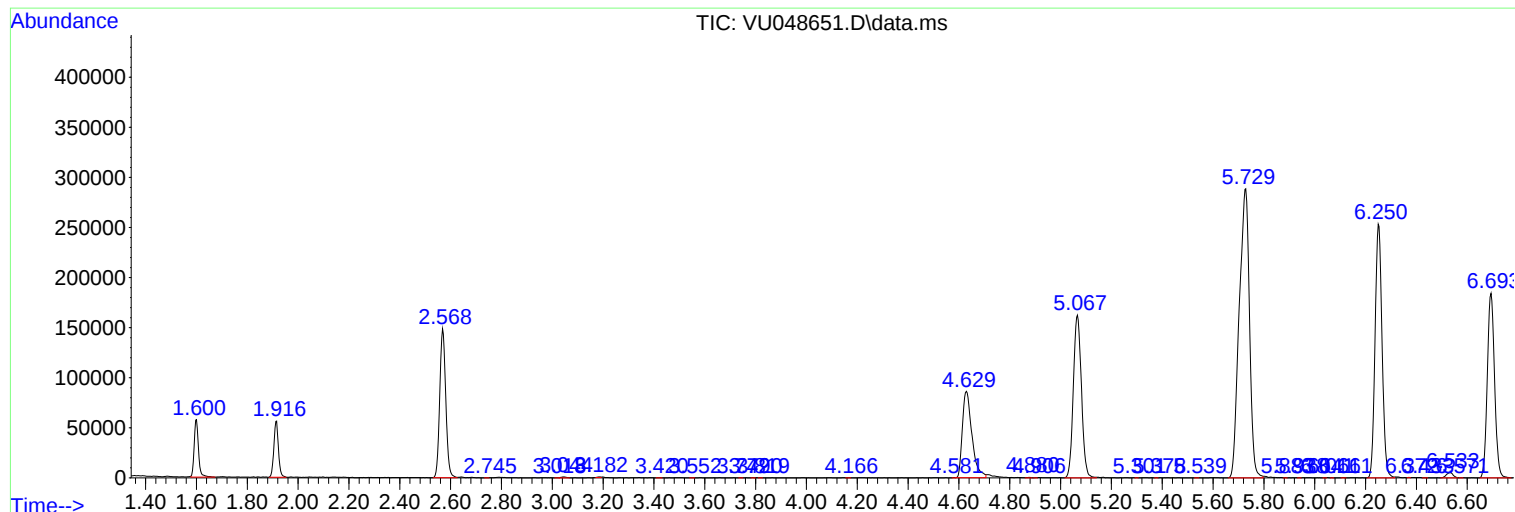

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052322\
Data File : VU048651.D
Acq On : 23 May 2022 11:45
Operator : SY/MD
Sample : VU0523MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK136

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052322\
Data File : VU048651.D
Acq On : 23 May 2022 11:45
Operator : SY/MD
Sample : VU0523MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK136

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------