

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052322\
 Data File : VU048653.D
 Acq On : 23 May 2022 14:08
 Operator : SY/MD
 Sample : N2929-01ME
 Misc : 8.37g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBTF7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M

Title : VOC Analysis

Signal : TIC: VU048653.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	85	rBV	34602	43771	5.52%	0.659%
2	2.305	298	300	305	rVB2	400	246	0.03%	0.004%
3	2.343	310	312	315	rBV2	311	168	0.02%	0.003%
4	2.391	326	327	329	rBV2	381	192	0.02%	0.003%
5	2.536	362	372	385	rVB	128795	203850	25.70%	3.069%
6	2.697	420	422	425	rVB	358	197	0.02%	0.003%
7	2.713	425	427	429	rBV	432	252	0.03%	0.004%
8	2.745	434	437	440	rVB2	322	207	0.03%	0.003%
9	2.800	451	454	461	rBB	211	264	0.03%	0.004%
10	2.954	487	502	520	rBV	36473	72167	9.10%	1.086%
11	3.182	560	573	584	rBV2	5863	12455	1.57%	0.187%
12	3.340	619	622	623	rBV	255	154	0.02%	0.002%
13	3.504	671	673	676	rBV	194	152	0.02%	0.002%
14	3.575	692	695	696	rBV2	393	247	0.03%	0.004%
15	4.015	828	832	835	rBB	174	163	0.02%	0.002%
16	4.189	882	886	889	rBB	190	153	0.02%	0.002%
17	4.211	890	893	895	rBV	251	185	0.02%	0.003%
18	4.295	913	919	921	rBV	202	242	0.03%	0.004%
19	4.462	965	971	982	rVV3	1160	1950	0.25%	0.029%
20	4.636	1012	1025	1070	rBV	61466	202305	25.50%	3.045%
21	4.877	1097	1100	1104	rBV2	405	310	0.04%	0.005%
22	5.063	1141	1158	1185	rBB	139719	326517	41.16%	4.915%
23	5.173	1189	1192	1194	rBB	349	196	0.02%	0.003%
24	5.292	1224	1229	1236	rBV3	419	618	0.08%	0.009%
25	5.321	1236	1238	1241	rVB	314	216	0.03%	0.003%
26	5.343	1241	1245	1246	rBV	530	373	0.05%	0.006%
27	5.443	1272	1276	1281	rBB2	411	430	0.05%	0.006%
28	5.497	1291	1293	1298	rBV	186	190	0.02%	0.003%
29	5.716	1342	1361	1382	rBV2	286519	744803	93.89%	11.212%
30	5.973	1435	1441	1445	rBV5	1025	1262	0.16%	0.019%
31	6.063	1467	1469	1474	rBB	244	191	0.02%	0.003%
32	6.121	1479	1487	1489	rBB	359	329	0.04%	0.005%
33	6.144	1489	1494	1500	rBB2	766	799	0.10%	0.012%
34	6.247	1512	1526	1547	rBV	273064	538126	67.84%	8.101%
35	6.407	1574	1576	1580	rBB	526	226	0.03%	0.003%
36	6.523	1604	1612	1625	rBB6	4408	7785	0.98%	0.117%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052322\
 Data File : VU048653.D
 Acq On : 23 May 2022 14:08
 Operator : SY/MD
 Sample : N2929-01ME
 Misc : 8.37g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBTF7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	6.603	1628	1637	1645	rBV3	1533	2489	0.31%	0.037%
38	6.690	1650	1664	1683	rBV	163329	332655	41.94%	5.008%
39	6.803	1694	1699	1705	rBV2	632	841	0.11%	0.013%
40	6.851	1712	1714	1719	rBV	276	189	0.02%	0.003%
41	6.874	1719	1721	1725	rVB2	275	174	0.02%	0.003%
42	7.057	1772	1778	1781	rBV2	399	373	0.05%	0.006%
43	7.073	1781	1783	1787	rVB	351	267	0.03%	0.004%
44	7.195	1809	1821	1841	rBV4	6156	17213	2.17%	0.259%
45	7.356	1868	1871	1873	rBV	238	174	0.02%	0.003%
46	7.378	1873	1878	1885	rVV2	992	1126	0.14%	0.017%
47	7.568	1924	1937	1956	rBV2	93502	182518	23.01%	2.748%
48	7.681	1967	1972	1973	rBV2	963	709	0.09%	0.011%
49	7.787	1995	2005	2009	rBV3	1211	2040	0.26%	0.031%
50	7.899	2026	2040	2057	rBV	326257	587076	74.01%	8.838%
51	8.076	2089	2095	2096	rBV	394	453	0.06%	0.007%
52	8.182	2116	2128	2148	rVB	64462	130265	16.42%	1.961%
53	8.298	2162	2164	2167	rBV	299	201	0.03%	0.003%
54	8.414	2196	2200	2202	rBV	376	339	0.04%	0.005%
55	8.452	2209	2212	2213	rBV	443	215	0.03%	0.003%
56	8.552	2234	2243	2256	rVB3	13844	22435	2.83%	0.338%
57	8.658	2257	2276	2302	rBV	213032	482884	60.87%	7.269%
58	8.783	2310	2315	2317	rBV2	358	329	0.04%	0.005%
59	8.925	2354	2359	2360	rBV	465	340	0.04%	0.005%
60	8.980	2374	2376	2378	rBV	279	155	0.02%	0.002%
61	9.070	2401	2404	2407	rBV	235	207	0.03%	0.003%
62	9.099	2412	2413	2418	rBV	240	185	0.02%	0.003%
63	9.150	2427	2429	2432	rBV3	416	339	0.04%	0.005%
64	9.224	2449	2452	2455	rBV	180	164	0.02%	0.002%
65	9.423	2500	2514	2534	rBV	363388	689437	86.91%	10.378%
66	9.629	2572	2578	2581	rBB2	288	320	0.04%	0.005%
67	9.648	2581	2584	2587	rBV2	365	286	0.04%	0.004%
68	9.697	2593	2599	2606	rBV4	1177	1544	0.19%	0.023%
69	9.902	2660	2663	2667	rBV	224	245	0.03%	0.004%
70	10.362	2802	2806	2808	rBV2	296	269	0.03%	0.004%
71	10.410	2818	2821	2824	rBV	140	151	0.02%	0.002%
72	10.468	2830	2839	2849	rVB8	4036	6700	0.84%	0.101%
73	10.513	2849	2853	2857	rBV	305	326	0.04%	0.005%
74	10.668	2899	2901	2903	rBV2	559	321	0.04%	0.005%
75	10.713	2910	2915	2918	rBV	357	352	0.04%	0.005%
76	10.764	2918	2931	2945	rBV	293410	486241	61.30%	7.320%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052322\
 Data File : VU048653.D
 Acq On : 23 May 2022 14:08
 Operator : SY/MD
 Sample : N2929-01ME
 Misc : 8.37g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBTF7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	10.870	2960	2964	2965	rBV	431	245	0.03%	0.004%
78	10.886	2967	2969	2971	rBV2	592	367	0.05%	0.006%
79	10.980	2994	2998	3000	rBV	209	190	0.02%	0.003%
80	11.118	3033	3041	3044	rBV5	3037	3865	0.49%	0.058%
81	11.266	3084	3087	3094	rBV	210	177	0.02%	0.003%
82	11.455	3139	3146	3147	rBV2	907	700	0.09%	0.011%
83	11.526	3166	3168	3170	rBV2	219	155	0.02%	0.002%
84	11.697	3216	3221	3227	rBV4	578	674	0.08%	0.010%
85	11.748	3232	3237	3246	rBV6	2012	2581	0.33%	0.039%
86	11.815	3246	3258	3276	rBV	497937	793250	100.00%	11.941%
87	11.918	3285	3290	3295	rVB4	779	604	0.08%	0.009%
88	11.944	3295	3298	3302	rBV3	584	450	0.06%	0.007%
89	12.198	3364	3377	3392	rBV	420648	682515	86.04%	10.274%
90	12.333	3414	3419	3427	rVB4	1698	2080	0.26%	0.031%
91	12.922	3600	3602	3605	rBB	380	184	0.02%	0.003%
92	12.963	3613	3615	3619	rVB	353	186	0.02%	0.003%
93	13.365	3737	3740	3742	rBV2	269	157	0.02%	0.002%
94	13.378	3742	3744	3745	rVV	417	168	0.02%	0.003%
95	13.394	3745	3749	3754	rVB4	1536	1367	0.17%	0.021%
96	13.777	3865	3868	3872	rBV	377	286	0.04%	0.004%
97	14.166	3981	3989	3997	rVB2	7004	9015	1.14%	0.136%
98	14.256	4014	4017	4019	rBV	265	168	0.02%	0.003%
99	15.545	4415	4418	4421	rBV3	889	618	0.08%	0.009%
100	16.005	4553	4561	4575	rVB2	20208	28707	3.62%	0.432%




Sum of corrected areas: 6642947

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052322\
Data File : VU048653.D
Acq On : 23 May 2022 14:08
Operator : SY/MD
Sample : N2929-01ME
Misc : 8.37g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBTF7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

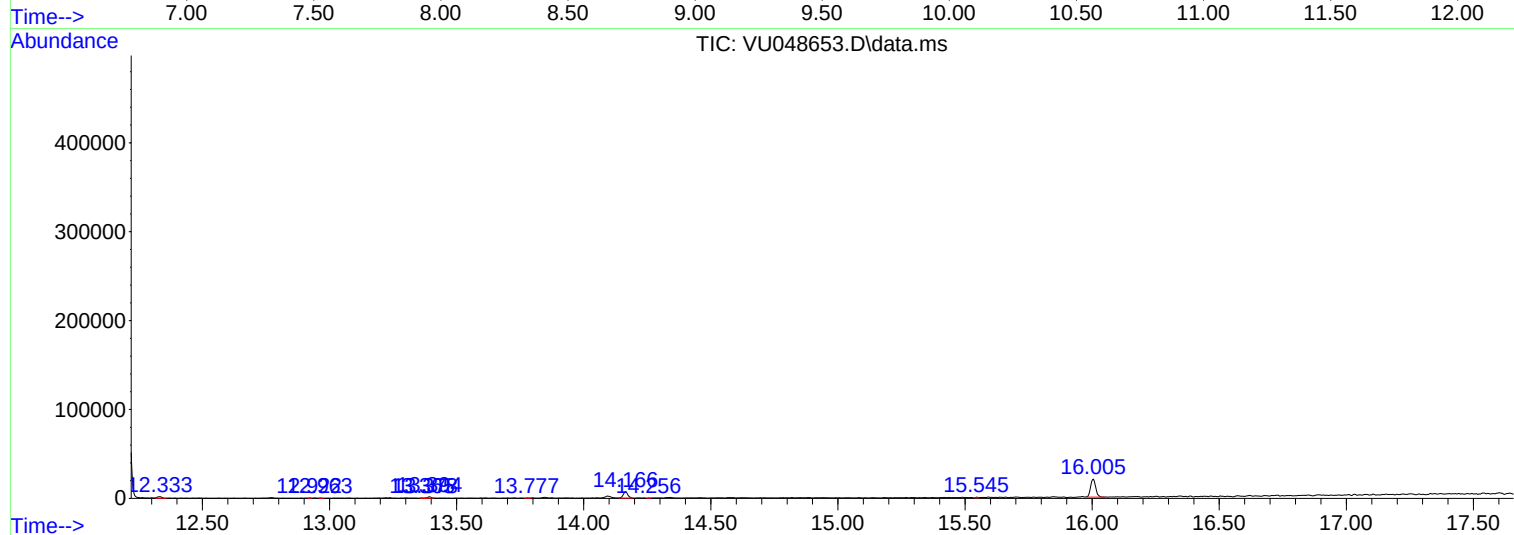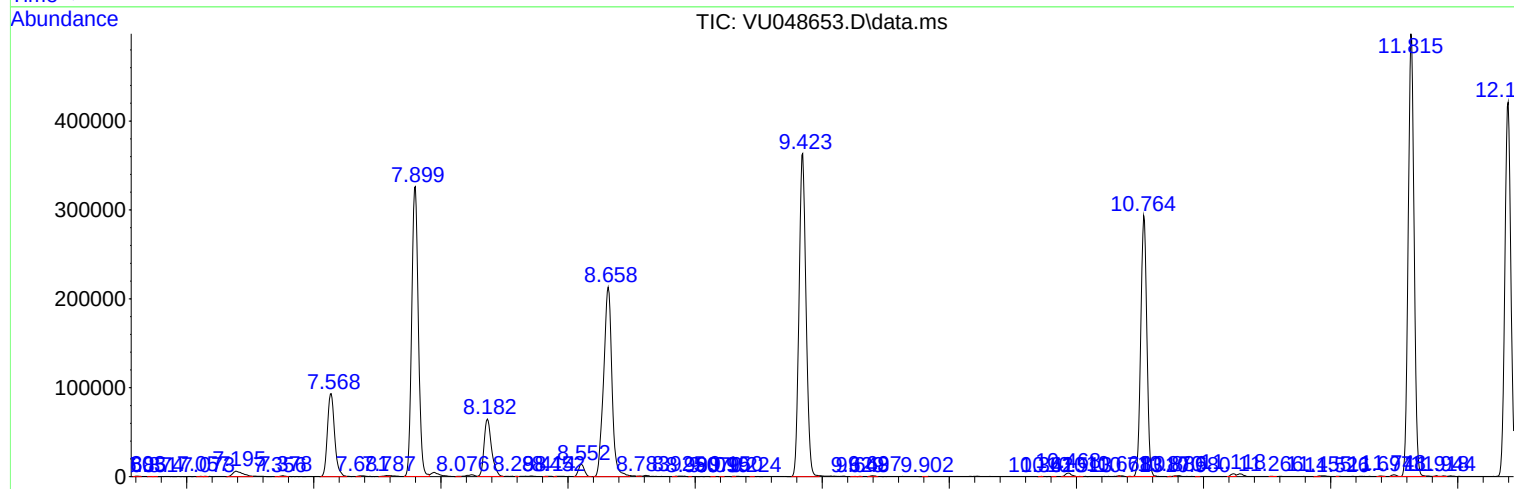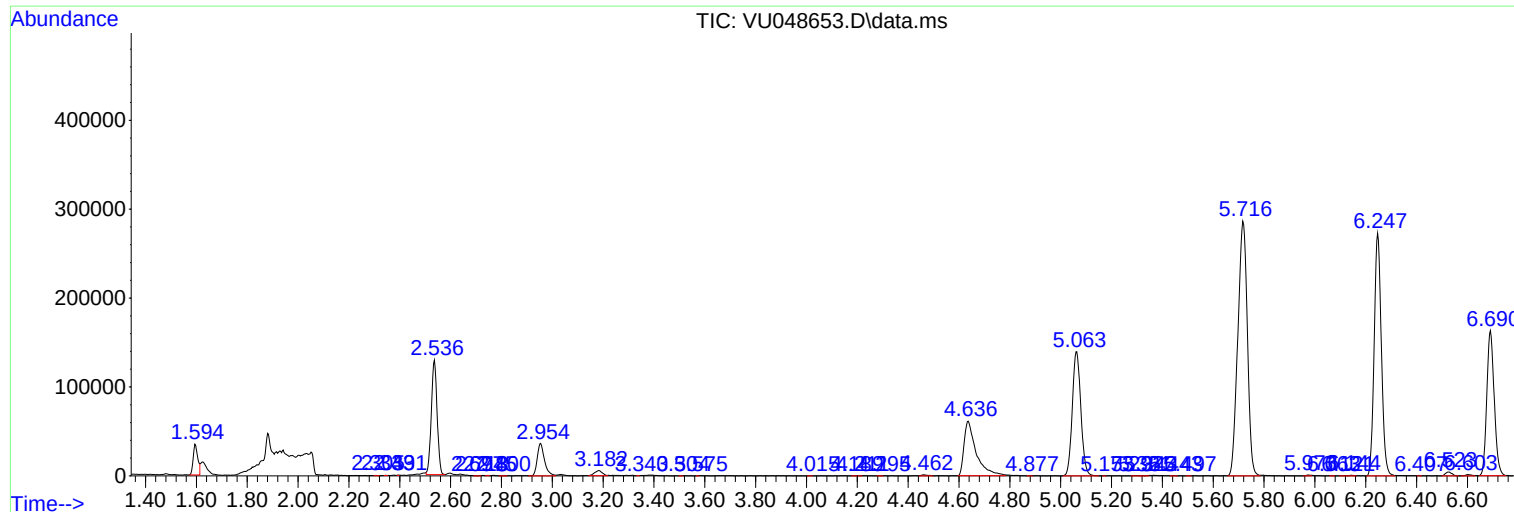

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052322\
Data File : VU048653.D
Acq On : 23 May 2022 14:08
Operator : SY/MD
Sample : N2929-01ME
Misc : 8.37g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBTF7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052322\
Data File : VU048653.D
Acq On : 23 May 2022 14:08
Operator : SY/MD
Sample : N2929-01ME
Misc : 8.37g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBTF7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc