


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052322\
 Data File : VU048649.D
 Acq On : 23 May 2022 09:17
 Operator : SY/MD
 Sample : BFB092
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB092

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis
 Last Update : Thu May 26 06:51:07 2022

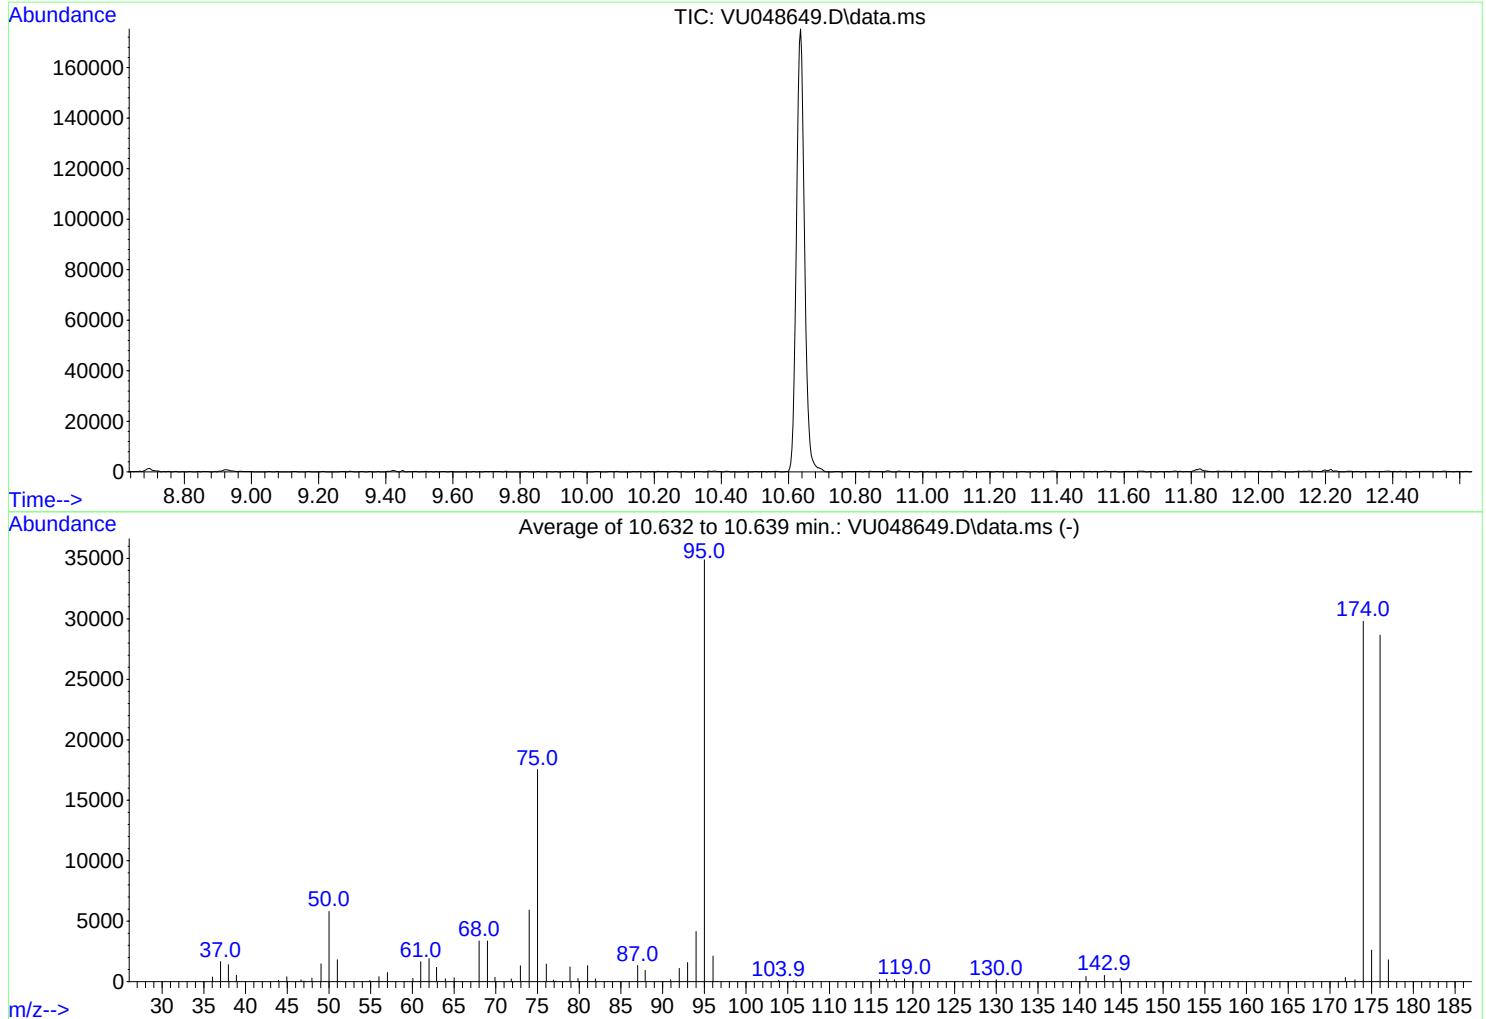

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	5813	PASS
75	95	30	80	50.3	17547	PASS
95	95	100	100	100.0	34883	PASS
96	95	5	9	6.1	2120	PASS
173	174	0.00	2	0.5	156	PASS
174	95	50	120	85.4	29800	PASS
175	174	5	9	8.8	2608	PASS
176	174	95	101	96.2	28667	PASS
177	176	5	9	6.3	1801	PASS

m/z	Abundance
44.00	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB092

m/z	Abundance
36.10	420.0
37.00	1774.0
38.00	1509.0
38.90	616.0
44.00	255.0
45.00	443.0
46.80	136.0
48.00	347.0
49.10	1422.0
50.00	5599.0
51.00	1706.0
54.90	155.0
56.00	346.0
57.00	768.0
60.10	278.0
61.00	1580.0
62.00	1977.0
62.90	1148.0
64.00	249.0
65.00	309.0
68.00	3576.0
69.00	3369.0
69.90	416.0
71.90	193.0
73.00	1293.0
74.00	6084.0
75.00	17312.0
76.10	1634.0
77.20	108.0
78.90	1164.0
79.90	275.0
81.00	1297.0
81.90	226.0
87.00	1170.0
87.90	1055.0
91.00	168.0
92.00	1039.0
93.00	1491.0
94.00	4228.0
95.00	35216.0
96.10	2035.0
103.90	151.0
116.00	156.0
116.90	207.0
117.80	175.0
119.00	191.0
128.00	114.0
130.00	157.0
140.80	378.0
142.90	586.0
144.90	285.0
147.90	124.0
171.90	333.0
173.00	468.0
174.00	29520.0
175.00	2645.0
176.00	28024.0
177.00	1796.0

Instrument :
MSVOA_U
ClientSampleId :
BFB092

m/z	Abundance
36.10	420.0
37.00	1715.0
38.00	1447.0
38.90	556.0
43.90	242.0
45.00	420.0
46.60	153.0
48.00	305.0
49.00	1523.0
50.00	6017.0
51.00	1903.0
54.90	129.0
56.00	407.0
57.00	768.0
60.10	279.0
61.00	1734.0
62.00	1976.0
62.90	1212.0
63.90	258.0
65.00	343.0
66.00	100.0
68.00	3451.0
69.00	3491.0
69.90	372.0
71.80	237.0
72.90	1372.0
74.00	6038.0
75.00	18104.0
76.00	1473.0
76.90	165.0
78.90	1274.0
79.80	246.0
81.00	1374.0
82.00	235.0
87.00	1387.0
87.90	957.0
91.00	163.0
92.00	1154.0
93.00	1644.0
94.00	4272.0
95.00	36016.0
96.00	2167.0
103.90	154.0
105.70	119.0
116.00	200.0
116.80	226.0
117.80	170.0
119.00	250.0
128.00	132.0
130.00	167.0
140.70	445.0
143.00	524.0
144.80	262.0
171.80	339.0
174.00	30552.0
175.00	2711.0
176.00	29576.0
177.00	1889.0

Instrument :
MSVOA_U
ClientSampleId :
BFB092

m/z	Abundance
36.00	333.0
37.00	1455.0
37.90	1252.0
38.90	419.0
43.90	233.0
44.90	329.0
46.60	172.0
47.00	162.0
47.90	222.0
49.00	1455.0
50.00	5823.0
51.00	1842.0
56.00	458.0
57.00	744.0
60.00	293.0
61.00	1666.0
62.00	1748.0
62.90	1176.0
63.90	223.0
65.00	292.0
68.00	3061.0
69.00	3223.0
69.90	287.0
71.80	235.0
72.90	1276.0
74.00	5623.0
75.00	17224.0
76.00	1260.0
76.90	229.0
78.90	1213.0
79.80	225.0
81.00	1304.0
82.00	211.0
87.00	1442.0
87.90	790.0
90.90	134.0
92.00	1100.0
93.00	1590.0
94.00	3930.0
95.00	33416.0
96.00	2158.0
105.70	133.0
116.00	216.0
116.80	206.0
117.80	136.0
119.00	263.0
128.00	118.0
130.00	153.0
140.80	462.0
143.00	450.0
144.80	202.0
171.80	358.0
174.00	29328.0
175.00	2468.0
176.00	28400.0
177.00	1719.0

Instrument :
MSVOA_U
ClientSampleId :
BFB092