

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\

Data File : VU032297.D

Acq On : 24 May 2019 08:40

Operator : JC/SP

Sample : K3001-15 50X

Misc : 5.0mL/MSVOA U/WATER

ALS Vial : 52 Sample Multiplier: 1

Quant Time: May 28 11:24:10 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M

Quant Title : VOC Analysis

QLast Update : Fri May 24 07:24:18 2019

Response via : Initial Calibration

Instrument :

MSVOA_U

Client Sample Id :


E3YF8

Manual Integrations

APPROVED

apatel

6/4/2019 8:33:35 AM

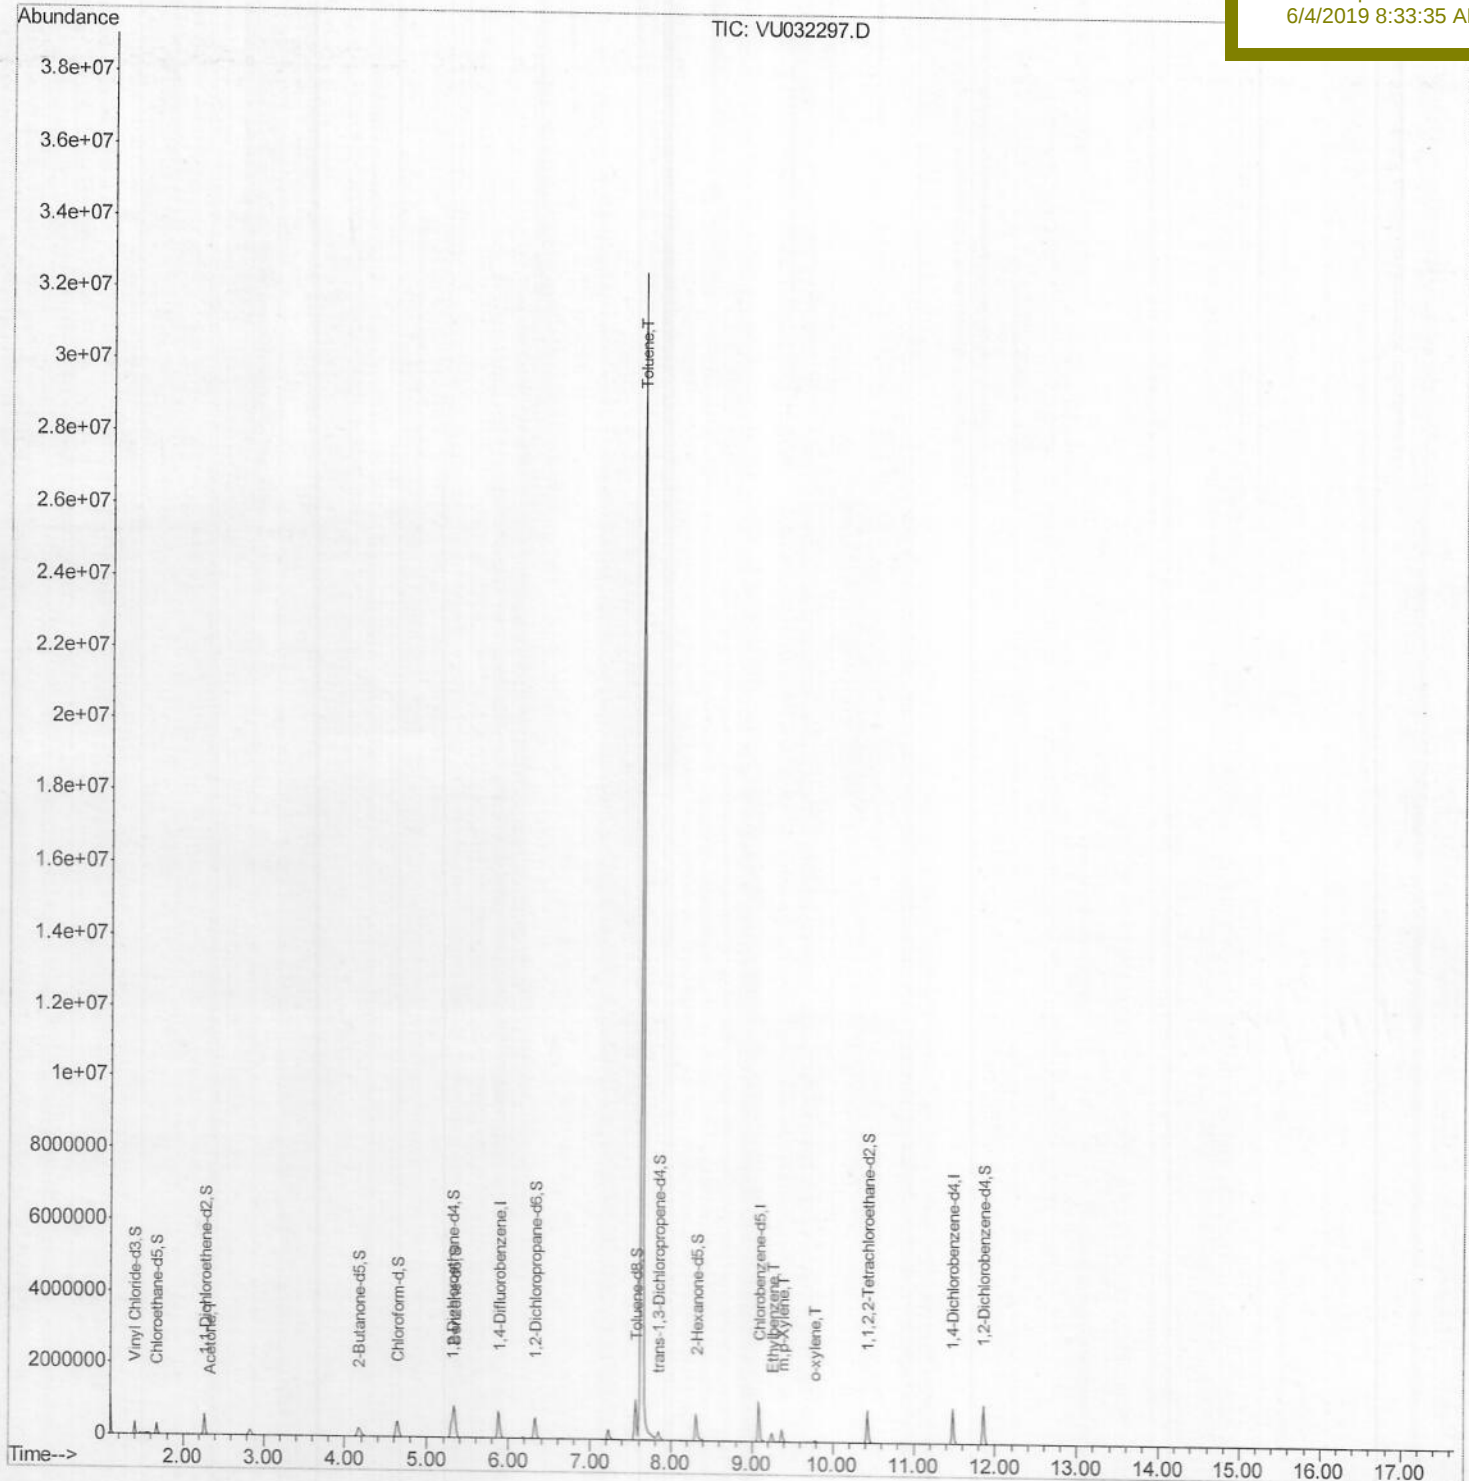

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU052419\
Quantitation Report (Qedit)




Data File : VU032297.D
Acq On : 24 May 2019 08:40
Operator : JC/SP
Sample : K3001-15 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Quant Time: May 25 01:31:06 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 24 07:24:18 2019
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
E3YF8

Manual Integrations
APPROVED

apatel
6/4/2019 8:33:35 AM

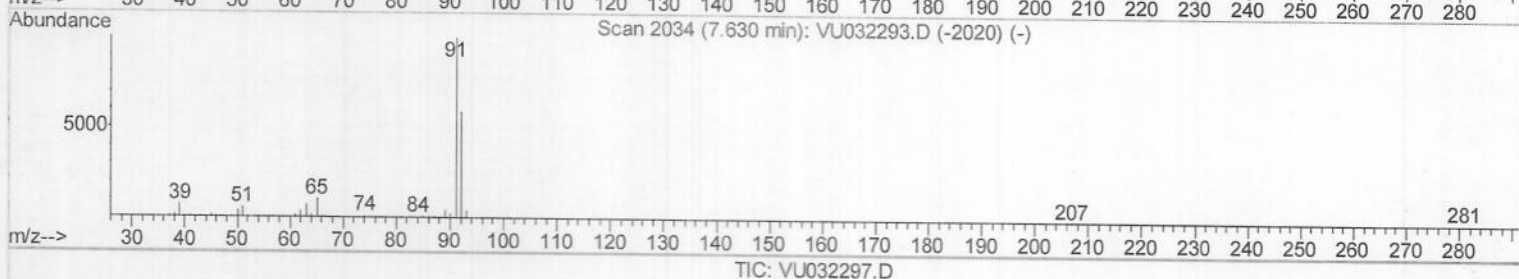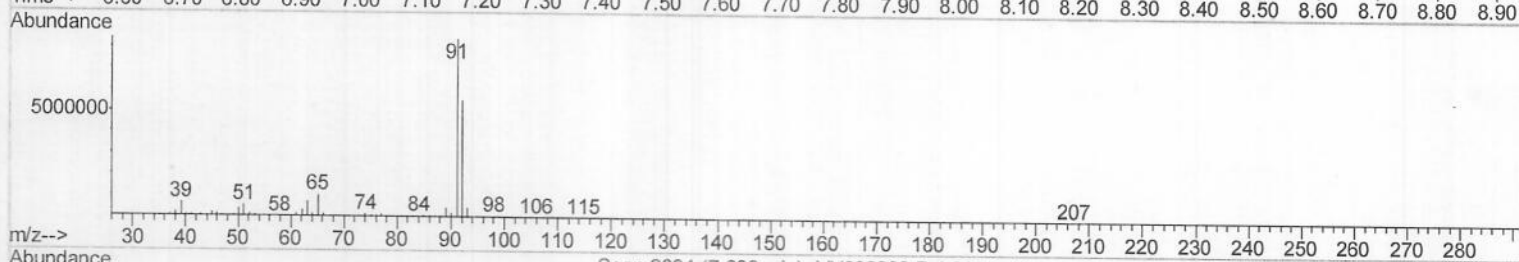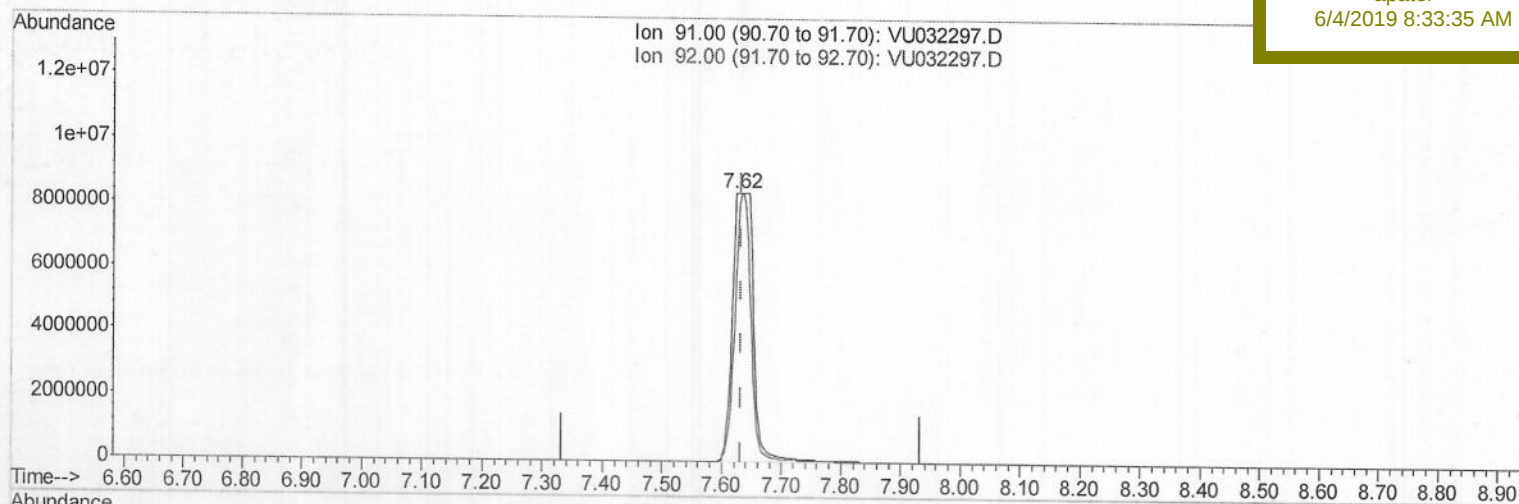

(42) Toluene (T)

7.623min (-0.010) 977.25ug/L m

response 20705464

Ion	Exp%	Act%
91.00	100	100
92.00	57.60	65.66
0.00	0.00	0.00
0.00	0.00	0.00

MD
5/30/19

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU052419\
 Data File : VU032297.D
 Acq On : 24 May 2019 08:40
 Operator : JC/SP
 Sample : K3001-15 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Quant Time: May 24 09:55:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 24 07:24:18 2019
 Response via : Initial Calibration

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YF8

Manual Integrations
 APPROVED

apatel
 6/4/2019 8:33:35 AM

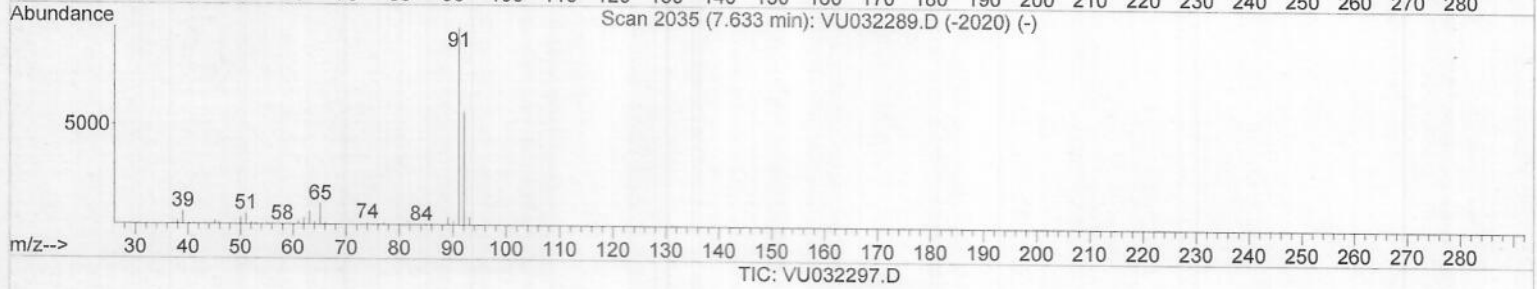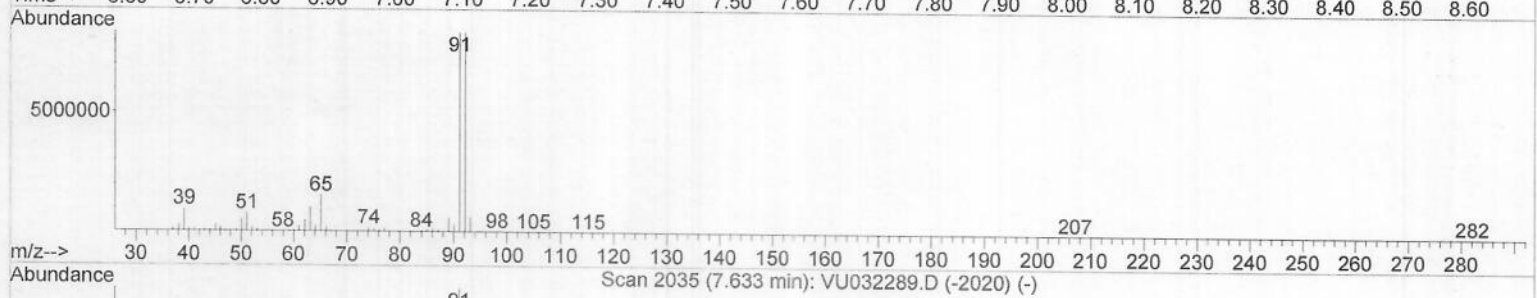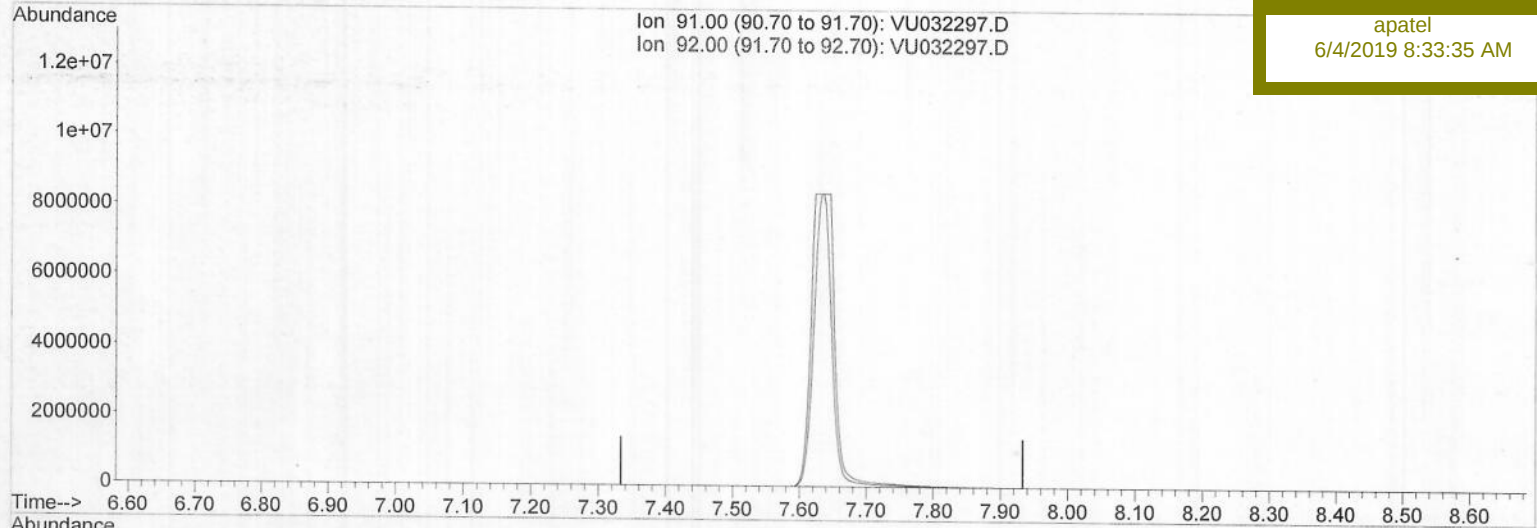

(42) Toluene (T)

7.633min (-7.633) 0.00ug/L d

response 0

Ion	Exp%	Act%
91.00	100	0.00
92.00	57.60	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\

Data File : VU032297.D

Acq On : 24 May 2019 08:40

Operator : JC/SP

Sample : K3001-15 50X

Misc : 5.0mL/MSVOA U/WATER

ALS Vial : 52 Sample Multiplier: 1

Quant Time: May 28 11:24:10 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M

Quant Title : VOC Analysis

QLast Update : Fri May 24 07:24:18 2019

Response via : Initial Calibration

Instrument :

MSVOA_U

ClientSampleId :

E3YF8

Manual Integrations

APPROVED

apatel

6/4/2019 8:33:35 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	700400	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	703441	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	282668	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	226177	61.78	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	123.56%
7) Chloroethane-d5	1.67	69	209185	59.54	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	119.08%
11) 1,1-Dichloroethene-d2	2.27	63	310389	42.75	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.50%
21) 2-Butanone-d5	4.17	46	374644	107.26	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	107.26%
24) Chloroform-d	4.64	84	464807	49.80	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.60%
26) 1,2-Dichloroethane-d4	5.30	65	300026	51.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.36%
32) Benzene-d6	5.33	84	959196	53.55	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.10%
36) 1,2-Dichloropropane-d6	6.32	67	295428	51.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.64%
41) Toluene-d8	7.56	98	816238	49.78	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.56%
43) trans-1,3-Dichloropropene-	7.85	79	126469	48.24	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.48%
47) 2-Hexanone-d5	8.31	63	259140	108.10	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	108.10%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	454001	47.67	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.34%
64) 1,2-Dichlorobenzene-d4	11.85	152	319518	53.79	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.58%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.32	43	5563	1.976	ug/L	88
42) Toluene	7.62	91	20705464m	977.247	ug/L	99
52) Ethylbenzene	9.25	91	188180	8.739	ug/L	99
53) m,p-Xylene	9.37	106	105148	12.651	ug/L	99
54) o-xylene	9.78	106	13176	1.520	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed