

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032294.D
 Acq On : 24 May 2019 07:29
 Operator : JC/SP
 Sample : VU0524WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK42

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	33	rBV2	8892	7663	0.30%	0.037%
2	1.396	88	95	106	rBV	324757	336214	12.95%	1.639%
3	1.669	172	180	199	rVB	260567	340166	13.10%	1.658%
4	1.878	240	245	252	rBV4	7295	9587	0.37%	0.047%
5	2.267	355	366	379	rBV	576787	877002	33.78%	4.276%
6	2.450	411	423	427	rBV	11529	18653	0.72%	0.091%
7	2.592	463	467	472	rBV3	1083	865	0.03%	0.004%
8	2.637	477	481	489	rVV5	914	1148	0.04%	0.006%
9	2.691	492	498	513	rVV7	2528	4716	0.18%	0.023%
10	2.833	528	542	564	rVB	107590	243088	9.36%	1.185%
11	2.981	579	588	590	rBV7	2416	2827	0.11%	0.014%
12	3.019	598	600	603	rVB2	1063	532	0.02%	0.003%
13	3.109	623	628	631	rVB2	740	686	0.03%	0.003%
14	3.373	702	710	711	rBV4	620	674	0.03%	0.003%
15	3.383	711	713	716	rVV	912	642	0.02%	0.003%
16	3.428	724	727	733	rVB3	729	662	0.03%	0.003%
17	3.505	745	751	753	rBV3	591	498	0.02%	0.002%
18	3.524	753	757	760	rVV2	606	558	0.02%	0.003%
19	3.547	760	764	768	rVV2	727	517	0.02%	0.003%
20	3.740	819	824	826	rBV2	1019	770	0.03%	0.004%
21	3.826	846	851	857	rVB3	906	829	0.03%	0.004%
22	3.871	860	865	869	rBV2	742	693	0.03%	0.003%
23	3.910	873	877	881	rBV2	508	545	0.02%	0.003%
24	4.170	944	958	989	rBV2	221016	650488	25.05%	3.171%
25	4.643	1088	1105	1131	rVV	420565	1001925	38.59%	4.885%
26	4.752	1138	1139	1145	rVB3	1152	537	0.02%	0.003%
27	4.887	1178	1181	1184	rBV3	782	668	0.03%	0.003%
28	4.974	1204	1208	1209	rBV2	1401	824	0.03%	0.004%
29	4.990	1209	1213	1224	rVB6	1991	3108	0.12%	0.015%
30	5.132	1252	1257	1262	rVB4	1037	1370	0.05%	0.007%
31	5.334	1296	1320	1354	rBV2	885907	2596492	100.00%	12.659%
32	5.881	1474	1490	1515	rBV	827745	1655023	63.74%	8.069%
33	6.174	1569	1581	1596	rBV6	15021	34641	1.33%	0.169%
34	6.325	1614	1628	1650	rBV	553969	1103395	42.50%	5.379%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032294.D
 Acq On : 24 May 2019 07:29
 Operator : JC/SP
 Sample : VU0524WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK42

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

35	6.563	1698	1702	1706	rBV4	632	646	0.02%	0.003%
36	6.604	1712	1715	1723	rVB4	922	1174	0.05%	0.006%
37	6.640	1723	1726	1731	rBV2	400	486	0.02%	0.002%
38	6.717	1748	1750	1754	rBV2	751	608	0.02%	0.003%
39	6.807	1776	1778	1784	rVB3	691	561	0.02%	0.003%
40	6.868	1795	1797	1799	rBV	1535	907	0.03%	0.004%
41	7.038	1845	1850	1854	rBV4	1001	984	0.04%	0.005%
42	7.225	1895	1908	1932	rBV	276509	517703	19.94%	2.524%
43	7.469	1977	1984	1985	rBV6	5985	5979	0.23%	0.029%
44	7.559	1999	2012	2031	rBV	1207524	2134408	82.20%	10.406%
45	7.845	2091	2101	2125	rBV	195192	345351	13.30%	1.684%
46	8.064	2167	2169	2172	rBV3	986	739	0.03%	0.004%
47	8.157	2193	2198	2200	rBV3	942	727	0.03%	0.004%
48	8.173	2200	2203	2208	rVB4	1147	1103	0.04%	0.005%
49	8.231	2214	2221	2230	rVB6	4710	7141	0.28%	0.035%
50	8.308	2234	2245	2286	rBV2	613518	1270733	48.94%	6.195%
51	8.559	2319	2323	2326	rBV3	1745	1409	0.05%	0.007%
52	8.620	2340	2342	2345	rVB3	1683	811	0.03%	0.004%
53	8.743	2377	2380	2383	rVB3	973	599	0.02%	0.003%
54	8.804	2396	2399	2402	rBV3	1456	903	0.03%	0.004%
55	8.826	2402	2406	2409	rBV5	951	709	0.03%	0.003%
56	8.952	2436	2445	2446	rBV4	1184	1126	0.04%	0.005%
57	9.013	2463	2464	2472	rVB3	717	910	0.04%	0.004%
58	9.083	2472	2486	2520	rBV	1224991	2114412	81.43%	10.308%
59	9.247	2533	2537	2553	rVB8	4154	9171	0.35%	0.045%
60	9.305	2553	2555	2558	rBV2	858	579	0.02%	0.003%
61	9.337	2561	2565	2570	rBV6	1061	1155	0.04%	0.006%
62	9.379	2572	2578	2585	rBV7	2918	4361	0.17%	0.021%
63	9.521	2620	2622	2629	rVB3	778	584	0.02%	0.003%
64	9.688	2670	2674	2677	rBV4	598	531	0.02%	0.003%
65	9.739	2688	2690	2693	rBV	722	495	0.02%	0.002%
66	9.784	2697	2704	2705	rBV5	2435	2399	0.09%	0.012%
67	10.173	2818	2825	2832	rVV7	3321	4763	0.18%	0.023%
68	10.222	2837	2840	2843	rVB4	996	607	0.02%	0.003%
69	10.308	2864	2867	2871	rBV3	589	515	0.02%	0.003%
70	10.427	2890	2904	2933	rBV	856785	1388990	53.49%	6.772%
71	10.566	2944	2947	2952	rBV4	616	731	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032294.D
 Acq On : 24 May 2019 07:29
 Operator : JC/SP
 Sample : VU0524WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK42

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

72	10.646	2968	2972	2975	rVV3	885	777	0.03%	0.004%
73	10.797	3015	3019	3025	rVB2	1030	946	0.04%	0.005%
74	11.009	3082	3085	3088	rBV2	682	581	0.02%	0.003%
75	11.054	3094	3099	3103	rBV4	897	954	0.04%	0.005%
76	11.276	3161	3168	3172	rBV2	818	1164	0.04%	0.006%
77	11.424	3204	3214	3219	rBV5	4969	7361	0.28%	0.036%
78	11.479	3219	3231	3252	rBV	1103792	1816127	69.95%	8.854%
79	11.855	3336	3348	3376	rBV	1149475	1938042	74.64%	9.448%
80	12.411	3518	3521	3524	rBV	568	499	0.02%	0.002%
81	12.427	3524	3526	3532	rVV4	739	593	0.02%	0.003%
82	12.504	3547	3550	3554	rVB3	971	705	0.03%	0.003%
83	12.524	3554	3556	3559	rBV2	751	549	0.02%	0.003%
84	12.559	3564	3567	3571	rVB3	1329	685	0.03%	0.003%
85	12.768	3628	3632	3635	rBV3	1199	877	0.03%	0.004%
86	12.861	3657	3661	3665	rBV4	517	619	0.02%	0.003%
87	12.900	3665	3673	3680	rBV9	4421	7821	0.30%	0.038%
88	13.183	3756	3761	3763	rBV	893	641	0.02%	0.003%
89	13.215	3767	3771	3773	rBV3	762	647	0.02%	0.003%
90	13.353	3812	3814	3817	rVB	926	525	0.02%	0.003%
91	13.376	3817	3821	3824	rBV3	1103	913	0.04%	0.004%
92	13.527	3862	3868	3870	rBV3	1986	1988	0.08%	0.010%
93	13.659	3907	3909	3913	rVB3	938	541	0.02%	0.003%
94	14.328	4114	4117	4121	rVB4	814	654	0.03%	0.003%
95	14.369	4126	4130	4132	rBV2	1085	842	0.03%	0.004%
96	14.382	4132	4134	4139	rVV2	739	539	0.02%	0.003%
97	14.662	4216	4221	4224	rBV3	1152	1194	0.05%	0.006%
98	14.678	4224	4226	4229	rVV2	995	576	0.02%	0.003%
99	15.083	4349	4352	4358	rVB3	1094	938	0.04%	0.005%
100	15.109	4358	4360	4362	rBV	965	526	0.02%	0.003%


Sum of corrected areas: 20511840

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU052419\
Data File : VU032294.D
Acq On : 24 May 2019 07:29
Operator : JC/SP
Sample : VU0524WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK42

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

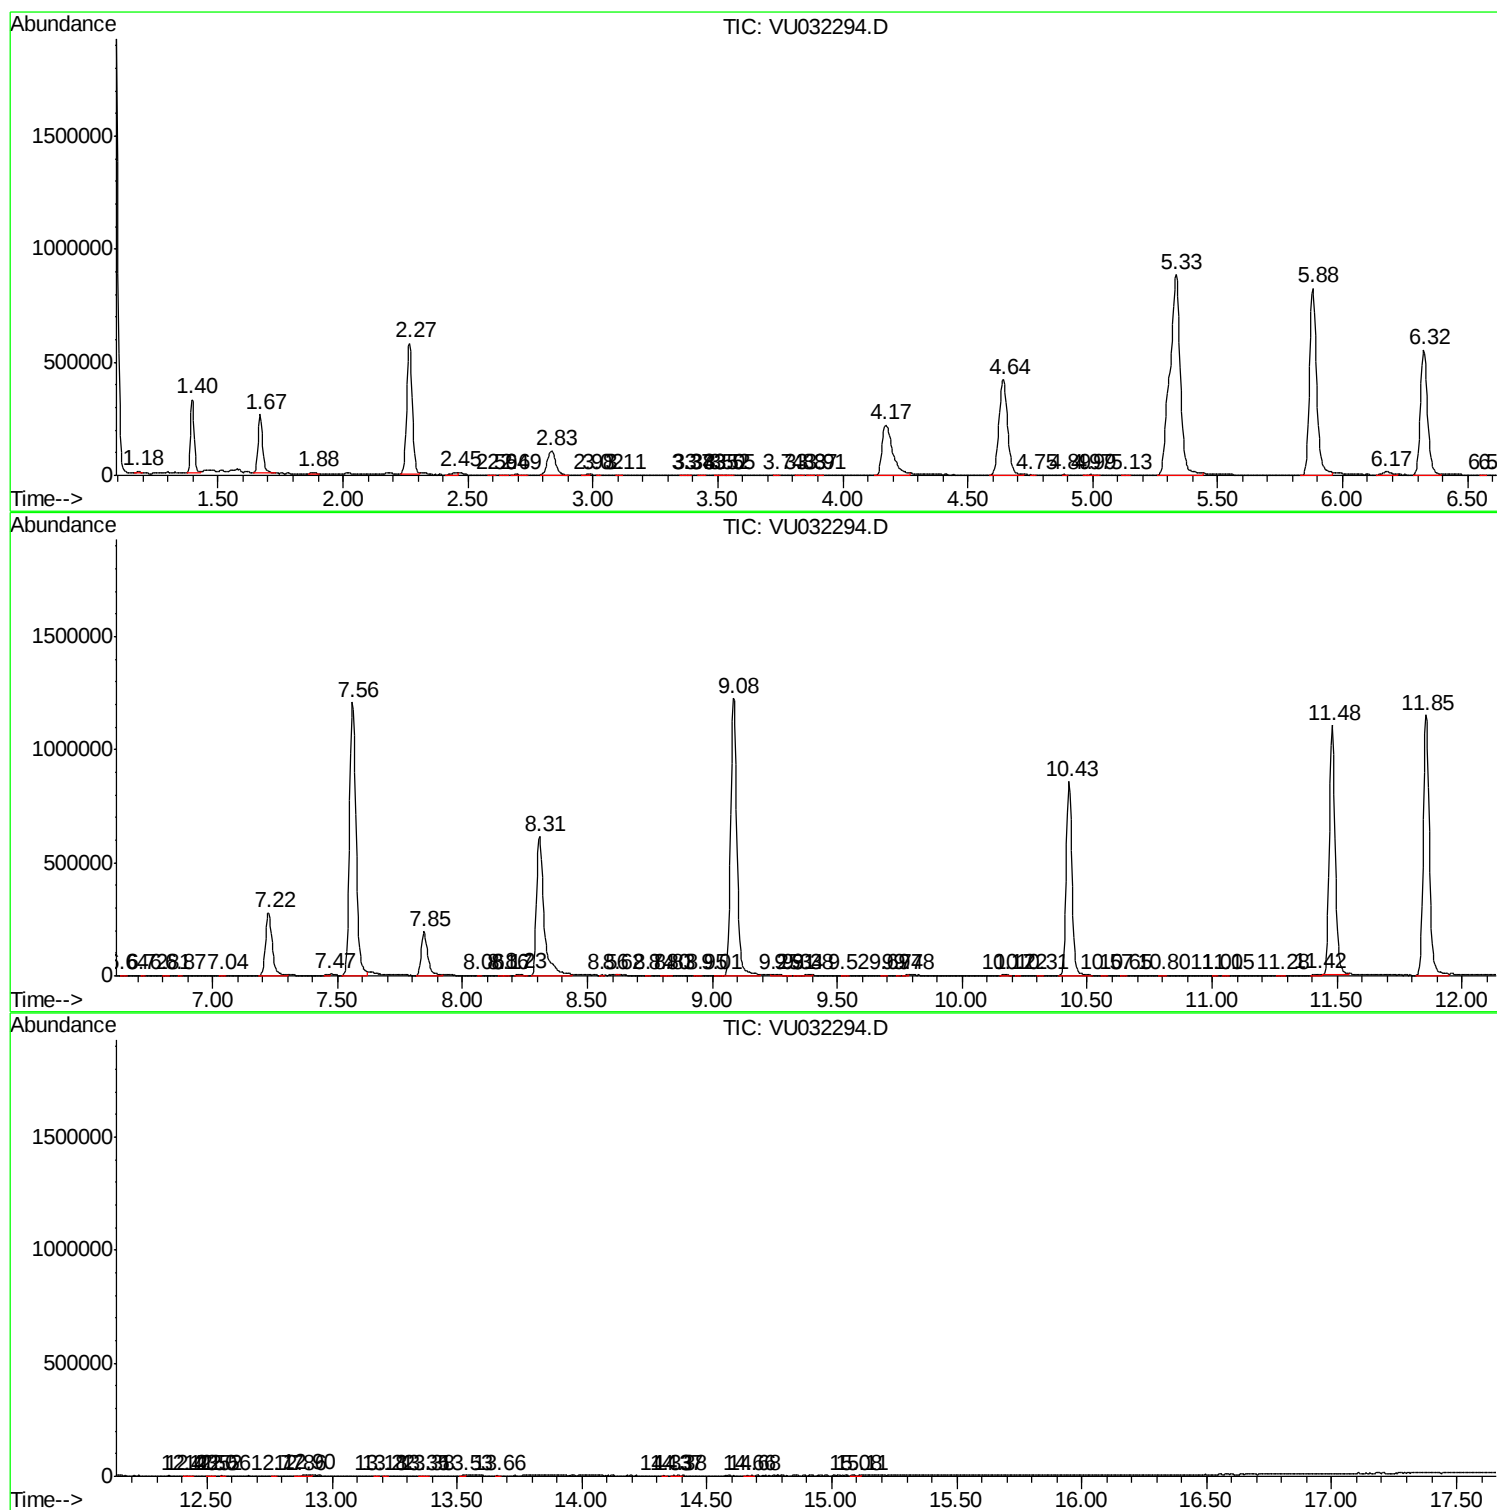

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU052419\
Data File : VU032294.D
Acq On : 24 May 2019 07:29
Operator : JC/SP
Sample : VU0524WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK42

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU052419\
Data File : VU032294.D
Acq On : 24 May 2019 07:29
Operator : JC/SP
Sample : VU0524WBL01
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK42

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc