

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032300.D
 Acq On : 24 May 2019 09:51
 Operator : JC/SP
 Sample : K3001-11 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YF6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	36	rVB5	10203	10324	0.24%	0.036%
2	1.396	88	95	105	rBV	368914	381848	8.86%	1.324%
3	1.669	172	180	196	rVB	295862	384681	8.93%	1.334%
4	2.180	335	339	350	rVB8	6762	10408	0.24%	0.036%
5	2.267	354	366	379	rBV	611086	930024	21.58%	3.225%
6	2.453	413	424	434	rBV2	12145	24762	0.57%	0.086%
7	2.527	444	447	451	rBV3	1628	999	0.02%	0.003%
8	2.701	492	501	504	rBV5	2344	3145	0.07%	0.011%
9	2.833	526	542	561	rVV	100416	223941	5.20%	0.777%
10	3.080	615	619	624	rVB3	1088	904	0.02%	0.003%
11	3.113	624	629	631	rBV3	795	734	0.02%	0.003%
12	3.174	644	648	650	rBV	1148	874	0.02%	0.003%
13	3.206	655	658	664	rVB4	781	632	0.01%	0.002%
14	3.322	689	694	700	rVB3	989	865	0.02%	0.003%
15	3.441	721	731	735	rBV5	3248	4928	0.11%	0.017%
16	4.174	946	959	986	rBV2	244489	692254	16.06%	2.401%
17	4.640	1086	1104	1132	rBV	459588	1090851	25.31%	3.783%
18	4.858	1169	1172	1175	rBV3	987	909	0.02%	0.003%
19	4.891	1179	1182	1184	rVV2	1402	779	0.02%	0.003%
20	5.202	1276	1279	1281	rBV3	1182	808	0.02%	0.003%
21	5.334	1297	1320	1354	rBV2	921828	2747520	63.76%	9.528%
22	5.672	1423	1425	1429	rVB4	1220	758	0.02%	0.003%
23	5.746	1443	1448	1451	rBV3	860	706	0.02%	0.002%
24	5.768	1452	1455	1460	rBV3	911	706	0.02%	0.002%
25	5.881	1476	1490	1518	rBV	832862	1681408	39.02%	5.831%
26	6.096	1554	1557	1559	rBV3	1281	657	0.02%	0.002%
27	6.177	1570	1582	1599	rBV7	14924	35040	0.81%	0.122%
28	6.238	1599	1601	1604	rVB2	1276	777	0.02%	0.003%
29	6.325	1614	1628	1645	rBV	586869	1184711	27.49%	4.108%
30	6.553	1696	1699	1702	rVB3	886	622	0.01%	0.002%
31	6.575	1702	1706	1711	rBV5	1064	768	0.02%	0.003%
32	6.643	1717	1727	1734	rBV7	4282	7241	0.17%	0.025%
33	6.720	1746	1751	1753	rBV4	1165	956	0.02%	0.003%
34	6.874	1794	1799	1800	rBV2	1289	1009	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032300.D
 Acq On : 24 May 2019 09:51
 Operator : JC/SP
 Sample : K3001-11 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YF6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

35	6.897	1802	1806	1812	rVB7	1678	1931	0.04%	0.007%
36	6.948	1820	1822	1829	rVB3	675	730	0.02%	0.003%
37	6.993	1833	1836	1839	rVB2	900	642	0.01%	0.002%
38	7.173	1885	1892	1896	rBV4	1158	1111	0.03%	0.004%
39	7.225	1896	1908	1930	rBV	294361	539847	12.53%	1.872%
40	7.469	1979	1984	1986	rBV3	1711	1691	0.04%	0.006%
41	7.559	1996	2012	2027	rBV	1207922	2145981	49.80%	7.442%
42	7.633	2029	2035	2055	rVB	85522	167396	3.88%	0.581%
43	7.845	2090	2101	2117	rBV	201534	353867	8.21%	1.227%
44	8.016	2150	2154	2155	rBV	907	654	0.02%	0.002%
45	8.148	2190	2195	2198	rBV4	787	745	0.02%	0.003%
46	8.231	2214	2221	2224	rBV6	1913	2213	0.05%	0.008%
47	8.308	2231	2245	2280	rBV2	698207	1364310	31.66%	4.731%
48	8.537	2312	2316	2325	rVB8	3872	4917	0.11%	0.017%
49	8.595	2330	2334	2336	rBV4	1118	844	0.02%	0.003%
50	8.646	2346	2350	2354	rVB6	1099	1194	0.03%	0.004%
51	8.701	2365	2367	2371	rBV3	914	696	0.02%	0.002%
52	8.723	2371	2374	2377	rVB3	1538	918	0.02%	0.003%
53	8.990	2453	2457	2459	rBV3	868	752	0.02%	0.003%
54	9.083	2471	2486	2512	rBV	1216844	2071644	48.07%	7.184%
55	9.244	2524	2536	2562	rBV	1571116	2558831	59.38%	8.874%
56	9.370	2562	2575	2608	rVB	2609614	4309408	100.00%	14.944%
57	9.627	2651	2655	2657	rVB2	897	682	0.02%	0.002%
58	9.717	2673	2683	2688	rBV8	5975	11053	0.26%	0.038%
59	9.778	2696	2702	2713	rVB3	7582	12424	0.29%	0.043%
60	9.913	2739	2744	2747	rBV5	3144	2981	0.07%	0.010%
61	9.945	2750	2754	2765	rVB9	6960	10878	0.25%	0.038%
62	10.048	2776	2786	2794	rBV9	6675	11846	0.27%	0.041%
63	10.164	2812	2822	2836	rVV	56386	91167	2.12%	0.316%
64	10.366	2878	2885	2886	rBV5	3138	2208	0.05%	0.008%
65	10.427	2892	2904	2934	rVB	904466	1476743	34.27%	5.121%
66	10.585	2943	2953	2968	rBV2	49958	84393	1.96%	0.293%
67	10.681	2975	2983	2986	rBV6	3883	5795	0.13%	0.020%
68	10.746	3000	3003	3005	rBV3	1091	727	0.02%	0.003%
69	10.849	3033	3035	3042	rVB4	663	777	0.02%	0.003%
70	10.919	3050	3057	3066	rVV7	3835	6150	0.14%	0.021%
71	10.971	3066	3073	3085	rVB7	7546	12582	0.29%	0.044%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032300.D
 Acq On : 24 May 2019 09:51
 Operator : JC/SP
 Sample : K3001-11 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YF6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

72	11.080	3104	3107	3110	rBV2	1279	895	0.02%	0.003%
73	11.096	3110	3112	3116	rVB2	1179	657	0.02%	0.002%
74	11.148	3117	3128	3140	rBV3	52757	86090	2.00%	0.299%
75	11.299	3167	3175	3176	rVV6	2841	3762	0.09%	0.013%
76	11.321	3176	3182	3193	rVB2	8260	12729	0.30%	0.044%
77	11.392	3199	3204	3207	rBV6	2518	2227	0.05%	0.008%
78	11.479	3219	3231	3248	rBV	1146281	1832916	42.53%	6.356%
79	11.569	3251	3259	3271	rVB	51964	86468	2.01%	0.300%
80	11.765	3311	3320	3335	rBV4	18911	36740	0.85%	0.127%
81	11.855	3336	3348	3371	rBV	1169386	1975405	45.84%	6.850%
82	12.058	3407	3411	3420	rVB4	7165	8437	0.20%	0.029%
83	12.254	3465	3472	3478	rBV	8096	12362	0.29%	0.043%
84	12.357	3496	3504	3520	rVB5	11940	24330	0.56%	0.084%
85	12.453	3531	3534	3540	rBV6	1317	1044	0.02%	0.004%
86	12.556	3556	3566	3572	rVB6	5658	9853	0.23%	0.034%
87	12.649	3586	3595	3601	rBV4	4639	6690	0.16%	0.023%
88	12.704	3607	3612	3613	rBV4	1984	1883	0.04%	0.007%
89	12.987	3696	3700	3704	rVB4	1492	1183	0.03%	0.004%
90	13.029	3710	3713	3715	rBV2	820	627	0.01%	0.002%
91	13.119	3734	3741	3749	rBV6	12785	21360	0.50%	0.074%
92	13.199	3764	3766	3769	rVB2	1267	688	0.02%	0.002%
93	13.286	3787	3793	3805	rVB9	8894	14949	0.35%	0.052%
94	14.086	4038	4042	4045	rBV3	738	635	0.01%	0.002%
95	14.228	4083	4086	4092	rVB3	1088	789	0.02%	0.003%
96	14.257	4092	4095	4097	rBV2	1075	720	0.02%	0.002%
97	14.726	4234	4241	4243	rBV5	1126	1253	0.03%	0.004%
98	14.954	4309	4312	4315	rVB4	1638	1052	0.02%	0.004%
99	15.350	4431	4435	4437	rBV3	1938	1651	0.04%	0.006%
100	15.511	4483	4485	4488	rBV3	1235	646	0.01%	0.002%


Sum of corrected areas: 28836318

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU052419\
Data File : VU032300.D
Acq On : 24 May 2019 09:51
Operator : JC/SP
Sample : K3001-11 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YF6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

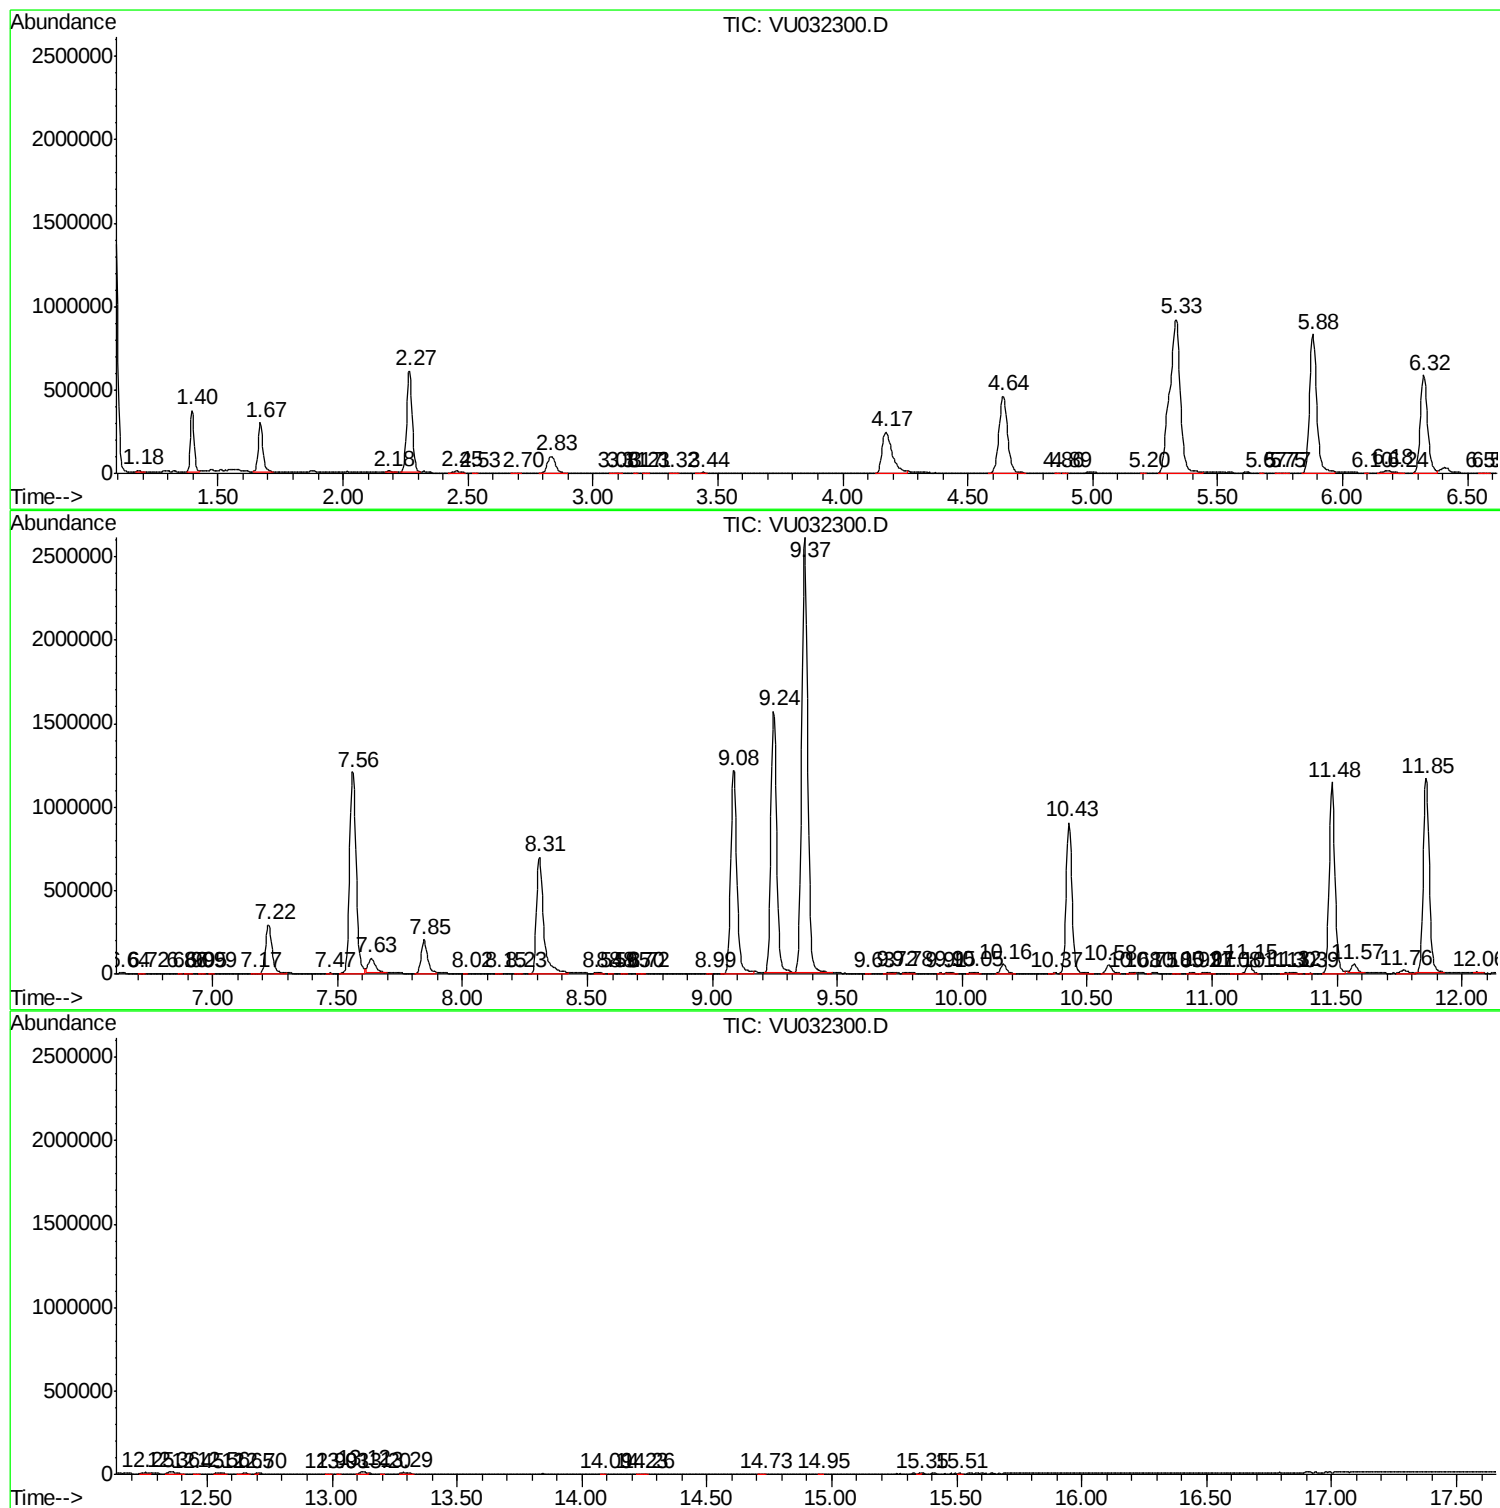

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU052419\
Data File : VU032300.D
Acq On : 24 May 2019 09:51
Operator : JC/SP
Sample : K3001-11 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YF6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU052419\
Data File : VU032300.D
Acq On : 24 May 2019 09:51
Operator : JC/SP
Sample : K3001-11 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YF6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc