

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032303.D
 Acq On : 24 May 2019 11:04
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.396	89	95	107	rBV	317135	327284	12.84%	1.623%
2	1.669	172	180	196	rVB	247226	324749	12.74%	1.610%
3	2.267	355	366	379	rBV	569397	869731	34.11%	4.313%
4	2.450	415	423	437	rBV3	14081	28516	1.12%	0.141%
5	2.611	468	473	475	rBV3	902	798	0.03%	0.004%
6	2.682	492	495	496	rBV2	1221	653	0.03%	0.003%
7	2.759	515	519	523	rBV4	1155	1028	0.04%	0.005%
8	2.833	525	542	558	rVV	120584	267718	10.50%	1.328%
9	2.936	572	574	577	rBV2	443	293	0.01%	0.001%
10	3.061	607	613	615	rBV	627	579	0.02%	0.003%
11	3.116	629	630	631	rBV	150	42	0.00%	0.000%
12	3.138	632	637	638	rBV3	276	229	0.01%	0.001%
13	3.209	657	659	663	rVB2	926	582	0.02%	0.003%
14	3.232	663	666	669	rBV	155	117	0.00%	0.001%
15	3.248	669	671	673	rBV	423	229	0.01%	0.001%
16	3.286	680	683	685	rBV2	315	119	0.00%	0.001%
17	3.302	686	688	692	rVB3	570	410	0.02%	0.002%
18	3.367	706	708	715	rVB5	585	533	0.02%	0.003%
19	3.405	717	720	722	rVB2	280	169	0.01%	0.001%
20	3.415	722	723	724	rBV2	385	142	0.01%	0.001%
21	3.444	728	732	735	rBV3	643	548	0.02%	0.003%
22	3.524	754	757	760	rBV2	536	300	0.01%	0.001%
23	3.556	764	767	769	rBV2	492	345	0.01%	0.002%
24	3.588	774	777	782	rBV3	691	599	0.02%	0.003%
25	3.627	787	789	792	rBV2	269	171	0.01%	0.001%
26	3.650	793	796	798	rVB2	392	186	0.01%	0.001%
27	3.698	809	811	813	rBV2	385	177	0.01%	0.001%
28	3.746	821	826	831	rVB3	457	402	0.02%	0.002%
29	3.781	834	837	843	rVB3	446	482	0.02%	0.002%
30	3.810	843	846	848	rBV2	321	175	0.01%	0.001%
31	3.823	848	850	854	rVB	450	275	0.01%	0.001%
32	3.846	855	857	860	rVB	310	151	0.01%	0.001%
33	3.862	860	862	863	rBV	372	132	0.01%	0.001%
34	3.920	877	880	882	rBV2	252	151	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032303.D
 Acq On : 24 May 2019 11:04
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

35	3.932	882	884	886	rBV	434	254	0.01%	0.001%
36	3.961	891	893	896	rBV	355	220	0.01%	0.001%
37	4.058	919	923	924	rBV2	712	325	0.01%	0.002%
38	4.093	932	934	935	rBV	399	199	0.01%	0.001%
39	4.174	943	959	988	rBV2	213287	621263	24.37%	3.081%
40	4.511	1062	1064	1067	rBV2	692	519	0.02%	0.003%
41	4.572	1080	1083	1085	rBV4	666	330	0.01%	0.002%
42	4.640	1086	1104	1136	rBV2	418822	995516	39.04%	4.937%
43	5.022	1221	1223	1224	rBV2	409	138	0.01%	0.001%
44	5.087	1240	1243	1247	rVB3	761	542	0.02%	0.003%
45	5.106	1247	1249	1250	rBV2	263	113	0.00%	0.001%
46	5.177	1266	1271	1273	rBV2	661	578	0.02%	0.003%
47	5.238	1287	1290	1294	rBV2	431	412	0.02%	0.002%
48	5.334	1297	1320	1349	rBV2	873942	2549718	100.00%	12.644%
49	5.778	1456	1458	1463	rVB4	899	629	0.02%	0.003%
50	5.810	1463	1468	1472	rBV4	1260	1137	0.04%	0.006%
51	5.881	1477	1490	1523	rBV	826294	1667530	65.40%	8.269%
52	6.177	1573	1582	1591	rBV7	9864	21254	0.83%	0.105%
53	6.325	1615	1628	1653	rBV	546338	1085074	42.56%	5.381%
54	6.588	1708	1710	1712	rBV	488	137	0.01%	0.001%
55	6.662	1731	1733	1734	rBV	559	229	0.01%	0.001%
56	6.743	1757	1758	1761	rBV	426	302	0.01%	0.001%
57	6.788	1769	1772	1774	rVB2	496	215	0.01%	0.001%
58	6.801	1774	1776	1780	rVB2	695	491	0.02%	0.002%
59	6.826	1780	1784	1785	rBV2	755	428	0.02%	0.002%
60	6.836	1785	1787	1789	rBV	514	283	0.01%	0.001%
61	6.977	1828	1831	1833	rBV2	1219	784	0.03%	0.004%
62	7.048	1851	1853	1855	rBV2	619	335	0.01%	0.002%
63	7.077	1859	1862	1866	rVB	682	418	0.02%	0.002%
64	7.096	1866	1868	1869	rBV	279	146	0.01%	0.001%
65	7.173	1886	1892	1895	rBV3	709	730	0.03%	0.004%
66	7.222	1895	1907	1925	rBV	273023	500113	19.61%	2.480%
67	7.559	1999	2012	2032	rBV	1205240	2125817	83.37%	10.542%
68	7.846	2090	2101	2124	rBV2	186535	337185	13.22%	1.672%
69	8.309	2234	2245	2289	rBV2	608200	1207490	47.36%	5.988%
70	8.698	2363	2366	2369	rBV4	808	645	0.03%	0.003%
71	8.881	2420	2423	2427	rVB2	897	539	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032303.D
 Acq On : 24 May 2019 11:04
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

72	8.900	2427	2429	2430	rBV	709	321	0.01%	0.002%
73	9.032	2467	2470	2473	rBV	428	372	0.01%	0.002%
74	9.083	2474	2486	2510	rBV	1225335	2095525	82.19%	10.392%
75	9.373	2566	2576	2591	rBV	19207	36703	1.44%	0.182%
76	9.501	2614	2616	2618	rBV3	615	268	0.01%	0.001%
77	9.601	2643	2647	2653	rVB3	906	922	0.04%	0.005%
78	9.662	2663	2666	2669	rVB3	676	452	0.02%	0.002%
79	9.784	2693	2704	2709	rBV6	2191	4016	0.16%	0.020%
80	9.861	2725	2728	2731	rVB2	645	290	0.01%	0.001%
81	9.907	2739	2742	2745	rBV2	804	511	0.02%	0.003%
82	10.054	2787	2788	2790	rBV	309	135	0.01%	0.001%
83	10.083	2794	2797	2801	rVB2	761	572	0.02%	0.003%
84	10.109	2801	2805	2807	rBV	497	315	0.01%	0.002%
85	10.173	2821	2825	2828	rVB2	1429	1128	0.04%	0.006%
86	10.215	2835	2838	2841	rBV2	607	351	0.01%	0.002%
87	10.299	2862	2864	2867	rBV2	630	378	0.01%	0.002%
88	10.427	2891	2904	2924	rBV	830586	1347727	52.86%	6.683%
89	10.974	3072	3074	3079	rBV2	530	416	0.02%	0.002%
90	11.225	3150	3152	3154	rBV3	527	286	0.01%	0.001%
91	11.257	3160	3162	3164	rBV	677	321	0.01%	0.002%
92	11.479	3220	3231	3256	rBV	1120000	1828263	71.70%	9.066%
93	11.855	3336	3348	3366	rBV	1125630	1895829	74.35%	9.402%


Sum of corrected areas: 20165154

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU052419\
Data File : VU032303.D
Acq On : 24 May 2019 11:04
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

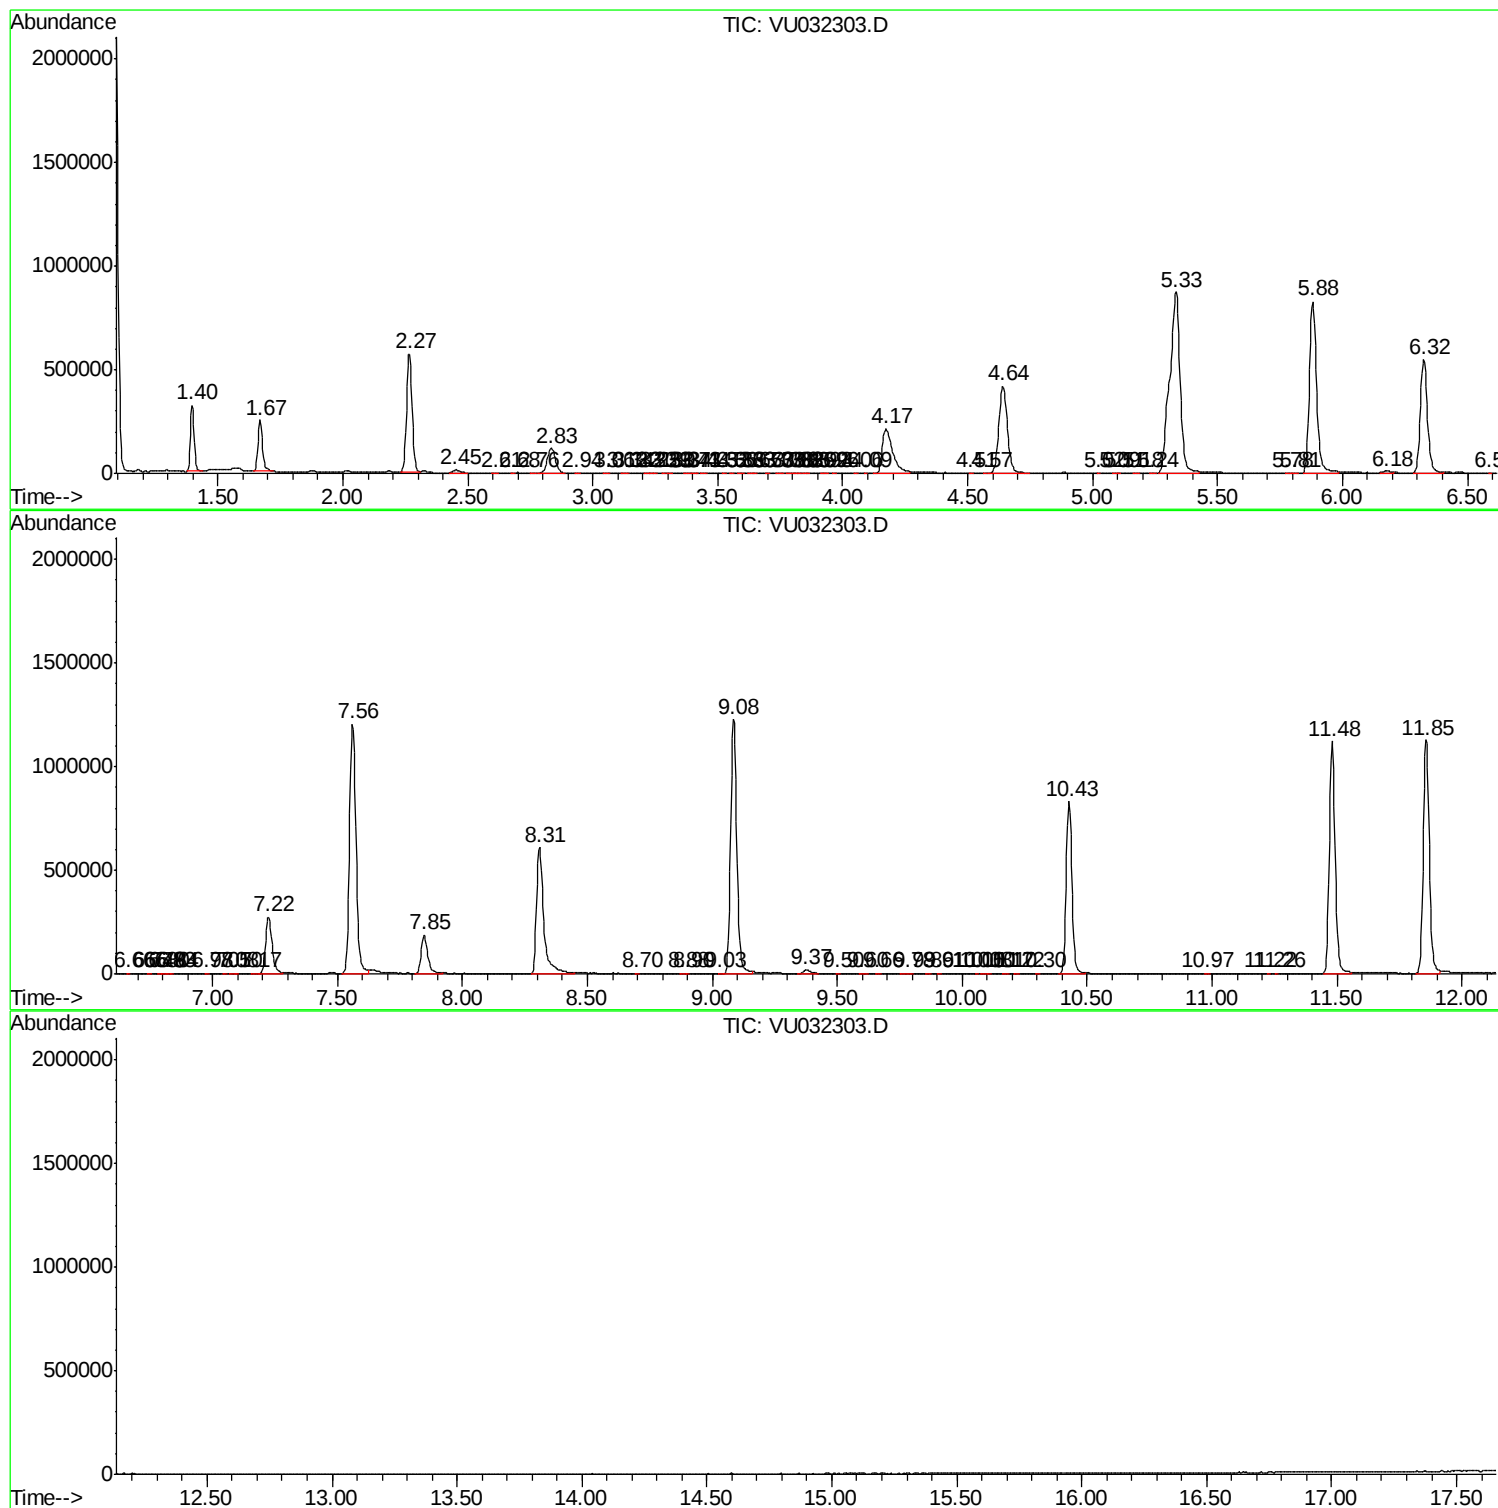

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU052419\
Data File : VU032303.D
Acq On : 24 May 2019 11:04
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU052419\
Data File : VU032303.D
Acq On : 24 May 2019 11:04
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc