

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032304.D
 Acq On : 24 May 2019 11:28
 Operator : JC/SP
 Sample : K3001-12 500X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YF7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	37	rBV3	9645	9777	0.10%	0.030%
2	1.395	88	95	106	rBV	335229	354979	3.78%	1.094%
3	1.672	173	181	199	rVB	275846	356393	3.80%	1.099%
4	1.881	240	246	254	rBV3	7294	9465	0.10%	0.029%
5	2.267	355	366	380	rBV	596421	908290	9.68%	2.800%
6	2.386	401	403	407	rVB2	1124	783	0.01%	0.002%
7	2.453	414	424	437	rBV3	5079	10047	0.11%	0.031%
8	2.688	492	497	501	rBV3	1010	1325	0.01%	0.004%
9	2.833	529	542	561	rVV	50222	110104	1.17%	0.339%
10	2.981	586	588	594	rVV3	749	540	0.01%	0.002%
11	3.071	608	616	618	rBV2	815	853	0.01%	0.003%
12	3.267	674	677	680	rBV2	726	537	0.01%	0.002%
13	3.347	700	702	705	rVB2	869	472	0.01%	0.001%
14	3.366	705	708	710	rBV2	655	476	0.01%	0.001%
15	3.434	724	729	733	rVB3	836	714	0.01%	0.002%
16	3.591	775	778	783	rVB3	644	551	0.01%	0.002%
17	4.071	924	927	932	rBV3	703	532	0.01%	0.002%
18	4.173	947	959	991	rBV	232978	649736	6.92%	2.003%
19	4.469	1048	1051	1055	rBV4	1052	758	0.01%	0.002%
20	4.643	1087	1105	1130	rBV	448154	1054484	11.23%	3.251%
21	4.868	1171	1175	1176	rBV3	1355	868	0.01%	0.003%
22	4.894	1180	1183	1190	rVB5	1471	1684	0.02%	0.005%
23	4.981	1204	1210	1212	rBV5	2368	2257	0.02%	0.007%
24	5.051	1227	1232	1236	rVB3	763	861	0.01%	0.003%
25	5.334	1296	1320	1345	rBV2	907579	2652140	28.25%	8.176%
26	5.607	1401	1405	1406	rBV3	1623	1029	0.01%	0.003%
27	5.752	1447	1450	1455	rBV4	1137	1194	0.01%	0.004%
28	5.778	1455	1458	1466	rVB8	1700	2160	0.02%	0.007%
29	5.816	1466	1470	1475	rBV4	1043	976	0.01%	0.003%
30	5.881	1475	1490	1517	rBV	846799	1711566	18.23%	5.276%
31	6.173	1572	1581	1598	rBV5	12479	27302	0.29%	0.084%
32	6.260	1605	1608	1613	rVB4	1543	1057	0.01%	0.003%
33	6.324	1613	1628	1647	rBV	578731	1159425	12.35%	3.574%
34	6.508	1682	1685	1688	rBV3	934	493	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032304.D
 Acq On : 24 May 2019 11:28
 Operator : JC/SP
 Sample : K3001-12 500X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YF7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

35	6.543	1694	1696	1703	rVB4	783	706	0.01%	0.002%
36	6.643	1724	1727	1729	rBV2	1306	712	0.01%	0.002%
37	6.691	1740	1742	1746	rBV2	637	523	0.01%	0.002%
38	6.762	1760	1764	1765	rVV	861	503	0.01%	0.002%
39	6.816	1777	1781	1786	rBV2	915	916	0.01%	0.003%
40	6.852	1786	1792	1794	rBV2	752	652	0.01%	0.002%
41	7.000	1834	1838	1842	rBV3	1171	1121	0.01%	0.003%
42	7.099	1864	1869	1873	rBV3	789	802	0.01%	0.002%
43	7.225	1896	1908	1932	rBV	303554	562233	5.99%	1.733%
44	7.427	1967	1971	1972	rBV2	956	568	0.01%	0.002%
45	7.562	1998	2013	2023	rBV	1216068	2135700	22.75%	6.584%
46	7.630	2023	2034	2091	rVV	5196566	9387119	100.00%	28.937%
47	7.845	2092	2101	2118	rVB	213866	371945	3.96%	1.147%
48	8.016	2152	2154	2160	rVB5	1469	805	0.01%	0.002%
49	8.125	2185	2188	2190	rBV2	869	538	0.01%	0.002%
50	8.231	2219	2221	2225	rVB3	1124	567	0.01%	0.002%
51	8.308	2234	2245	2279	rBV2	663625	1311195	13.97%	4.042%
52	8.527	2311	2313	2316	rBV3	1067	808	0.01%	0.002%
53	8.614	2333	2340	2343	rBV8	2264	2918	0.03%	0.009%
54	8.765	2384	2387	2392	rBV3	829	599	0.01%	0.002%
55	8.839	2405	2410	2411	rBV4	763	551	0.01%	0.002%
56	8.865	2416	2418	2426	rVB2	981	895	0.01%	0.003%
57	8.958	2441	2447	2450	rBV4	705	717	0.01%	0.002%
58	9.086	2473	2487	2515	rBV	1278730	2174440	23.16%	6.703%
59	9.247	2526	2537	2563	rBV	241284	404063	4.30%	1.246%
60	9.369	2563	2575	2604	rBV	682362	1140871	12.15%	3.517%
61	9.537	2624	2627	2631	rBV4	717	607	0.01%	0.002%
62	9.585	2636	2642	2645	rBV5	811	989	0.01%	0.003%
63	9.778	2690	2702	2717	rBV	216047	360007	3.84%	1.110%
64	10.093	2797	2800	2804	rBV2	854	637	0.01%	0.002%
65	10.148	2814	2817	2818	rBV2	1191	691	0.01%	0.002%
66	10.170	2818	2824	2831	rVB4	5035	6747	0.07%	0.021%
67	10.263	2848	2853	2855	rBV3	544	566	0.01%	0.002%
68	10.283	2855	2859	2863	rVB4	978	843	0.01%	0.003%
69	10.427	2891	2904	2927	rBV	895522	1455296	15.50%	4.486%
70	10.588	2948	2954	2963	rVB3	5111	7345	0.08%	0.023%
71	10.681	2975	2983	2990	rBV2	12353	20154	0.21%	0.062%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032304.D
 Acq On : 24 May 2019 11:28
 Operator : JC/SP
 Sample : K3001-12 500X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YF7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

72	10.774	3002	3012	3020	rVB3	8239	12860	0.14%	0.040%
73	10.881	3039	3045	3048	rBV3	1092	1199	0.01%	0.004%
74	10.919	3048	3057	3065	rVV5	5861	9309	0.10%	0.029%
75	10.974	3065	3074	3082	rVV4	5928	10866	0.12%	0.033%
76	11.006	3082	3084	3090	rVB3	1062	841	0.01%	0.003%
77	11.147	3118	3128	3143	rVB2	22358	36208	0.39%	0.112%
78	11.398	3203	3206	3207	rBV2	1141	712	0.01%	0.002%
79	11.479	3219	3231	3252	rBV	1194968	1944443	20.71%	5.994%
80	11.810	3331	3334	3336	rBV2	1187	916	0.01%	0.003%
81	11.855	3336	3348	3369	rBV	1208720	2014975	21.47%	6.212%
82	12.141	3431	3437	3438	rBV3	1432	1396	0.01%	0.004%
83	12.257	3470	3473	3483	rBV7	1526	2336	0.02%	0.007%
84	12.405	3517	3519	3524	rVB2	1193	559	0.01%	0.002%
85	12.546	3561	3563	3567	rBV2	746	694	0.01%	0.002%
86	12.813	3642	3646	3649	rBV2	822	604	0.01%	0.002%
87	12.877	3663	3666	3668	rBV2	854	530	0.01%	0.002%
88	13.070	3722	3726	3729	rBV2	791	667	0.01%	0.002%
89	13.128	3736	3744	3747	rBV4	1777	2237	0.02%	0.007%
90	13.199	3763	3766	3770	rBV2	676	698	0.01%	0.002%
91	13.282	3789	3792	3795	rBV3	697	643	0.01%	0.002%
92	13.321	3801	3804	3807	rBV4	855	569	0.01%	0.002%
93	13.427	3834	3837	3841	rVB	702	468	0.00%	0.001%
94	13.501	3857	3860	3866	rBV3	1093	980	0.01%	0.003%
95	13.877	3974	3977	3982	rBV2	855	609	0.01%	0.002%
96	14.540	4180	4183	4187	rVB3	1149	786	0.01%	0.002%
97	14.559	4187	4189	4191	rBV2	922	530	0.01%	0.002%
98	14.697	4228	4232	4234	rBV4	1191	1049	0.01%	0.003%
99	14.723	4238	4240	4243	rVV	1035	664	0.01%	0.002%
100	14.765	4251	4253	4258	rBV	934	849	0.01%	0.003%


Sum of corrected areas: 32439374

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU052419\
Data File : VU032304.D
Acq On : 24 May 2019 11:28
Operator : JC/SP
Sample : K3001-12 500X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YF7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

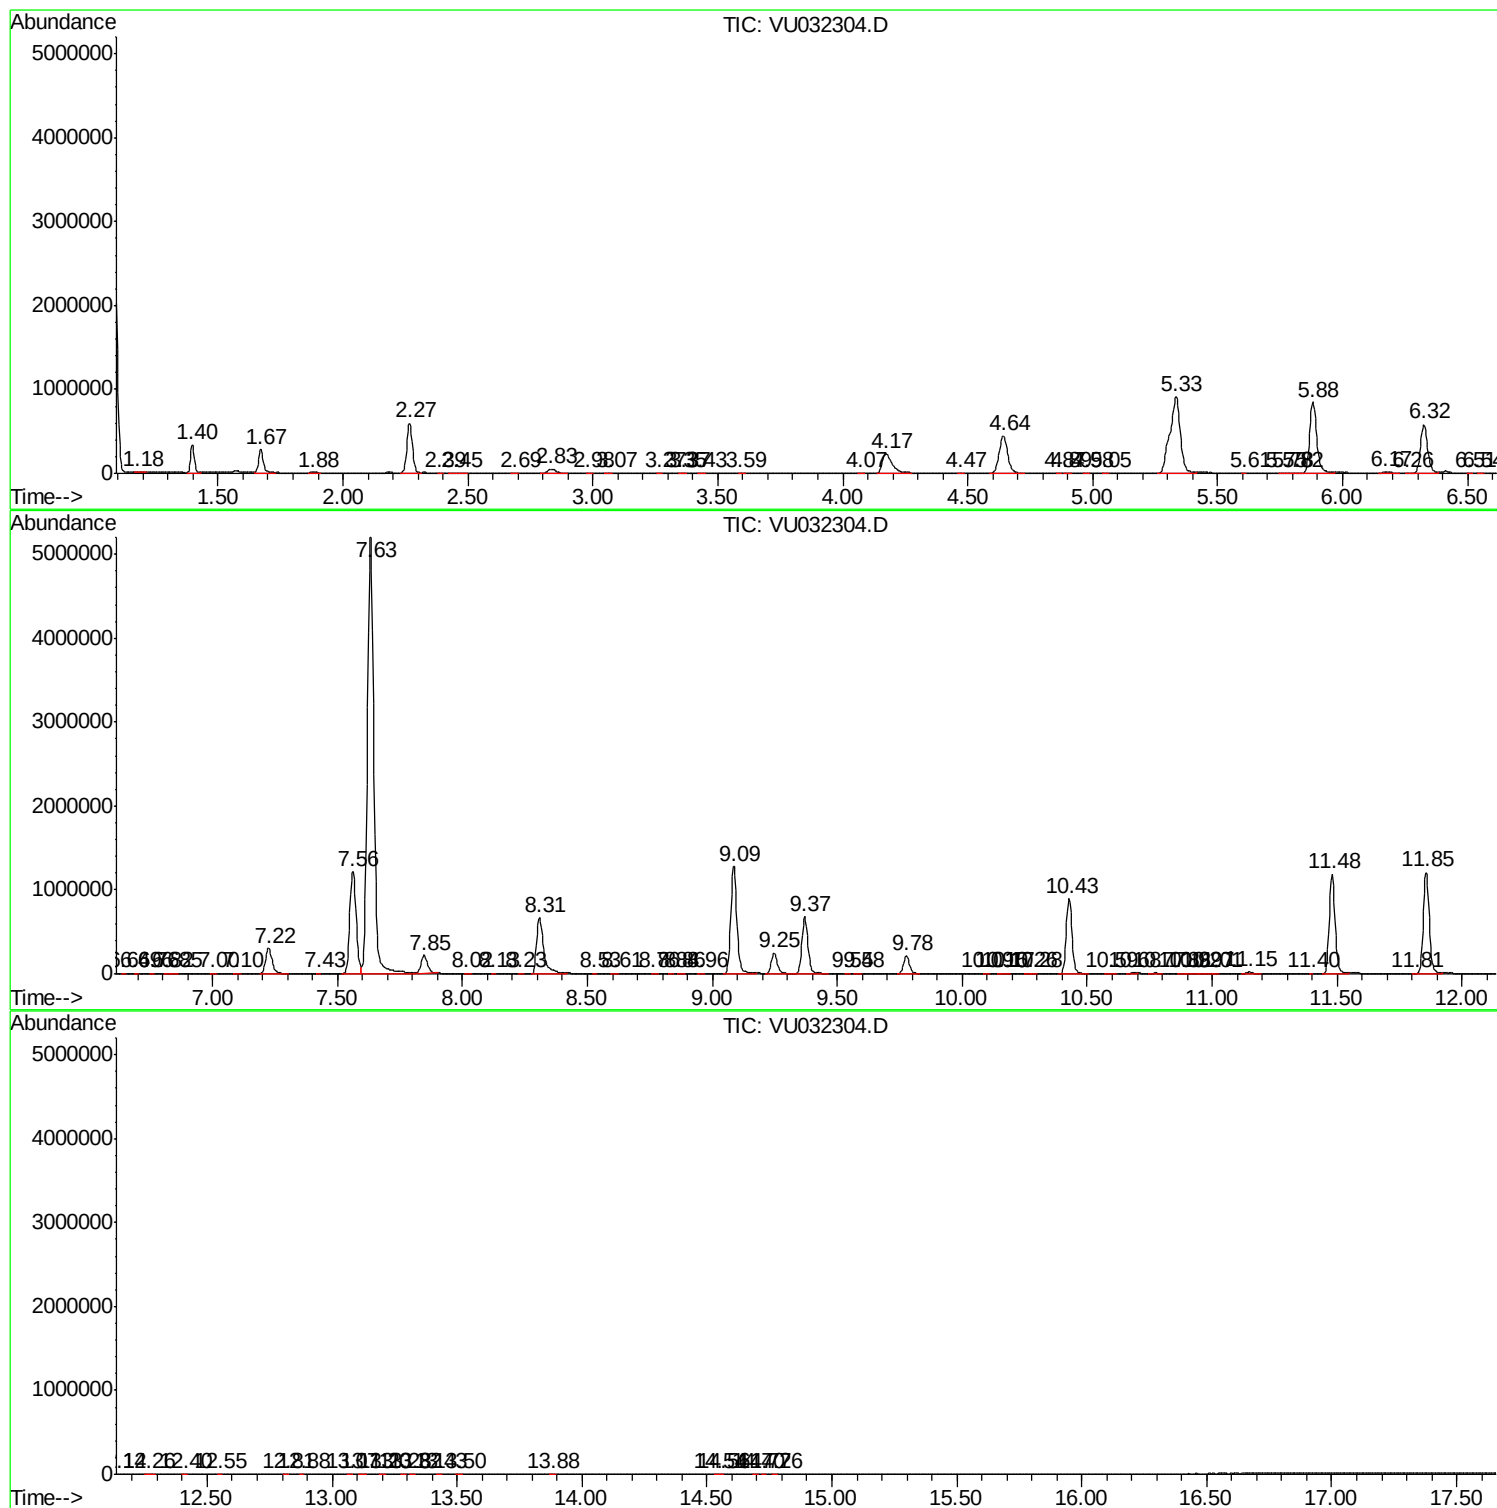

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU052419\
Data File : VU032304.D
Acq On : 24 May 2019 11:28
Operator : JC/SP
Sample : K3001-12 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YF7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU052419\
Data File : VU032304.D
Acq On : 24 May 2019 11:28
Operator : JC/SP
Sample : K3001-12 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YF7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc