

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032311.D
 Acq On : 24 May 2019 14:13
 Operator : JC/SP
 Sample : K3018-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XJ4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.396	89	95	105	rBV	364492	362578	13.42%	1.559%
2	1.672	173	181	200	rVB	285370	371684	13.75%	1.598%
3	1.881	238	246	260	rVB	219859	298605	11.05%	1.284%
4	2.267	356	366	379	rBV	620295	920044	34.04%	3.956%
5	2.450	412	423	444	rBV	30371	62031	2.30%	0.267%
6	2.662	486	489	493	rBV2	904	633	0.02%	0.003%
7	2.833	530	542	556	rBV2	12369	26250	0.97%	0.113%
8	2.997	590	593	594	rBV2	501	251	0.01%	0.001%
9	3.106	624	627	629	rVB2	359	215	0.01%	0.001%
10	3.122	629	632	633	rBV	391	194	0.01%	0.001%
11	3.158	641	643	646	rBV2	248	180	0.01%	0.001%
12	3.273	677	679	681	rBV2	341	235	0.01%	0.001%
13	3.296	684	686	689	rVB	470	289	0.01%	0.001%
14	3.486	742	745	748	rBV2	502	279	0.01%	0.001%
15	3.502	748	750	753	rVB3	463	205	0.01%	0.001%
16	3.566	768	770	772	rVB2	672	249	0.01%	0.001%
17	3.585	772	776	778	rBV	582	409	0.02%	0.002%
18	3.630	787	790	797	rVB4	477	591	0.02%	0.003%
19	3.662	797	800	802	rBV	487	305	0.01%	0.001%
20	3.691	808	809	811	rVB	440	87	0.00%	0.000%
21	3.707	811	814	817	rBV	506	322	0.01%	0.001%
22	3.749	824	827	828	rBV	282	156	0.01%	0.001%
23	3.820	846	849	852	rBV	345	298	0.01%	0.001%
24	3.875	863	866	868	rBV2	280	187	0.01%	0.001%
25	3.916	874	879	882	rBV4	673	585	0.02%	0.003%
26	3.929	882	883	888	rVB	705	419	0.02%	0.002%
27	3.958	888	892	894	rBV2	349	258	0.01%	0.001%
28	3.977	894	898	899	rBV2	362	219	0.01%	0.001%
29	4.006	903	907	909	rBV3	867	675	0.02%	0.003%
30	4.035	913	916	918	rBV	251	134	0.00%	0.001%
31	4.048	918	920	922	rVV2	452	234	0.01%	0.001%
32	4.067	922	926	931	rVV3	726	661	0.02%	0.003%
33	4.093	932	934	937	rVB	401	212	0.01%	0.001%
34	4.174	946	959	989	rBV	225513	618247	22.88%	2.658%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032311.D
 Acq On : 24 May 2019 14:13
 Operator : JC/SP
 Sample : K3018-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XJ4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

35	4.643	1088	1105	1134	rBV2	453390	1079102	39.93%	4.640%
36	4.823	1159	1161	1162	rBV2	767	293	0.01%	0.001%
37	4.862	1171	1173	1175	rBV3	1676	752	0.03%	0.003%
38	5.058	1231	1234	1236	rBV3	509	345	0.01%	0.001%
39	5.125	1244	1255	1256	rBV5	4111	4909	0.18%	0.021%
40	5.222	1281	1285	1287	rBV	621	440	0.02%	0.002%
41	5.334	1297	1320	1348	rBV2	917707	2702458	100.00%	11.620%
42	5.743	1443	1447	1450	rBV3	675	622	0.02%	0.003%
43	5.881	1477	1490	1522	rBV	836390	1716720	63.52%	7.381%
44	6.183	1574	1584	1602	rVB5	50614	113374	4.20%	0.487%
45	6.325	1615	1628	1653	rBV	575446	1166321	43.16%	5.015%
46	6.579	1702	1707	1709	rBV4	865	771	0.03%	0.003%
47	6.617	1717	1719	1721	rVB2	934	419	0.02%	0.002%
48	6.633	1721	1724	1727	rBV2	1018	669	0.02%	0.003%
49	6.736	1753	1756	1758	rBV3	428	252	0.01%	0.001%
50	6.765	1763	1765	1766	rBV3	399	140	0.01%	0.001%
51	6.849	1788	1791	1793	rBV	427	250	0.01%	0.001%
52	6.878	1796	1800	1801	rBV3	1548	1028	0.04%	0.004%
53	6.984	1831	1833	1835	rBV2	484	317	0.01%	0.001%
54	7.109	1867	1872	1873	rBV2	580	427	0.02%	0.002%
55	7.164	1886	1889	1890	rBV	269	145	0.01%	0.001%
56	7.225	1896	1908	1931	rBV	303272	559649	20.71%	2.406%
57	7.559	1999	2012	2033	rBV	1243474	2202912	81.52%	9.472%
58	7.845	2091	2101	2124	rBV	215749	374527	13.86%	1.610%
59	8.222	2206	2218	2235	rBV	1133801	1948908	72.12%	8.380%
60	8.308	2236	2245	2283	rVB2	667062	1297652	48.02%	5.580%
61	8.804	2396	2399	2401	rBV2	812	431	0.02%	0.002%
62	8.897	2427	2428	2431	rBV2	590	302	0.01%	0.001%
63	9.083	2474	2486	2511	rBV	1261131	2155310	79.75%	9.267%
64	9.379	2568	2578	2585	rBV7	5068	8657	0.32%	0.037%
65	9.530	2620	2625	2626	rBV3	728	539	0.02%	0.002%
66	9.652	2661	2663	2667	rBV4	683	564	0.02%	0.002%
67	9.710	2679	2681	2682	rBV	580	223	0.01%	0.001%
68	9.755	2687	2695	2698	rBV5	1529	1554	0.06%	0.007%
69	9.813	2710	2713	2716	rBV2	986	668	0.02%	0.003%
70	10.016	2773	2776	2778	rBV	830	441	0.02%	0.002%
71	10.135	2809	2813	2819	rBV3	734	856	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032311.D
 Acq On : 24 May 2019 14:13
 Operator : JC/SP
 Sample : K3018-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XJ4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

72	10.276	2854	2857	2859	rBV2	635	428	0.02%	0.002%
73	10.379	2886	2889	2891	rBV2	751	448	0.02%	0.002%
74	10.427	2891	2904	2929	rVV	893299	1444044	53.43%	6.209%
75	10.681	2981	2983	2986	rBV	640	468	0.02%	0.002%
76	10.884	3041	3046	3049	rBV3	521	614	0.02%	0.003%
77	10.977	3073	3075	3076	rVB2	564	146	0.01%	0.001%
78	11.086	3104	3109	3110	rBV2	1447	1129	0.04%	0.005%
79	11.318	3178	3181	3185	rBV2	670	386	0.01%	0.002%
80	11.479	3219	3231	3254	rBV	1113703	1836438	67.95%	7.896%
81	11.855	3336	3348	3374	rBV	1155277	1961165	72.57%	8.433%
82	12.765	3629	3631	3637	rBV2	912	600	0.02%	0.003%
83	13.617	3894	3896	3898	rBV2	1027	474	0.02%	0.002%


Sum of corrected areas: 23257208

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU052419\
Data File : VU032311.D
Acq On : 24 May 2019 14:13
Operator : JC/SP
Sample : K3018-07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XJ4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

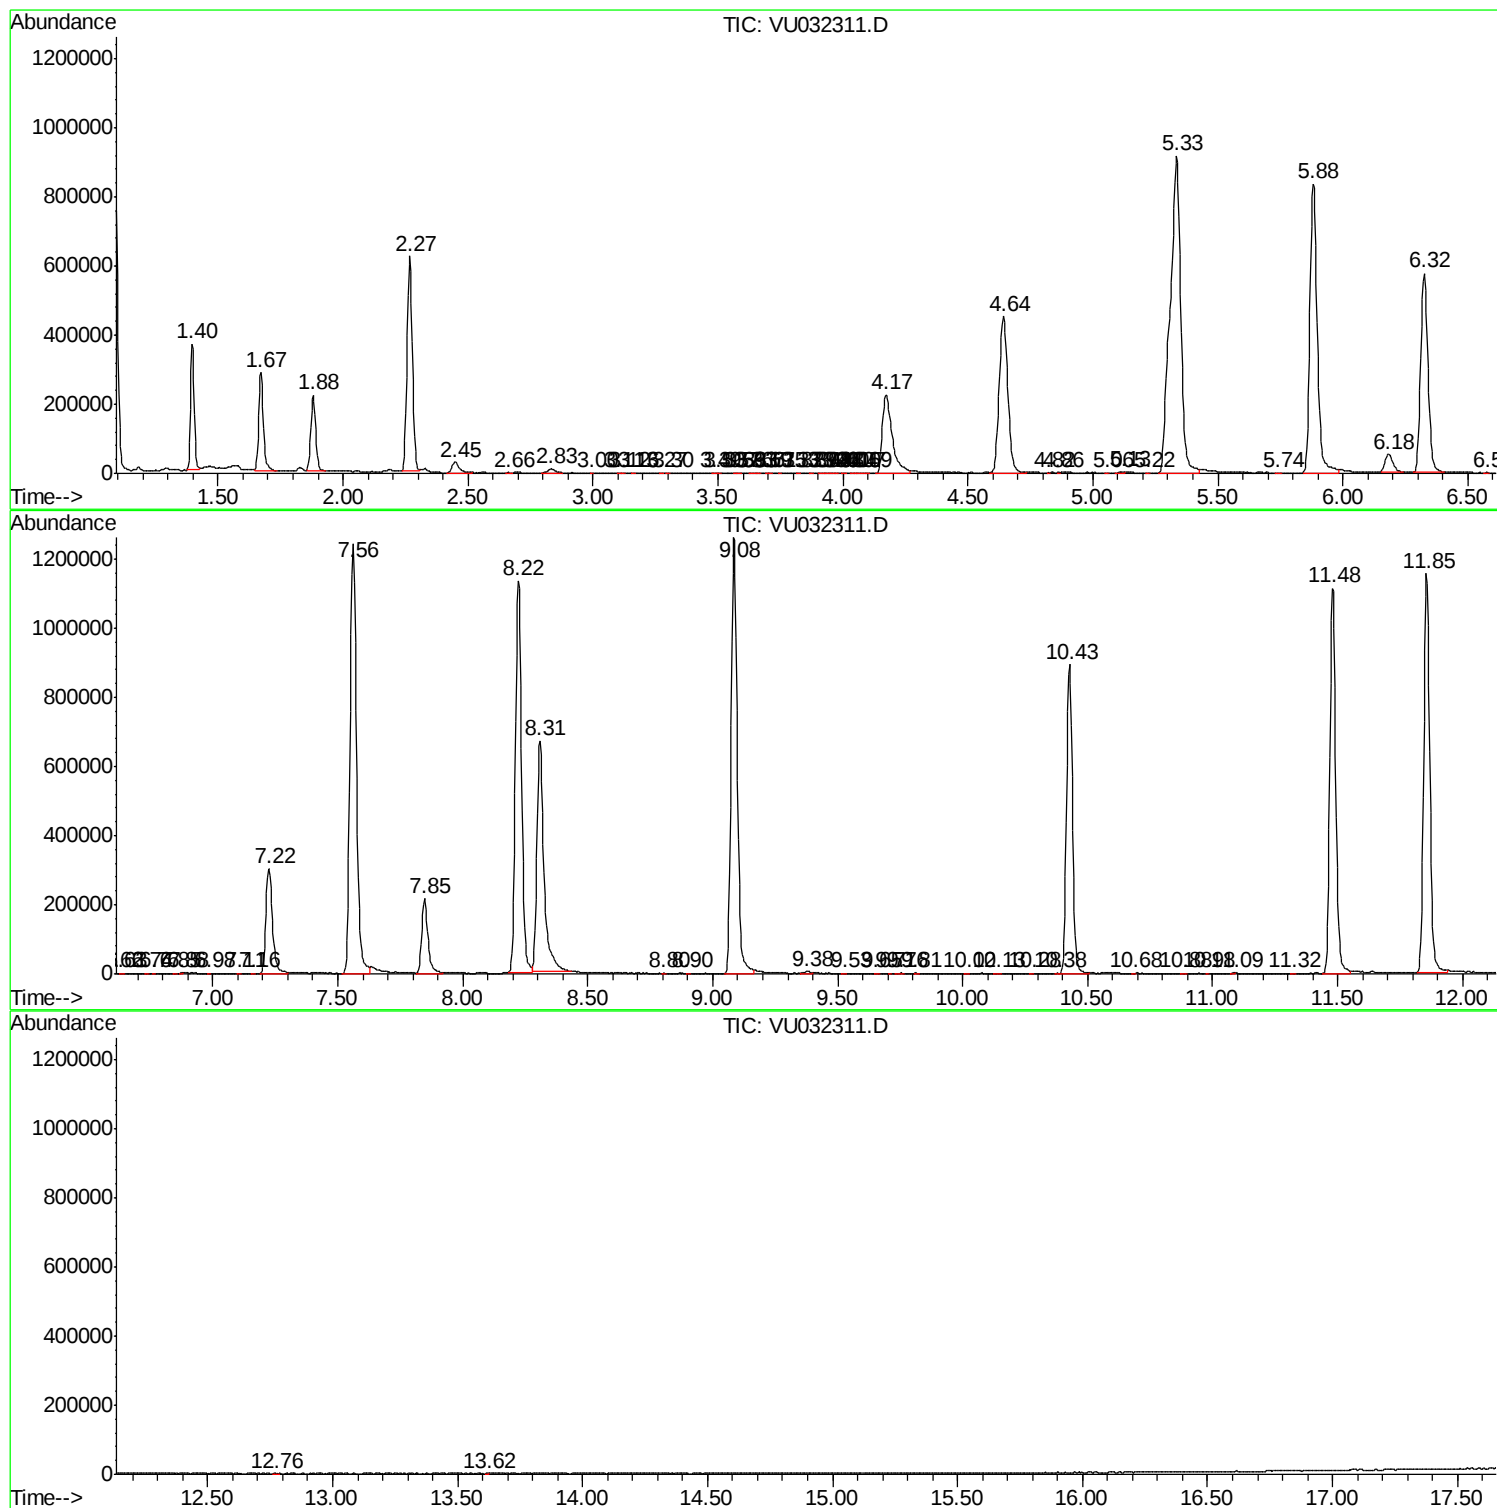

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU052419\
Data File : VU032311.D
Acq On : 24 May 2019 14:13
Operator : JC/SP
Sample : K3018-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XJ4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU052419\
Data File : VU032311.D
Acq On : 24 May 2019 14:13
Operator : JC/SP
Sample : K3018-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XJ4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc