

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032314.D
 Acq On : 24 May 2019 16:47
 Operator : JC/SP
 Sample : K3001-09DL 250X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YF4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	35	rVB2	10902	10827	0.43%	0.047%
2	1.395	88	95	105	rBV	311220	332784	13.21%	1.449%
3	1.672	173	181	200	rVB	252067	343762	13.65%	1.497%
4	2.267	356	366	379	rVB	558483	837483	33.25%	3.647%
5	2.450	414	423	424	rBV2	6354	6754	0.27%	0.029%
6	2.601	465	470	473	rVB3	814	596	0.02%	0.003%
7	2.698	495	500	510	rVB5	3528	5057	0.20%	0.022%
8	2.836	528	543	560	rVV2	57620	124274	4.93%	0.541%
9	2.981	579	588	599	rBV6	2525	4423	0.18%	0.019%
10	3.193	651	654	656	rBV3	672	532	0.02%	0.002%
11	3.286	679	683	685	rBV2	672	543	0.02%	0.002%
12	3.444	725	732	736	rBV4	1005	1394	0.06%	0.006%
13	3.498	744	749	753	rBV2	595	661	0.03%	0.003%
14	3.727	817	820	826	rVB3	662	620	0.02%	0.003%
15	3.894	866	872	875	rBV3	773	822	0.03%	0.004%
16	3.971	892	896	901	rBV2	748	759	0.03%	0.003%
17	4.003	901	906	909	rBV2	743	654	0.03%	0.003%
18	4.058	920	923	928	rBV2	558	556	0.02%	0.002%
19	4.173	942	959	986	rBV	226258	636865	25.28%	2.773%
20	4.517	1064	1066	1070	rBV2	691	534	0.02%	0.002%
21	4.643	1089	1105	1134	rBV	423453	1005095	39.90%	4.377%
22	4.810	1155	1157	1161	rVB4	1299	693	0.03%	0.003%
23	4.842	1162	1167	1171	rBV4	970	1013	0.04%	0.004%
24	4.980	1206	1210	1214	rBV4	1428	1577	0.06%	0.007%
25	5.083	1236	1242	1246	rBV2	797	818	0.03%	0.004%
26	5.334	1296	1320	1345	rBV2	853800	2518919	100.00%	10.969%
27	5.620	1405	1409	1414	rBV5	1445	1553	0.06%	0.007%
28	5.675	1423	1426	1429	rBV4	1258	884	0.04%	0.004%
29	5.765	1451	1454	1460	rVB3	819	690	0.03%	0.003%
30	5.813	1467	1469	1474	rVB3	721	590	0.02%	0.003%
31	5.881	1477	1490	1525	rBV	828069	1683112	66.82%	7.329%
32	6.177	1569	1582	1596	rBV10	12011	28792	1.14%	0.125%
33	6.324	1614	1628	1646	rBV	546674	1104205	43.84%	4.808%
34	6.543	1694	1696	1705	rVB6	1509	1442	0.06%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032314.D
 Acq On : 24 May 2019 16:47
 Operator : JC/SP
 Sample : K3001-09DL 250X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YF4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

35	6.585	1705	1709	1713	rBV5	741	732	0.03%	0.003%
36	6.607	1713	1716	1722	rVB6	995	963	0.04%	0.004%
37	6.733	1750	1755	1757	rBV3	752	624	0.02%	0.003%
38	6.881	1794	1801	1804	rBV6	1632	2051	0.08%	0.009%
39	6.996	1834	1837	1843	rVB2	761	707	0.03%	0.003%
40	7.064	1854	1858	1863	rBV3	836	874	0.03%	0.004%
41	7.157	1884	1887	1889	rBV	913	554	0.02%	0.002%
42	7.225	1894	1908	1938	rBV	290554	537830	21.35%	2.342%
43	7.353	1945	1948	1949	rBV2	1031	589	0.02%	0.003%
44	7.376	1954	1955	1962	rVB5	1399	1402	0.06%	0.006%
45	7.411	1962	1966	1967	rBV3	1369	929	0.04%	0.004%
46	7.472	1976	1985	1998	rVB6	7592	16325	0.65%	0.071%
47	7.562	1998	2013	2028	rBV	1153246	2029986	80.59%	8.840%
48	7.636	2031	2036	2058	rVB	68042	126962	5.04%	0.553%
49	7.845	2090	2101	2118	rBV	200131	355734	14.12%	1.549%
50	8.032	2156	2159	2164	rBV6	856	1004	0.04%	0.004%
51	8.138	2187	2192	2195	rBV3	741	550	0.02%	0.002%
52	8.173	2201	2203	2207	rVB2	1057	760	0.03%	0.003%
53	8.228	2212	2220	2221	rBV4	2032	2144	0.09%	0.009%
54	8.308	2231	2245	2283	rBV2	644046	1291148	51.26%	5.622%
55	8.578	2325	2329	2330	rBV3	1176	856	0.03%	0.004%
56	8.633	2343	2346	2348	rBV4	1040	685	0.03%	0.003%
57	8.897	2424	2428	2436	rVB4	776	858	0.03%	0.004%
58	9.086	2473	2487	2518	rBV	1230737	2102538	83.47%	9.156%
59	9.254	2530	2539	2552	rVB	22991	36438	1.45%	0.159%
60	9.369	2562	2575	2614	rBV	1351189	2257623	89.63%	9.831%
61	9.543	2626	2629	2633	rBV4	1132	827	0.03%	0.004%
62	9.643	2656	2660	2663	rBV4	1229	1187	0.05%	0.005%
63	9.694	2671	2676	2678	rBV6	788	692	0.03%	0.003%
64	9.781	2696	2703	2705	rBV3	7278	7796	0.31%	0.034%
65	9.871	2728	2731	2739	rVB6	1108	1038	0.04%	0.005%
66	9.961	2755	2759	2762	rBV3	936	749	0.03%	0.003%
67	9.996	2765	2770	2773	rVV2	592	602	0.02%	0.003%
68	10.164	2813	2822	2834	rBV2	13292	21696	0.86%	0.094%
69	10.427	2890	2904	2923	rBV	878778	1423886	56.53%	6.200%
70	10.591	2948	2955	2962	rBV5	5030	6692	0.27%	0.029%
71	10.684	2973	2984	3001	rBV2	10780	25212	1.00%	0.110%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052419\
 Data File : VU032314.D
 Acq On : 24 May 2019 16:47
 Operator : JC/SP
 Sample : K3001-09DL 250X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YF4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis

72	10.771	3005	3011	3023	rVB3	9482	13607	0.54%	0.059%
73	10.977	3062	3075	3089	rVB3	6305	12217	0.49%	0.053%
74	11.147	3118	3128	3141	rBV2	25179	41693	1.66%	0.182%
75	11.321	3176	3182	3188	rBV5	1784	2365	0.09%	0.010%
76	11.421	3202	3213	3219	rBV6	9674	17075	0.68%	0.074%
77	11.479	3220	3231	3253	rBV	1164783	1894413	75.21%	8.249%
78	11.636	3277	3280	3282	rBV3	1328	912	0.04%	0.004%
79	11.855	3336	3348	3381	rBV	1177339	1961783	77.88%	8.543%
80	12.183	3447	3450	3452	rVB3	1763	989	0.04%	0.004%
81	12.257	3471	3473	3474	rBV2	1168	556	0.02%	0.002%
82	12.636	3589	3591	3593	rVV3	953	543	0.02%	0.002%
83	12.668	3595	3601	3606	rVV6	1969	2616	0.10%	0.011%
84	12.897	3663	3672	3683	rBV7	9011	18614	0.74%	0.081%
85	13.016	3705	3709	3712	rBV4	1563	1357	0.05%	0.006%
86	13.118	3736	3741	3743	rBV4	2028	1647	0.07%	0.007%
87	13.289	3790	3794	3797	rBV2	1281	1172	0.05%	0.005%
88	13.421	3832	3835	3839	rBV2	828	683	0.03%	0.003%
89	13.524	3855	3867	3875	rBV8	8835	20413	0.81%	0.089%
90	13.761	3930	3941	3944	rBV	12635	22287	0.88%	0.097%
91	13.993	4004	4013	4017	rBV5	13426	20774	0.82%	0.090%
92	14.414	4140	4144	4147	rBV3	951	905	0.04%	0.004%
93	14.524	4175	4178	4180	rBV2	1004	606	0.02%	0.003%
94	14.536	4180	4182	4185	rVB2	1301	716	0.03%	0.003%
95	14.704	4232	4234	4239	rBV3	807	569	0.02%	0.002%
96	14.848	4273	4279	4280	rBV3	1257	1239	0.05%	0.005%
97	14.964	4312	4315	4317	rBV2	1150	675	0.03%	0.003%
98	15.109	4356	4360	4364	rBV3	1890	1796	0.07%	0.008%
99	15.144	4368	4371	4374	rBV2	1540	1095	0.04%	0.005%
100	15.218	4391	4394	4396	rBV3	1162	715	0.03%	0.003%


Sum of corrected areas: 22964558

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU052419\
Data File : VU032314.D
Acq On : 24 May 2019 16:47
Operator : JC/SP
Sample : K3001-09DL 250X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YF4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

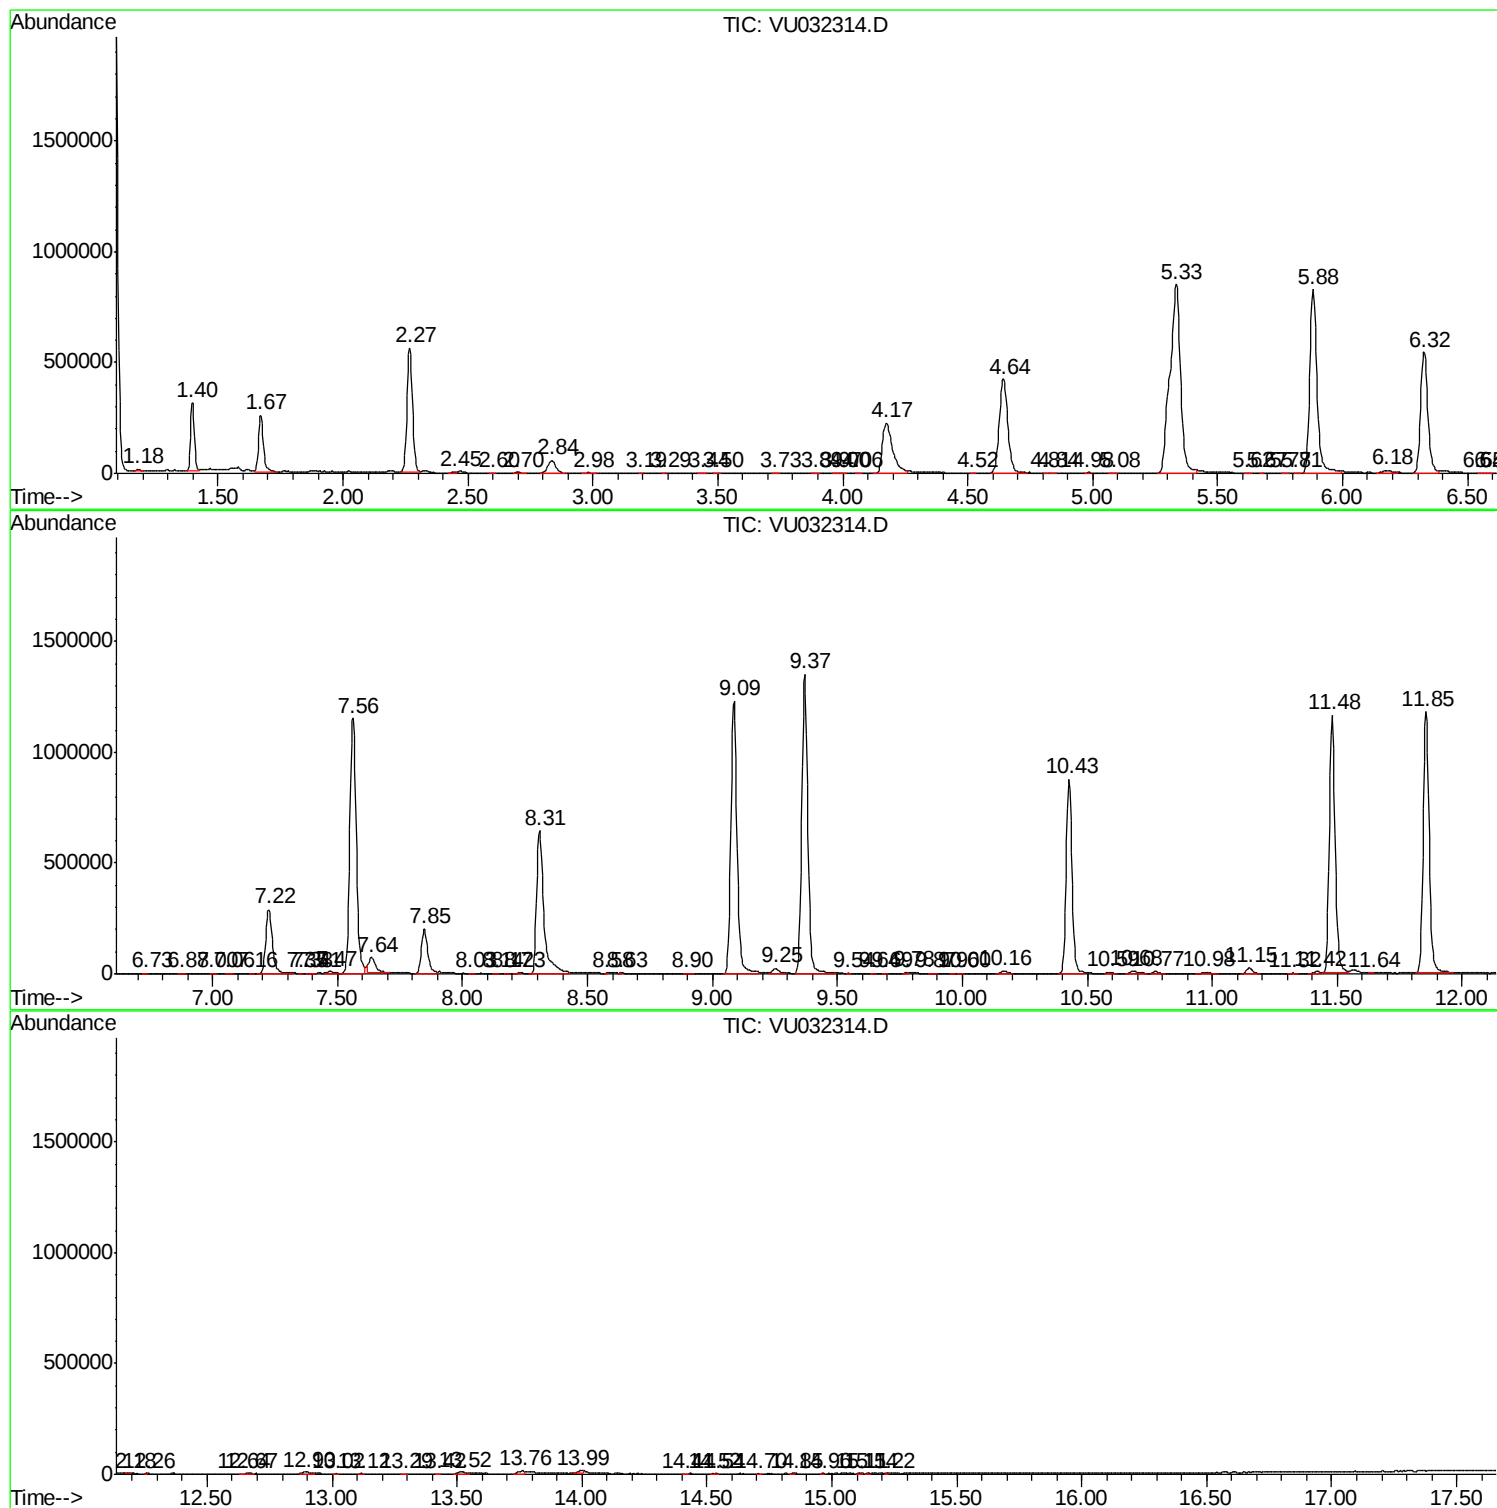

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU052419\
Data File : VU032314.D
Acq On : 24 May 2019 16:47
Operator : JC/SP
Sample : K3001-09DL 250X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YF4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU052419\
Data File : VU032314.D
Acq On : 24 May 2019 16:47
Operator : JC/SP
Sample : K3001-09DL 250X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YF4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc