


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU052419\
 Data File : VU032286.D
 Acq On : 24 May 2019 02:56
 Operator : JC/SP
 Sample : BFB45
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB45

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052419WMA.M
 Title : VOC Analysis
 Last Update : Fri May 24 23:32:32 2019

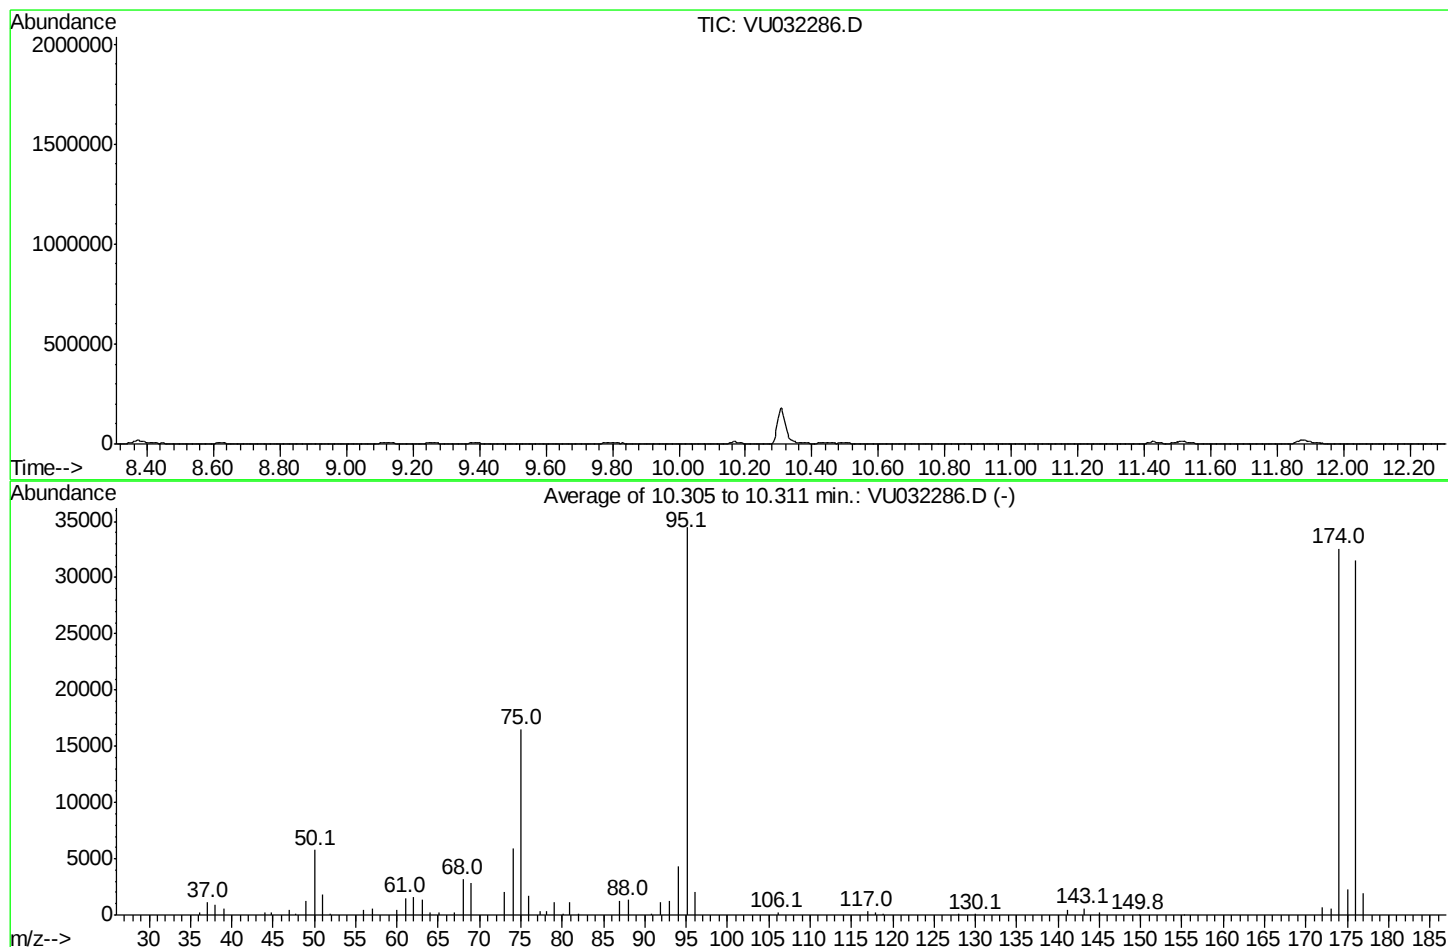

AutoFind: Scans 2866, 2867, 2868; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	5799	PASS
75	95	30	80	47.7	16454	PASS
95	95	100	100	100.0	34469	PASS
96	95	5	9	5.9	2045	PASS
173	174	0.00	2	1.8	578	PASS
174	95	50	120	94.6	32605	PASS
175	174	5	9	7.0	2287	PASS
176	174	95	101	96.7	31538	PASS
177	176	5	9	6.1	1919	PASS

Scan 2854 (10.266 min): VU032286.D
BFB45

m/z	Abundance
39.10	737.0
44.10	449.0
207.10	139.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.10	162.0
37.00	1164.0
38.10	1034.0
39.00	633.0
39.80	435.0
44.00	733.0
44.90	274.0
46.90	466.0
47.80	247.0
49.00	1204.0
50.10	5820.0
51.00	1896.0
51.90	209.0
55.90	432.0
57.00	660.0
60.00	593.0
61.00	1580.0
62.10	1662.0
63.00	1418.0
64.00	198.0
65.20	144.0
67.00	215.0
68.00	3076.0
69.00	2711.0
73.10	2188.0
74.10	6039.0
75.00	17256.0
76.00	2067.0
77.30	321.0
78.20	363.0
79.00	1291.0
80.10	117.0
80.90	1130.0
81.90	210.0
87.00	1517.0
88.00	1335.0
90.90	132.0
92.00	1161.0
93.00	1381.0
94.00	4209.0
95.10	34968.0
96.10	2364.0
106.10	207.0
117.00	307.0
117.90	247.0
118.80	231.0
141.10	309.0
143.10	621.0
145.00	254.0
149.80	111.0
155.20	105.0
172.00	643.0
173.10	648.0
174.00	33080.0
175.10	2258.0
176.00	31368.0
177.00	2020.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.10	196.0
37.10	1125.0
38.00	923.0
39.00	518.0
39.80	467.0
44.00	654.0
44.90	241.0
46.90	571.0
47.80	166.0
48.90	1297.0
50.10	6082.0
51.00	1863.0
51.90	130.0
55.90	432.0
57.00	631.0
60.00	491.0
61.00	1572.0
62.10	1642.0
63.00	1377.0
64.10	245.0
65.20	224.0
67.00	255.0
68.00	3396.0
69.00	2856.0
73.10	2196.0
74.10	6155.0
75.00	16776.0
76.00	1794.0
77.30	319.0
78.20	325.0
79.00	1116.0
80.10	136.0
80.90	1197.0
81.90	172.0
87.00	1231.0
88.00	1381.0
90.70	178.0
92.00	1270.0
93.00	1241.0
94.00	4657.0
95.10	35608.0
96.10	2124.0
106.10	251.0
116.90	341.0
117.80	264.0
118.90	150.0
127.90	107.0
130.00	132.0
141.10	466.0
143.10	556.0
145.00	272.0
171.90	722.0
173.10	599.0
174.00	33840.0
175.10	2385.0
176.00	32600.0
177.00	1975.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	194.0
37.10	1117.0
37.90	847.0
39.00	398.0
39.80	525.0
43.90	601.0
44.80	186.0
46.90	373.0
47.80	100.0
49.00	1318.0
50.10	5495.0
51.00	1674.0
55.90	392.0
57.00	547.0
60.00	261.0
61.00	1445.0
62.00	1456.0
63.00	1370.0
64.10	214.0
65.10	265.0
67.00	166.0
68.00	3054.0
69.00	3034.0
73.00	1732.0
74.10	5548.0
75.10	15330.0
76.00	1336.0
77.20	251.0
78.10	293.0
78.90	989.0
80.10	183.0
80.90	1129.0
82.00	132.0
87.00	1059.0
88.00	1262.0
90.70	156.0
91.90	1117.0
93.00	1024.0
94.00	4215.0
95.10	32832.0
96.10	1649.0
106.10	212.0
116.90	369.0
117.80	263.0
119.00	117.0
127.90	165.0
130.10	143.0
141.10	495.0
143.10	422.0
145.00	293.0
171.90	694.0
173.00	487.0
174.00	30896.0
175.10	2219.0
176.00	30648.0
177.00	1763.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45