

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052421\
 Data File : VU043914.D
 Acq On : 24 May 2021 17:38
 Operator : SY/MD
 Sample : VU0524WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK199

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR052421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043914.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	94	rVB	86666	97347	11.47%	1.465%
2	1.912	169	178	190	rVB	63855	81195	9.57%	1.222%
3	2.565	369	381	398	rVB	137118	219194	25.82%	3.298%
4	3.051	522	532	542	rVB2	8825	15828	1.86%	0.238%
5	4.694	1024	1043	1091	rBV2	98611	393346	46.34%	5.919%
6	5.073	1143	1161	1191	rVB	156865	343188	40.43%	5.164%
7	5.729	1346	1365	1390	rBV2	338083	808433	95.25%	12.165%
8	6.256	1513	1529	1550	rBV	277581	517247	60.94%	7.783%
9	6.700	1651	1667	1686	rBV	198256	377782	44.51%	5.685%
10	7.575	1925	1939	1957	rBV	95090	163753	19.29%	2.464%
11	7.902	2025	2041	2056	rBV	366549	634355	74.74%	9.546%
12	7.973	2057	2063	2075	rVB	5841	10438	1.23%	0.157%
13	8.185	2118	2129	2144	rBV2	59910	99928	11.77%	1.504%
14	8.648	2259	2273	2304	rBV	457793	848781	100.00%	12.772%
15	8.928	2352	2360	2372	rVB3	4872	8501	1.00%	0.128%
16	9.423	2500	2514	2530	rBV	393866	642063	75.65%	9.662%
17	10.764	2915	2931	2951	rBV	166480	263912	31.09%	3.971%
18	11.819	3246	3259	3273	rBV	352475	555181	65.41%	8.354%
19	12.198	3365	3377	3394	rBV	351603	565073	66.57%	8.503%




Sum of corrected areas: 6645545

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052421\
Data File : VU043914.D
Acq On : 24 May 2021 17:38
Operator : SY/MD
Sample : VU0524WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK199

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR052421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

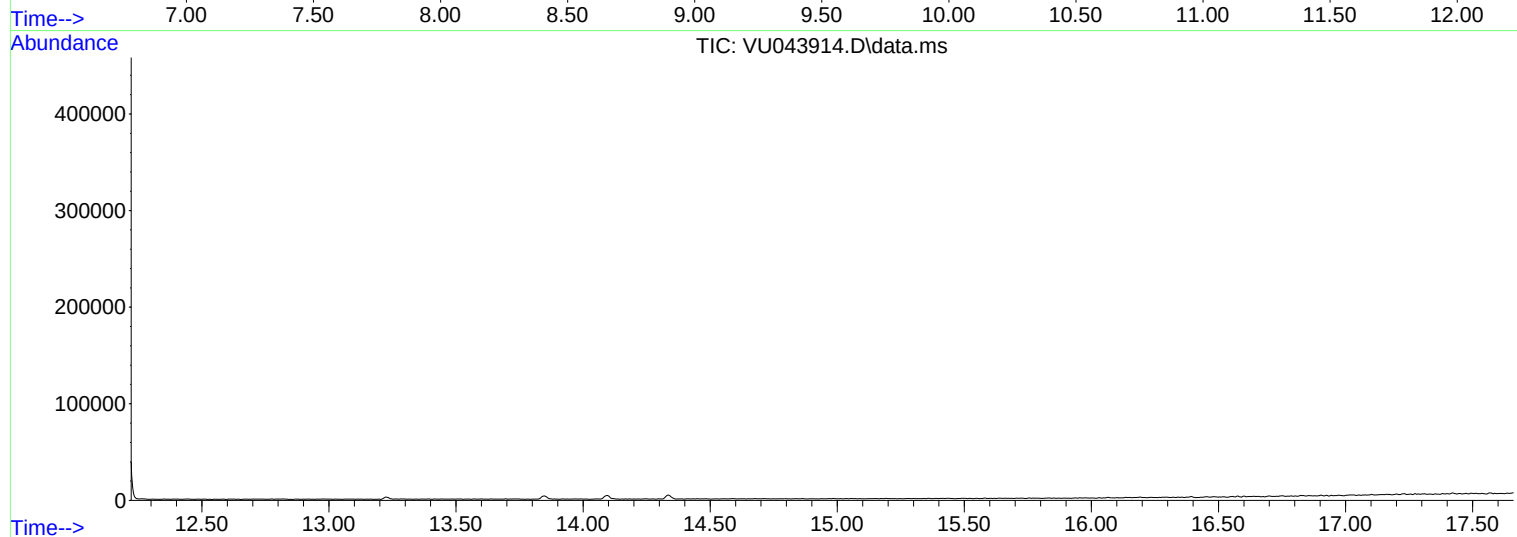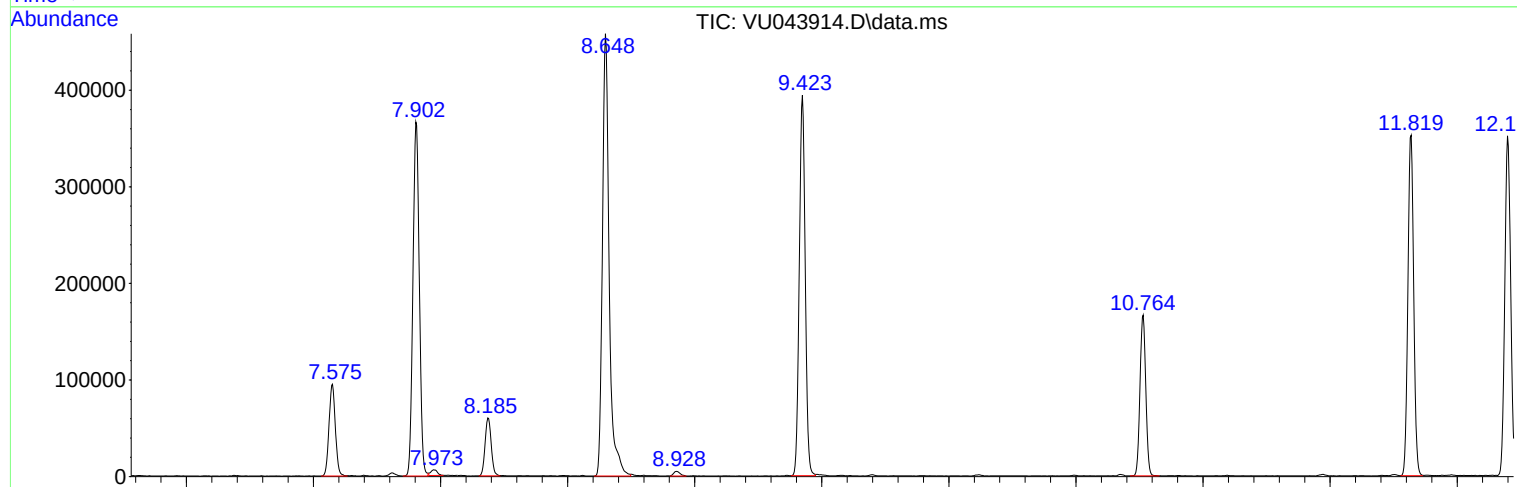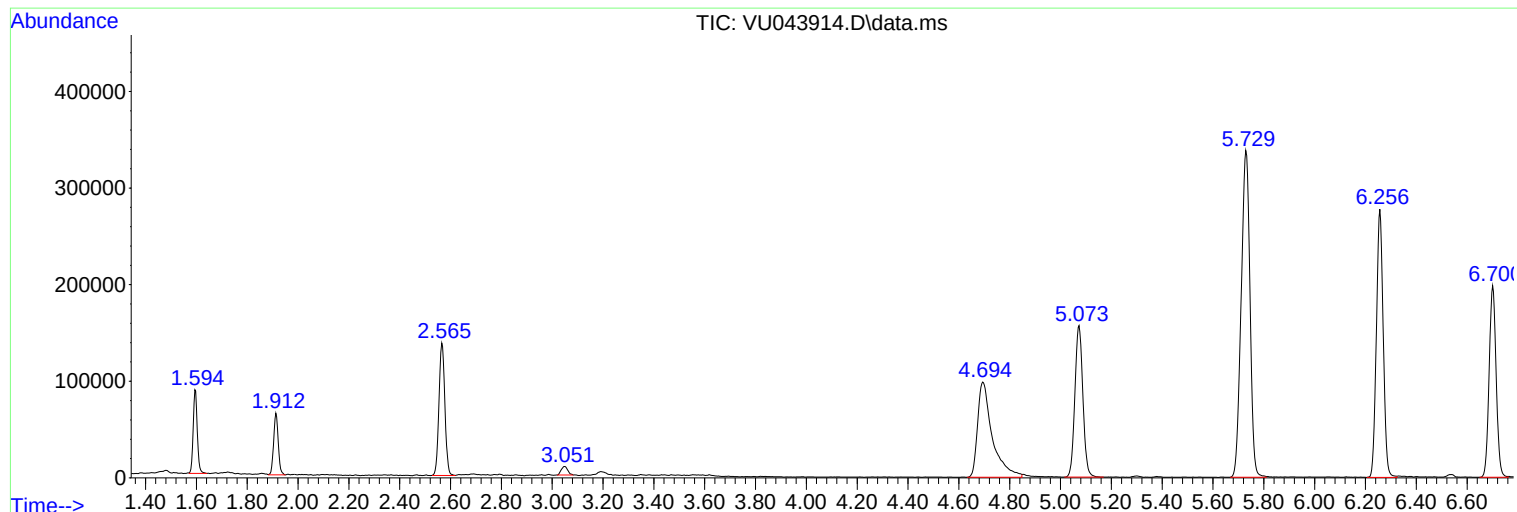

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052421\
Data File : VU043914.D
Acq On : 24 May 2021 17:38
Operator : SY/MD
Sample : VU0524WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK199

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR052421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052421\
Data File : VU043914.D
Acq On : 24 May 2021 17:38
Operator : SY/MD
Sample : VU0524WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK199

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR052421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
