

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052421\
 Data File : VU043960.D
 Acq On : 25 May 2021 13:48
 Operator : SY/MD
 Sample : M2464-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR052421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043960.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	71	79	94	rVB	68419	76244	9.70%	1.286%
2	1.913	169	178	190	rVB	53157	67522	8.59%	1.139%
3	2.565	369	381	397	rVB	115642	182920	23.27%	3.085%
4	3.048	521	531	541	rBV2	11639	20413	2.60%	0.344%
5	4.697	1019	1044	1101	rBV	95646	367537	46.76%	6.199%
6	5.073	1143	1161	1185	rVB	141652	307050	39.07%	5.179%
7	5.729	1345	1365	1388	rBV2	297879	713846	90.82%	12.040%
8	6.256	1515	1529	1548	rBV	243731	458008	58.27%	7.725%
9	6.700	1653	1667	1686	rBV	174823	338427	43.06%	5.708%
10	7.575	1926	1939	1956	rBV2	82111	141486	18.00%	2.386%
11	7.903	2027	2041	2055	rBV	312310	537823	68.43%	9.071%
12	7.973	2058	2063	2078	rVB	5188	8467	1.08%	0.143%
13	8.189	2118	2130	2146	rBV	52606	86580	11.02%	1.460%
14	8.649	2260	2273	2313	rBV	425053	785994	100.00%	13.257%
15	8.932	2350	2361	2371	rBV3	6712	11821	1.50%	0.199%
16	9.423	2500	2514	2537	rBV	357374	587086	74.69%	9.902%
17	10.764	2918	2931	2947	rVB	155358	244920	31.16%	4.131%
18	11.819	3246	3259	3274	rBV	315689	488032	62.09%	8.231%
19	12.198	3365	3377	3402	rVB	315529	504875	64.23%	8.515%




Sum of corrected areas: 5929051

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052421\
Data File : VU043960.D
Acq On : 25 May 2021 13:48
Operator : SY/MD
Sample : M2464-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR052421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

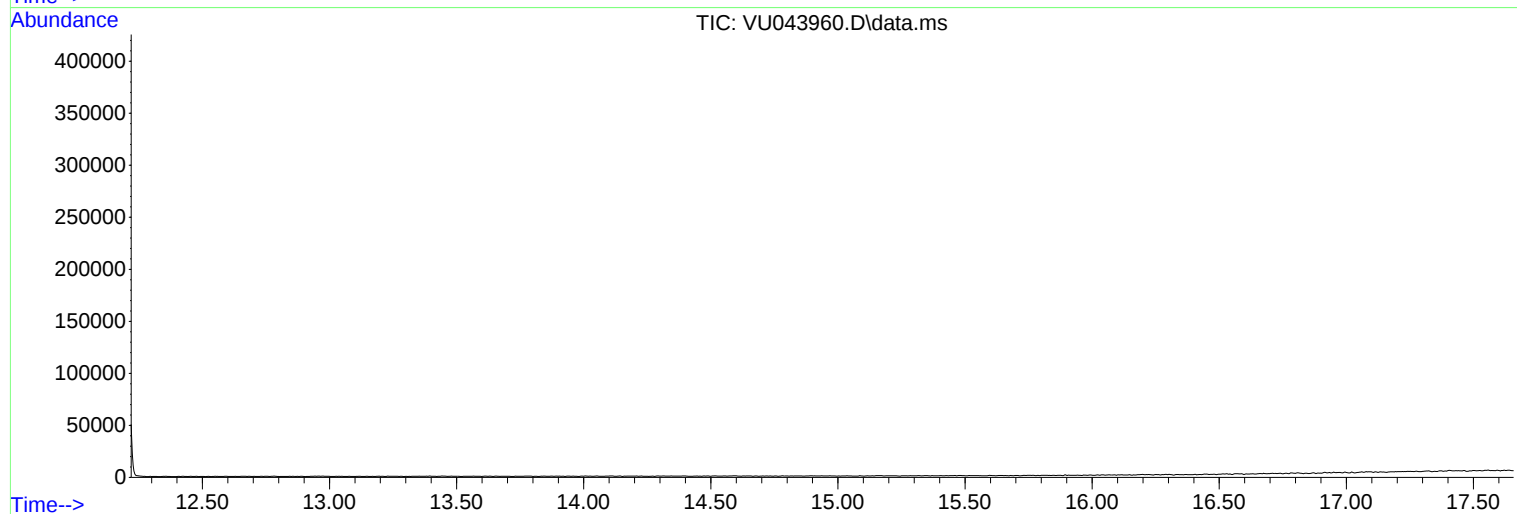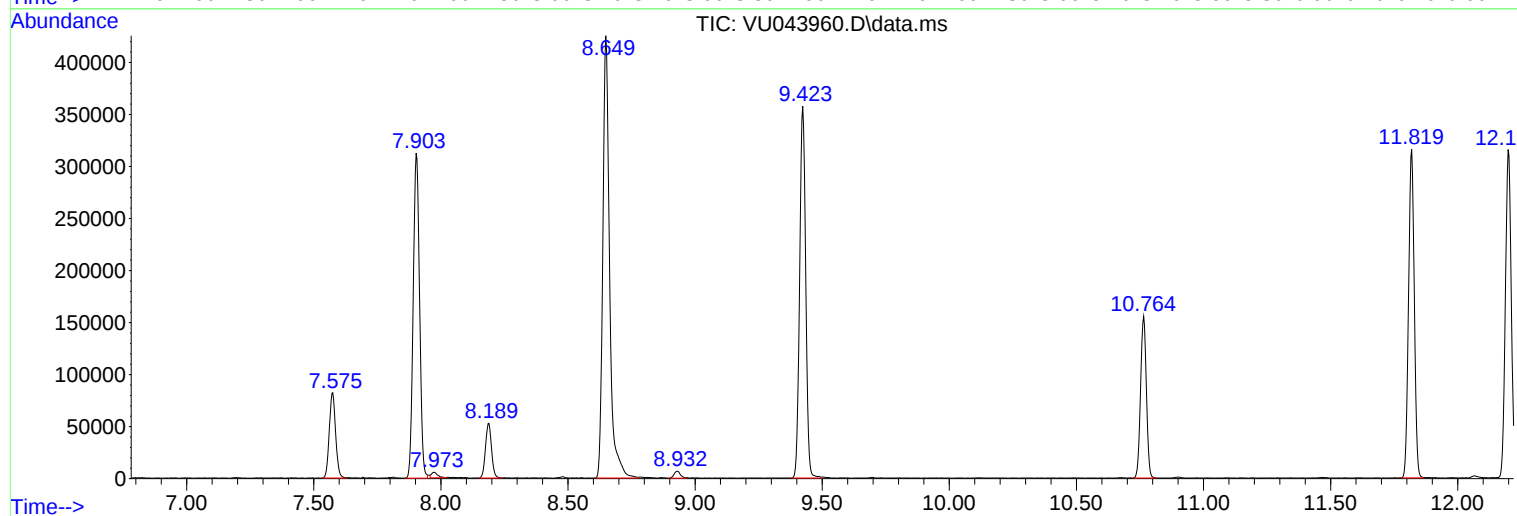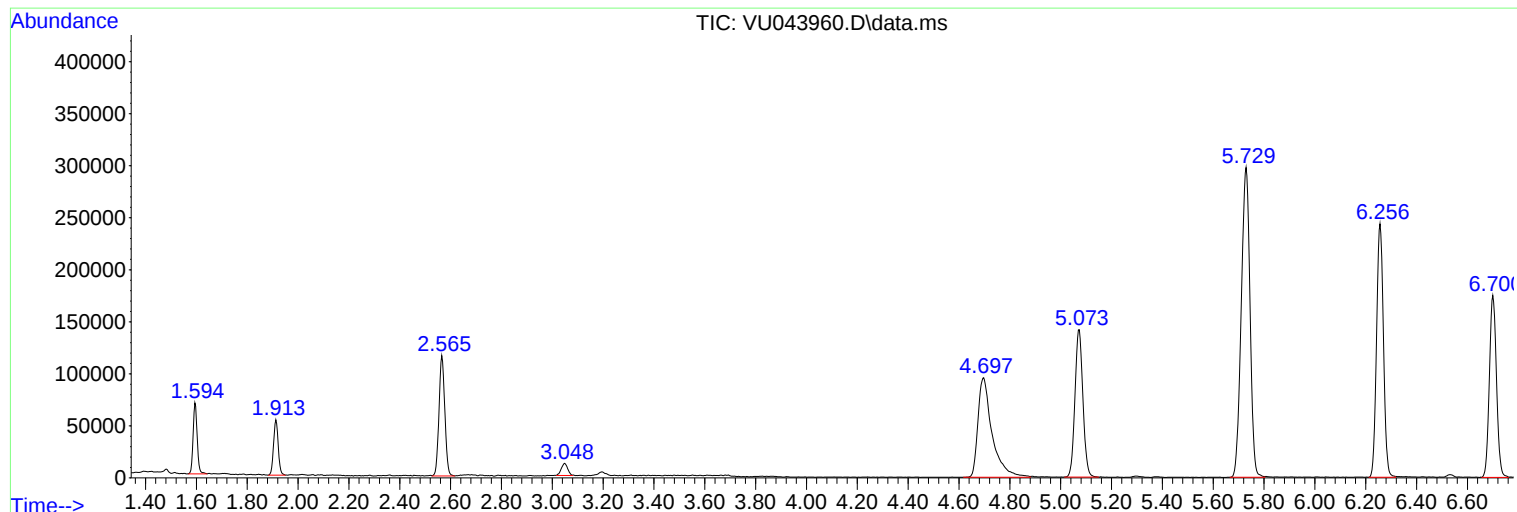

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052421\
Data File : VU043960.D
Acq On : 25 May 2021 13:48
Operator : SY/MD
Sample : M2464-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR052421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052421\
Data File : VU043960.D
Acq On : 25 May 2021 13:48
Operator : SY/MD
Sample : M2464-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR052421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
