


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052421\
 Data File : VU043904.D
 Acq On : 24 May 2021 10:30
 Operator : SY/MD
 Sample : BFB50
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB150

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR052421WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue May 25 07:46:23 2021

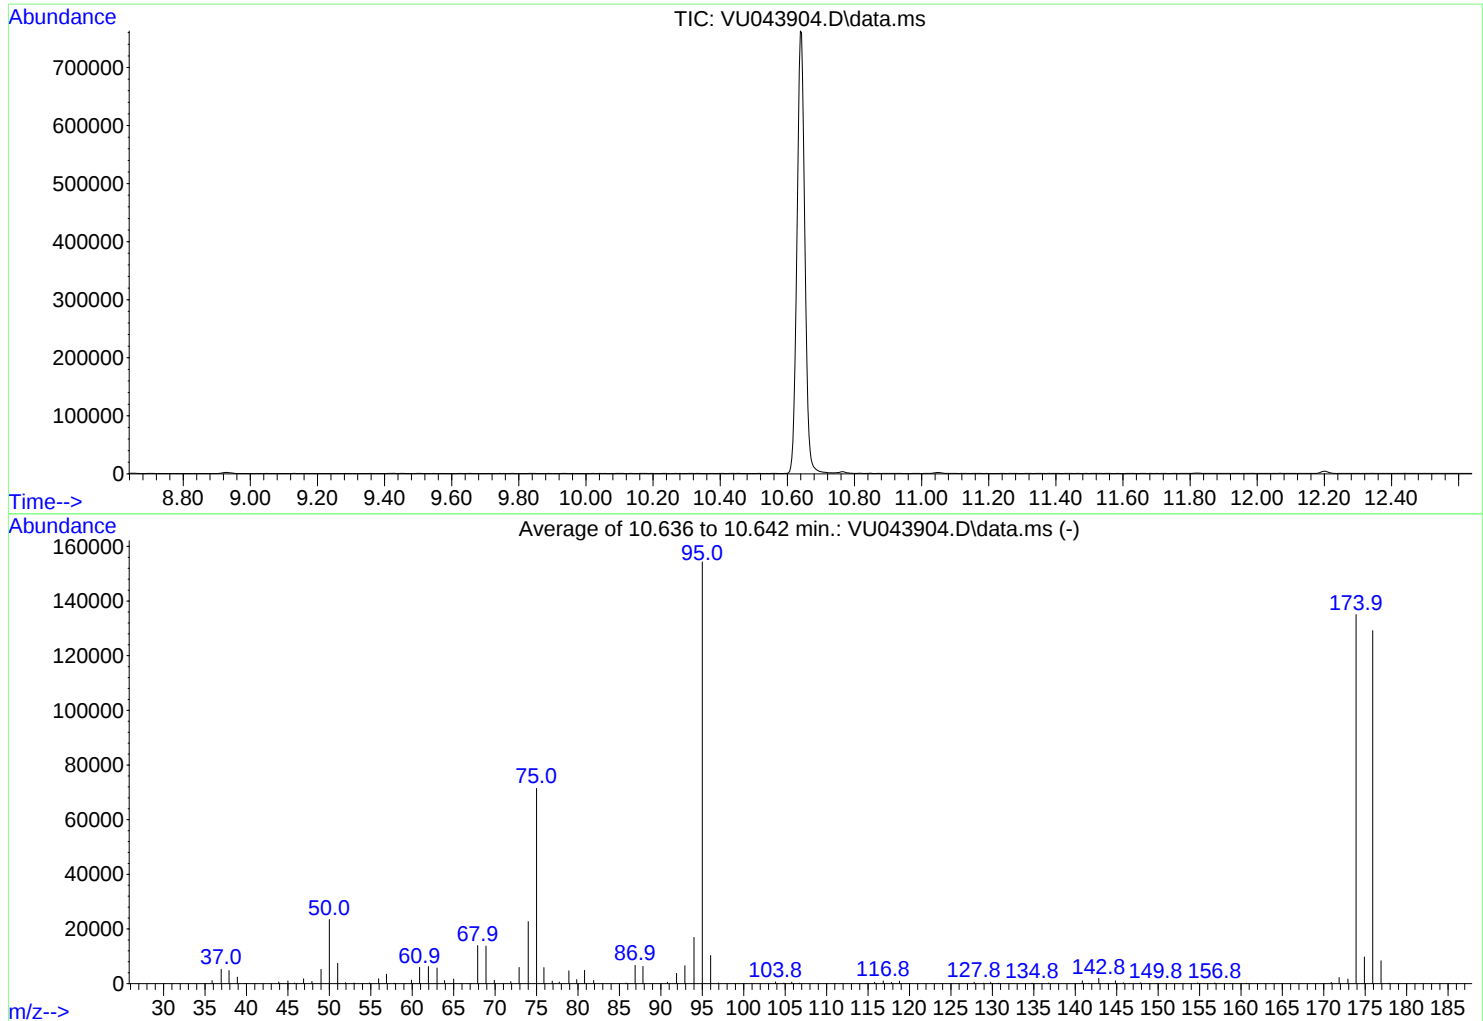

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	23459	PASS
75	95	30	80	46.3	71443	PASS
95	95	100	100	100.0	154347	PASS
96	95	5	9	6.7	10321	PASS
173	174	0.00	2	1.3	1704	PASS
174	95	50	120	87.5	135075	PASS
175	174	5	9	7.2	9759	PASS
176	174	95	101	95.6	129168	PASS
177	176	5	9	6.5	8380	PASS

m/z	Abundance
39.80	243.0
43.90	485.0

Instrument :
MSVOA_U
ClientSampleId :
BFB150

m/z	Abundance
35.80	1023.0
37.00	4926.0
37.90	4635.0
38.90	2251.0
39.80	342.0
42.90	111.0
43.90	1086.0
45.00	975.0
45.80	249.0
46.90	1708.0
47.90	771.0
49.00	4975.0
50.00	22312.0
51.00	7163.0
51.90	330.0
53.00	262.0
55.00	287.0
55.90	1842.0
56.90	3127.0
57.80	144.0
59.90	1227.0
60.90	5780.0
62.00	6256.0
63.00	5271.0
63.90	1128.0
65.00	1575.0
65.90	103.0
67.10	313.0
67.90	12989.0
68.90	13324.0
69.90	1280.0
71.90	754.0
72.90	5690.0
74.00	21544.0
75.00	68192.0
75.90	5775.0
76.90	950.0
77.80	474.0
78.90	4493.0
79.90	1408.0
80.80	4839.0
81.90	1131.0
85.80	230.0
86.90	6415.0
87.80	5777.0
90.80	497.0
91.90	3562.0
92.90	5907.0
94.00	16220.0
95.00	146112.0
96.00	9911.0
96.90	296.0
103.90	682.0
104.90	211.0
105.80	616.0
106.70	165.0
111.00	110.0
114.70	112.0
115.80	495.0
116.90	971.0
117.80	518.0
118.80	891.0
123.80	106.0
127.80	457.0
129.00	161.0
129.80	469.0
130.70	225.0
134.70	199.0
136.80	229.0
140.90	1022.0
141.60	149.0
142.90	1730.0
143.90	141.0
144.90	1078.0
145.80	334.0
146.60	127.0
147.90	342.0
149.70	133.0
154.90	271.0
156.80	289.0
158.80	115.0
160.60	152.0
170.90	466.0
171.80	2049.0
172.90	1578.0
173.90	124200.0
174.90	9144.0
175.90	119280.0
176.90	7810.0
177.80	195.0

Instrument :
MSVOA_U
ClientSampleId :
BFB150

m/z	Abundance
35.80	1157.0
37.00	5499.0
37.90	4965.0
38.90	2479.0
39.80	327.0
43.90	1050.0
45.00	1042.0
45.80	224.0
46.90	1844.0
47.90	873.0
49.00	5364.0
50.00	24216.0
51.00	7739.0
51.90	374.0
53.00	236.0
54.80	285.0
56.00	1858.0
56.90	3582.0
57.80	181.0
59.90	1328.0
60.90	6072.0
61.90	6378.0
63.00	5931.0
63.90	1124.0
65.00	1730.0
65.90	125.0
67.90	14440.0
68.90	14237.0
69.90	1273.0
71.90	811.0
72.90	6067.0
74.00	23456.0
75.00	73872.0
75.90	5993.0
76.90	981.0
77.80	581.0
78.90	4809.0
79.90	1524.0
80.80	5021.0
81.90	1216.0
82.90	119.0
85.80	279.0
86.90	6937.0
87.90	6468.0
90.80	559.0
91.90	3835.0
92.90	6808.0
94.00	17504.0
95.00	159424.0
96.00	10610.0
97.00	322.0
103.90	668.0
104.90	216.0
105.80	639.0
106.70	162.0
111.00	126.0
114.70	109.0
115.80	540.0
116.90	1028.0
117.90	514.0
118.80	946.0
123.80	109.0
127.80	530.0
129.00	187.0
129.80	534.0
130.80	196.0
134.80	201.0
136.80	284.0
140.90	1081.0
141.70	183.0
142.80	1952.0
143.90	122.0
144.80	1082.0
145.80	371.0
146.60	103.0
147.90	381.0
149.70	139.0
152.90	136.0
154.80	292.0
156.90	304.0
158.80	146.0
160.70	164.0
170.90	488.0
171.90	2315.0
172.90	1759.0
173.90	139584.0
174.90	9985.0
175.90	133248.0
176.90	8654.0
177.80	206.0

Instrument :
MSVOA_U
ClientSampleId :
BFB150

m/z	Abundance
35.90	1162.0
36.90	5447.0
37.90	4774.0
38.90	2468.0
39.80	299.0
43.90	1065.0
45.00	1011.0
45.80	197.0
46.10	228.0
46.90	1681.0
47.90	851.0
49.00	5297.0
50.00	23848.0
51.00	7457.0
52.00	350.0
53.00	184.0
54.80	311.0
55.90	1788.0
56.90	3616.0
57.90	190.0
59.90	1316.0
60.90	6012.0
62.00	6141.0
63.00	6033.0
63.90	1034.0
65.00	1745.0
65.90	134.0
66.70	252.0
67.90	14369.0
68.90	13789.0
69.90	1103.0
71.90	740.0
72.90	6037.0
74.00	23216.0
75.00	72264.0
75.90	5788.0
76.90	921.0
77.70	647.0
78.90	4790.0
79.80	1479.0
80.80	4768.0
81.90	1231.0
82.90	135.0
85.80	256.0
86.90	6767.0
87.90	6657.0
90.80	556.0
91.90	3890.0
92.90	6893.0
94.00	17048.0
95.00	157504.0
96.00	10441.0
96.90	301.0
103.80	632.0
104.80	204.0
105.80	575.0
106.80	155.0
111.80	102.0
114.80	135.0
115.80	531.0
116.80	1065.0
117.90	472.0
118.80	909.0
127.80	580.0
128.90	250.0
129.80	551.0
130.80	163.0
134.90	239.0
136.80	294.0
140.80	1031.0
141.70	194.0
142.80	2096.0
143.80	113.0
144.80	1050.0
145.80	325.0
147.80	350.0
148.90	118.0
149.80	107.0
152.90	157.0
154.70	318.0
156.90	300.0
158.70	164.0
160.70	144.0
170.90	403.0
171.90	2378.0
172.90	1776.0
173.90	141440.0
174.90	10147.0
175.90	134976.0
176.90	8677.0
177.90	198.0

Instrument :
MSVOA_U
ClientSampleId :
BFB150