




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058959.D
Acq On : 23 May 2024 19:33
Operator : MD/SY
Sample : P2566-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHR8

Manual IntegrationsAPPROVED

Quant Time: May 24 07:07:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 24 06:52:32 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/27/2024
Supervised By :Mahesh Dadoda 05/27/2024

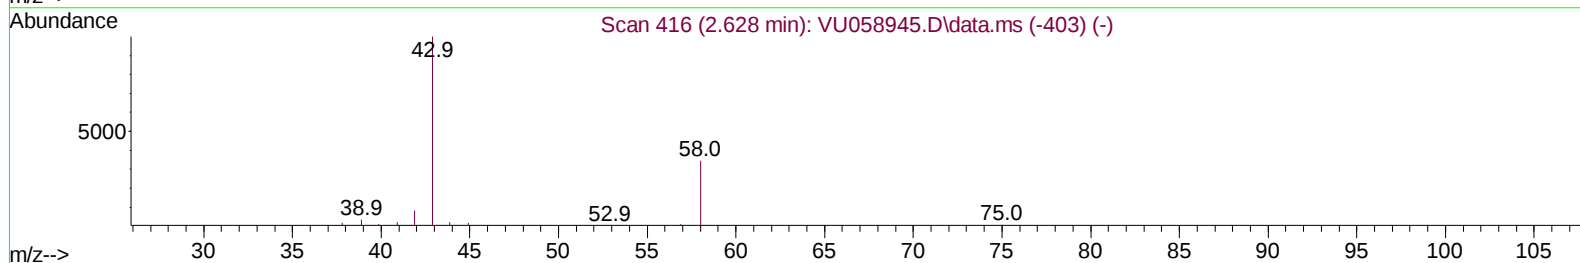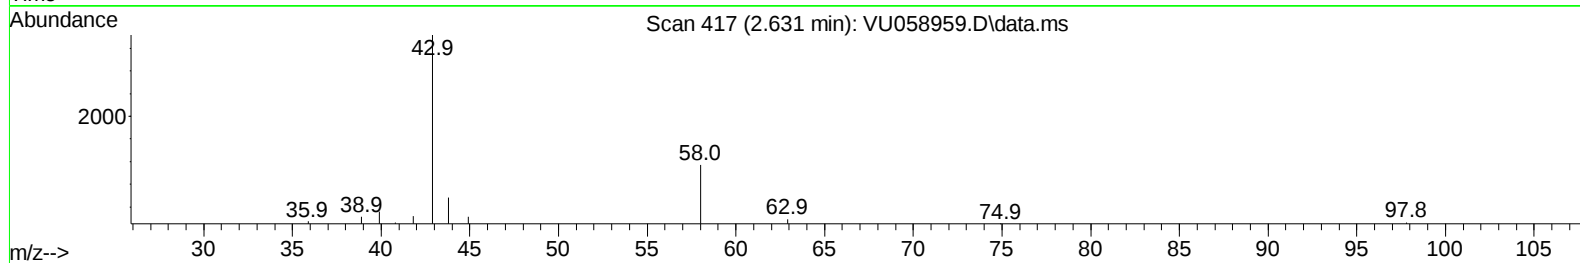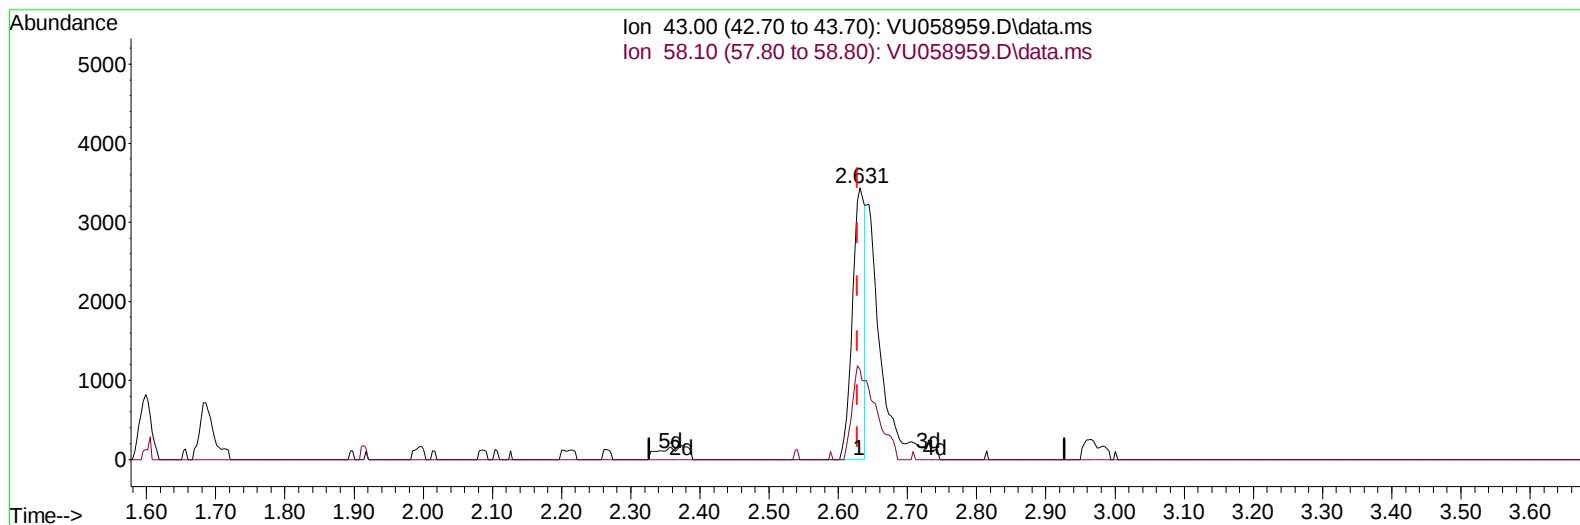

TIC: VU058959.D\data.ms

(13) Acetone (T)

2.631min (+ 0.003) 3.65 ug/L

response 4122

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	33.60	33.16
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058959.D
Acq On : 23 May 2024 19:33
Operator : MD/SY
Sample : P2566-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHR8

Manual IntegrationsAPPROVED

Quant Time: May 24 07:07:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 24 06:52:32 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/27/2024
Supervised By :Mahesh Dadoda 05/27/2024

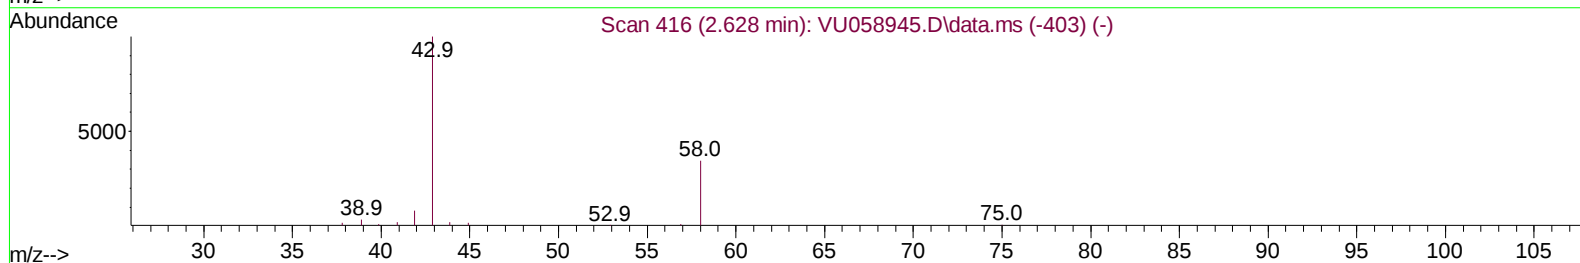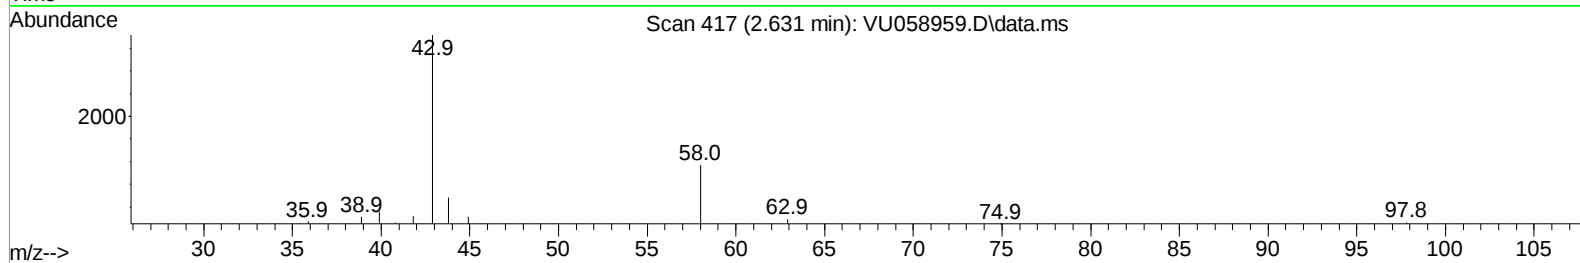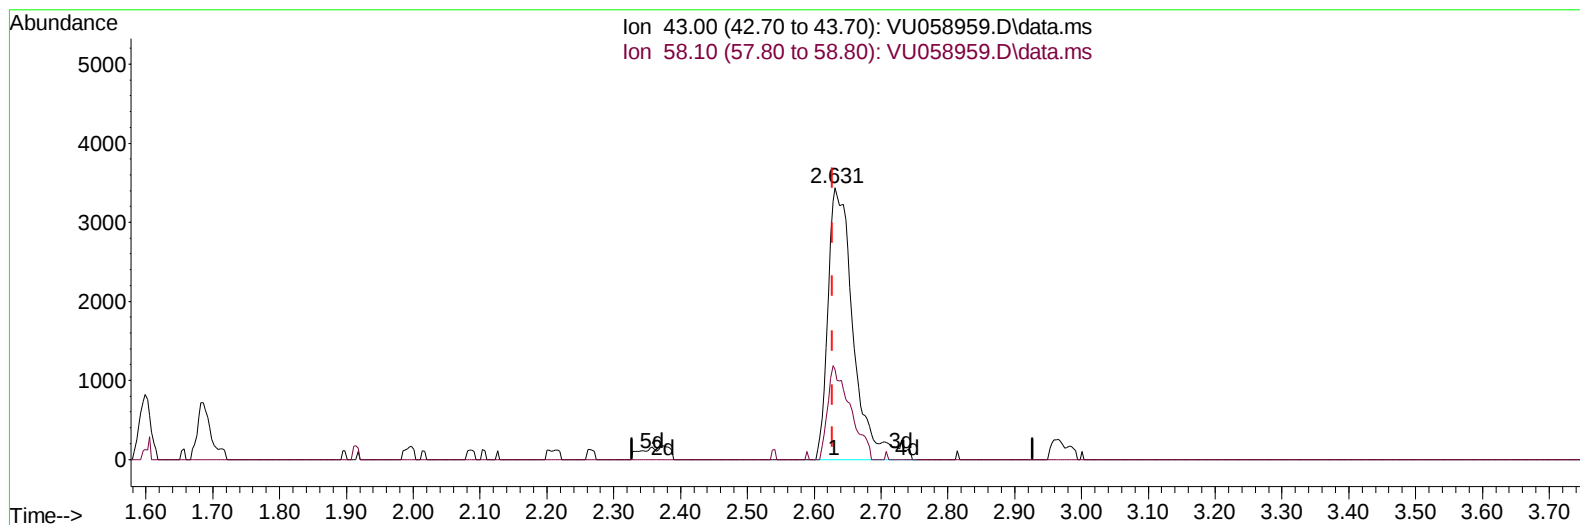

TIC: VU058959.D\data.ms

(13) Acetone (T)

2.631min (+ 0.003) 8.06 ug/L m

response 9094

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	33.60	15.03
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
 Data File : VU058959.D
 Acq On : 23 May 2024 19:33
 Operator : MD/SY
 Sample : P2566-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHR8

Manual IntegrationsAPPROVED

Quant Time: May 24 07:07:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 24 06:52:32 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/27/2024
 Supervised By :Mahesh Dadoda 05/27/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		176220	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		182251	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		80871	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		90136	48.362	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	96.720%	
7) Chloroethane-d5	1.911	69		73152	47.227	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	94.460%	
11) 1,1-Dichloroethene-d2	2.563	63		109247	38.366	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	76.740%	
21) 2-Butanone-d5	4.621	46		122600	95.764	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	95.760%	
24) Chloroform-d	5.055	84		154250	48.250	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	96.500%	
26) 1,2-Dichloroethane-d4	5.695	65		97890	50.069	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	100.140%	
32) Benzene-d6	5.721	84		308690	49.682	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	99.360%	
36) 1,2-Dichloropropane-d6	6.682	67		103158	50.266	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	100.540%	
41) Toluene-d8	7.894	98		261864	47.019	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	94.040%	
43) trans-1,3-Dichloroprop...	8.177	79		41721	45.275	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	90.540%	
47) 2-Hexanone-d5	8.627	63		79653	93.845	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	93.840%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		148996	48.259	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	96.520%	
66) 1,2-Dichlorobenzene-d4	12.187	152		90956	54.508	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	109.020%	
Target Compounds							
13) Acetone	2.631	43		9094m	8.057	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058959.D
Acq On : 23 May 2024 19:33
Operator : MD/SY
Sample : P2566-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHR8

Manual IntegrationsAPPROVED

Quant Time: May 24 07:07:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 24 06:52:32 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/27/2024
Supervised By :Mahesh Dadoda 05/27/2024

