

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
 Data File : VU058950.D
 Acq On : 23 May 2024 15:54
 Operator : MD/SY
 Sample : VU0524WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK050

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M

Title : VOC Analysis

Signal : TIC: VU058950.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	111	rVB	124845	144941	15.92%	2.191%
2	1.907	184	192	210	rVB	102361	134818	14.81%	2.038%
3	2.563	383	396	414	rBV	177144	294857	32.39%	4.457%
4	2.756	453	456	458	rBV2	314	196	0.02%	0.003%
5	2.792	458	467	472	rVV3	1272	1827	0.20%	0.028%
6	2.923	504	508	511	rVB2	333	217	0.02%	0.003%
7	2.946	511	515	517	rBV2	250	178	0.02%	0.003%
8	3.039	535	544	558	rVB4	6324	12028	1.32%	0.182%
9	3.177	582	587	590	rBV2	489	513	0.06%	0.008%
10	3.358	634	643	653	rBV4	827	1493	0.16%	0.023%
11	3.650	730	734	737	rVB2	231	177	0.02%	0.003%
12	3.827	785	789	792	rBV2	250	185	0.02%	0.003%
13	3.882	800	806	811	rBV2	433	530	0.06%	0.008%
14	3.946	820	826	829	rVV2	354	359	0.04%	0.005%
15	3.988	835	839	843	rBV2	219	219	0.02%	0.003%
16	4.049	853	858	861	rBV2	236	249	0.03%	0.004%
17	4.361	951	955	961	rBV	247	236	0.03%	0.004%
18	4.454	977	984	990	rBV2	253	302	0.03%	0.005%
19	4.554	1009	1015	1018	rBV2	215	202	0.02%	0.003%
20	4.615	1025	1034	1071	rBV	83859	225605	24.78%	3.410%
21	4.968	1140	1144	1147	rVB3	251	234	0.03%	0.004%
22	5.055	1155	1171	1193	rBV	161084	358025	39.33%	5.412%
23	5.232	1223	1226	1230	rVB2	353	259	0.03%	0.004%
24	5.267	1233	1237	1240	rBV2	422	304	0.03%	0.005%
25	5.628	1346	1349	1354	rVB2	229	182	0.02%	0.003%
26	5.718	1357	1377	1413	rBV2	332329	910368	100.00%	13.761%
27	5.923	1439	1441	1446	rVB3	356	229	0.03%	0.003%
28	6.020	1466	1471	1472	rBV	212	187	0.02%	0.003%
29	6.116	1493	1501	1502	rBV2	283	289	0.03%	0.004%
30	6.181	1516	1521	1527	rVB2	340	352	0.04%	0.005%
31	6.242	1527	1540	1565	rBV	219652	429794	47.21%	6.497%
32	6.409	1588	1592	1594	rBV2	321	260	0.03%	0.004%
33	6.451	1601	1605	1607	rBV2	252	176	0.02%	0.003%
34	6.467	1607	1610	1615	rVB3	367	279	0.03%	0.004%
35	6.531	1618	1630	1641	rBV10	4749	9691	1.06%	0.146%
36	6.682	1662	1677	1704	rBV	209417	413632	45.44%	6.252%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
 Data File : VU058950.D
 Acq On : 23 May 2024 15:54
 Operator : MD/SY
 Sample : VU0524WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK050

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

37	6.846	1726	1728	1731	rVB2	341	181	0.02%	0.003%
38	6.885	1733	1740	1746	rVB2	163	190	0.02%	0.003%
39	7.171	1825	1829	1832	rVB2	349	233	0.03%	0.004%
40	7.190	1832	1835	1838	rBV	278	273	0.03%	0.004%
41	7.216	1838	1843	1845	rVV2	338	348	0.04%	0.005%
42	7.377	1887	1893	1895	rVB2	215	198	0.02%	0.003%
43	7.457	1912	1918	1922	rBV2	269	303	0.03%	0.005%
44	7.560	1936	1950	1975	rBV	107941	197523	21.70%	2.986%
45	7.891	2038	2053	2073	rBV	390141	686771	75.44%	10.381%
46	8.097	2114	2117	2122	rVB2	380	275	0.03%	0.004%
47	8.174	2131	2141	2161	rBV2	75416	134193	14.74%	2.028%
48	8.428	2215	2220	2224	rVB2	229	196	0.02%	0.003%
49	8.470	2227	2233	2238	rVB2	555	620	0.07%	0.009%
50	8.502	2238	2243	2246	rBV	267	250	0.03%	0.004%
51	8.553	2252	2259	2263	rVB4	1072	989	0.11%	0.015%
52	8.627	2272	2282	2315	rBV	240648	464881	51.07%	7.027%
53	8.885	2359	2362	2366	rBV2	334	266	0.03%	0.004%
54	9.036	2405	2409	2413	rBV2	364	322	0.04%	0.005%
55	9.084	2419	2424	2428	rBV2	341	336	0.04%	0.005%
56	9.171	2447	2451	2456	rVB2	387	340	0.04%	0.005%
57	9.203	2456	2461	2463	rBV2	248	232	0.03%	0.004%
58	9.225	2464	2468	2473	rVB2	314	292	0.03%	0.004%
59	9.412	2513	2526	2564	rBV	340317	572152	62.85%	8.648%
60	9.541	2564	2566	2569	rBV2	450	238	0.03%	0.004%
61	9.688	2607	2612	2614	rBV	527	402	0.04%	0.006%
62	9.936	2682	2689	2691	rBV	263	291	0.03%	0.004%
63	10.123	2742	2747	2751	rBV3	452	555	0.06%	0.008%
64	10.184	2762	2766	2769	rBV2	334	340	0.04%	0.005%
65	10.290	2795	2799	2803	rBV2	198	176	0.02%	0.003%
66	10.483	2854	2859	2865	rVB2	547	686	0.08%	0.010%
67	10.534	2870	2875	2878	rBV2	338	312	0.03%	0.005%
68	10.566	2881	2885	2889	rBV	310	239	0.03%	0.004%
69	10.749	2929	2942	2959	rBV	291501	473178	51.98%	7.152%
70	11.212	3081	3086	3088	rBV2	331	280	0.03%	0.004%
71	11.270	3101	3104	3107	rBV2	302	207	0.02%	0.003%
72	11.663	3220	3226	3229	rBV2	342	392	0.04%	0.006%
73	11.749	3246	3253	3258	rBV2	1665	2154	0.24%	0.033%
74	11.807	3259	3271	3300	rVV	312015	527709	57.97%	7.977%
75	12.087	3352	3358	3362	rBV2	287	402	0.04%	0.006%
76	12.187	3377	3389	3408	rBV	359512	591945	65.02%	8.948%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
 Data File : VU058950.D
 Acq On : 23 May 2024 15:54
 Operator : MD/SY
 Sample : VU0524WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK050

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

77	12.312	3426	3428	3437	rVB3	515	556	0.06%	0.008%
78	12.347	3437	3439	3443	rVB2	386	226	0.02%	0.003%
79	12.370	3443	3446	3450	rBV2	238	190	0.02%	0.003%
80	12.393	3450	3453	3455	rBV2	311	175	0.02%	0.003%
81	12.473	3475	3478	3482	rVB2	242	187	0.02%	0.003%
82	12.756	3562	3566	3568	rBV2	395	337	0.04%	0.005%
83	12.878	3601	3604	3606	rBV2	250	176	0.02%	0.003%
84	13.026	3645	3650	3652	rBV2	368	337	0.04%	0.005%
85	13.228	3707	3713	3715	rBV3	1057	976	0.11%	0.015%
86	13.351	3749	3751	3757	rVB2	291	228	0.03%	0.003%
87	13.528	3803	3806	3809	rBV2	368	326	0.04%	0.005%
88	13.782	3882	3885	3888	rBV	367	245	0.03%	0.004%
89	13.855	3903	3908	3916	rBV5	1449	1704	0.19%	0.026%
90	13.917	3924	3927	3932	rBV2	379	387	0.04%	0.006%
91	14.335	4051	4057	4060	rBV4	1019	1211	0.13%	0.018%
92	14.376	4067	4070	4072	rBV	386	266	0.03%	0.004%
93	14.409	4078	4080	4085	rBV2	378	260	0.03%	0.004%
94	14.727	4175	4179	4185	rBV	625	767	0.08%	0.012%
95	15.071	4284	4286	4288	rBV2	435	289	0.03%	0.004%
96	15.273	4346	4349	4356	rBV3	500	599	0.07%	0.009%
97	15.466	4406	4409	4415	rBV2	401	397	0.04%	0.006%
98	16.244	4648	4651	4652	rBV2	712	443	0.05%	0.007%
99	16.405	4697	4701	4705	rVB5	950	808	0.09%	0.012%
100	16.425	4705	4707	4708	rBV	608	301	0.03%	0.005%




Sum of corrected areas: 6615654

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058950.D
Acq On : 23 May 2024 15:54
Operator : MD/SY
Sample : VU0524WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK050

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

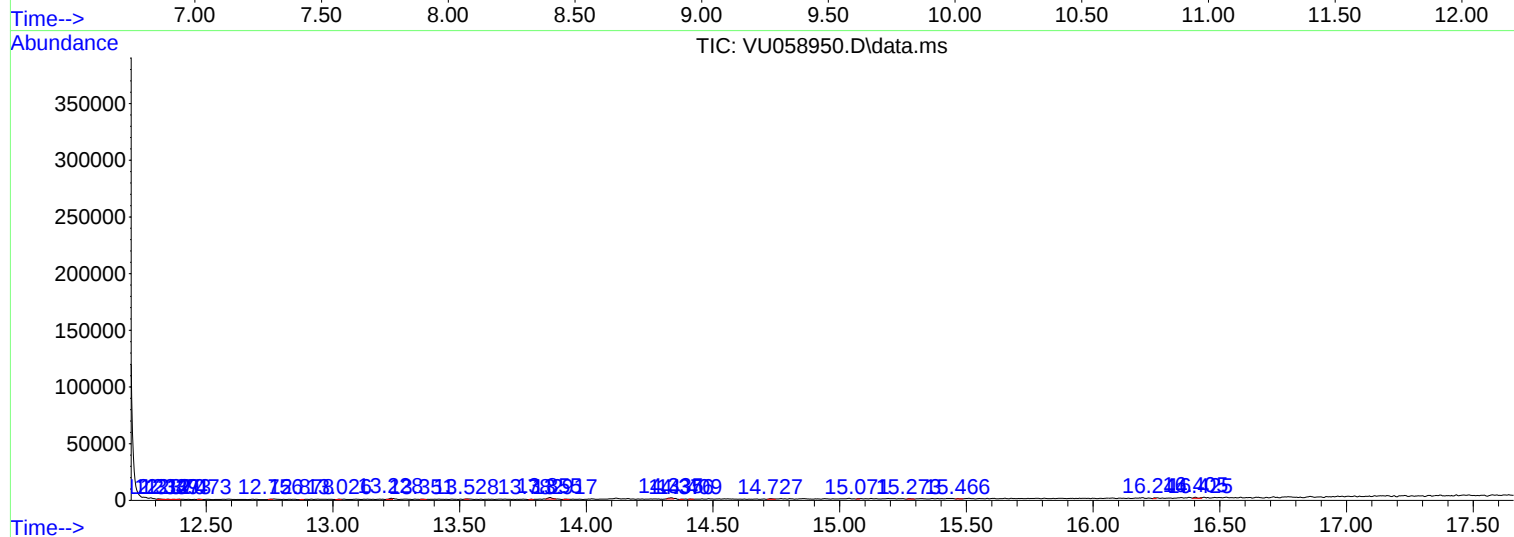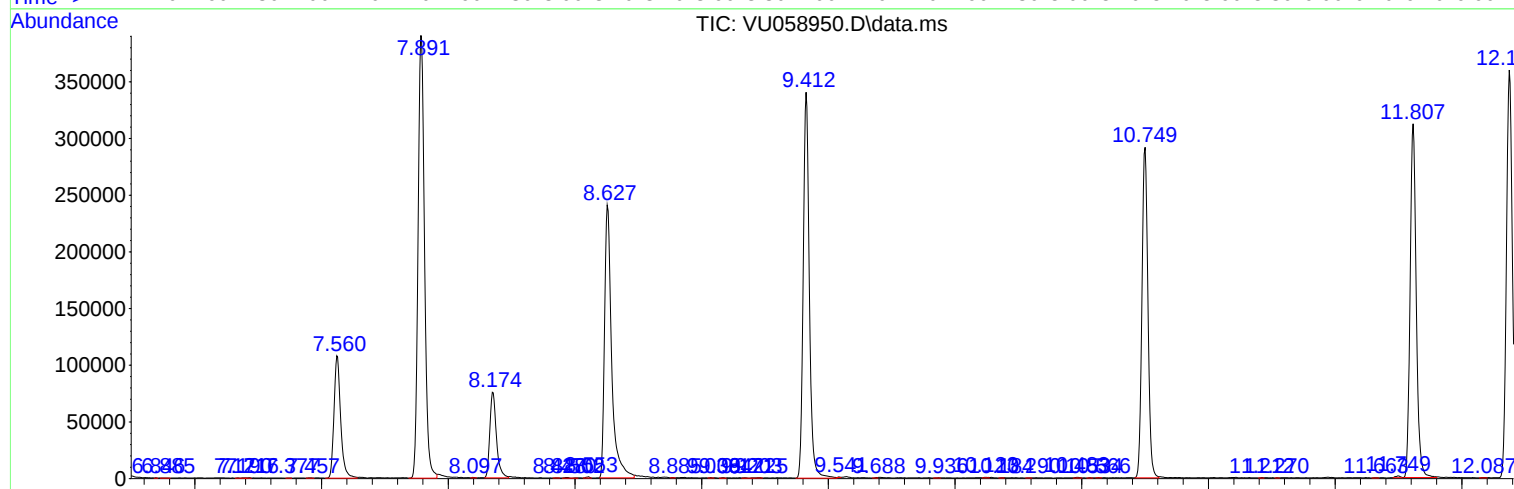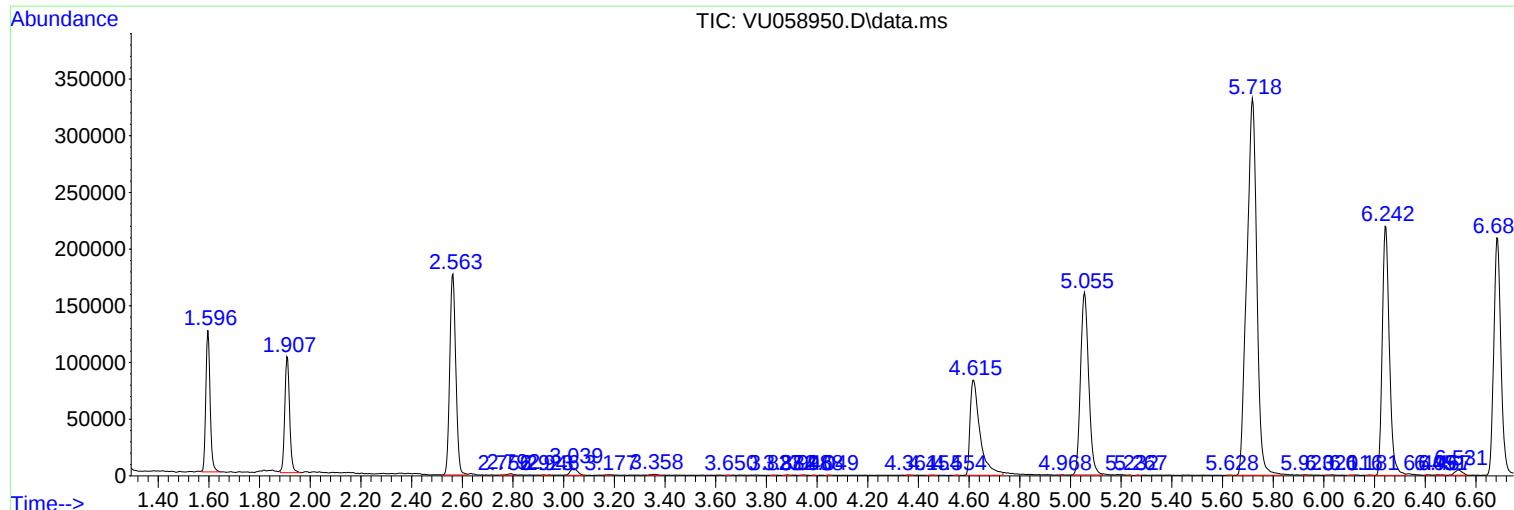

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058950.D
Acq On : 23 May 2024 15:54
Operator : MD/SY
Sample : VU0524WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK050

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058950.D
Acq On : 23 May 2024 15:54
Operator : MD/SY
Sample : VU0524WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK050

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc