

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
 Data File : VU058966.D
 Acq On : 24 May 2024 13:18
 Operator : MD/SY
 Sample : VU0524WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M

Title : VOC Analysis

Signal : TIC: VU058966.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	116	rVB	109638	131483	15.06%	2.144%
2	1.910	185	193	205	rBV	101411	128163	14.68%	2.090%
3	2.563	383	396	416	rBV	162079	267026	30.58%	4.354%
4	2.637	416	419	420	rBV2	468	273	0.03%	0.004%
5	2.785	458	465	467	rBV3	812	808	0.09%	0.013%
6	2.917	503	506	511	rBV2	204	189	0.02%	0.003%
7	3.042	534	545	554	rVV2	3977	6804	0.78%	0.111%
8	3.181	580	588	596	rVB4	822	1583	0.18%	0.026%
9	3.287	617	621	625	rVB2	191	180	0.02%	0.003%
10	3.348	637	640	646	rVV	206	195	0.02%	0.003%
11	3.467	672	677	680	rBV2	204	221	0.03%	0.004%
12	3.608	717	721	724	rBV2	249	193	0.02%	0.003%
13	3.627	725	727	731	rVB	305	174	0.02%	0.003%
14	3.669	737	740	743	rVB	259	173	0.02%	0.003%
15	3.698	743	749	751	rBV2	215	216	0.02%	0.004%
16	3.727	754	758	763	rVB2	189	188	0.02%	0.003%
17	3.756	763	767	773	rBV2	249	251	0.03%	0.004%
18	4.335	944	947	949	rBV2	231	174	0.02%	0.003%
19	4.393	959	965	971	rBV2	168	179	0.02%	0.003%
20	4.454	980	984	989	rBV2	320	361	0.04%	0.006%
21	4.621	1026	1036	1066	rBV	81263	227345	26.04%	3.707%
22	5.055	1156	1171	1196	rBV	155024	344587	39.47%	5.618%
23	5.216	1217	1221	1228	rVB4	447	541	0.06%	0.009%
24	5.377	1268	1271	1278	rVB2	207	235	0.03%	0.004%
25	5.422	1278	1285	1288	rBV3	362	389	0.04%	0.006%
26	5.473	1298	1301	1306	rVV2	183	234	0.03%	0.004%
27	5.717	1357	1377	1404	rBV2	323813	873086	100.00%	14.235%
28	5.920	1437	1440	1444	rVB4	336	199	0.02%	0.003%
29	5.997	1459	1464	1471	rVB3	366	549	0.06%	0.009%
30	6.026	1471	1473	1478	rBV2	386	314	0.04%	0.005%
31	6.129	1500	1505	1507	rBV	240	183	0.02%	0.003%
32	6.245	1529	1541	1566	rBV	206018	402864	46.14%	6.569%
33	6.438	1599	1601	1606	rVB3	299	262	0.03%	0.004%
34	6.479	1609	1614	1621	rVB2	373	534	0.06%	0.009%
35	6.534	1621	1631	1645	rBV6	7255	14584	1.67%	0.238%
36	6.618	1649	1657	1659	rBV2	198	240	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
 Data File : VU058966.D
 Acq On : 24 May 2024 13:18
 Operator : MD/SY
 Sample : VU0524WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

37	6.685	1664	1678	1700	rBV	202793	404234	46.30%	6.591%
38	6.791	1707	1711	1713	rBV4	502	347	0.04%	0.006%
39	6.856	1727	1731	1735	rVB2	193	173	0.02%	0.003%
40	6.959	1756	1763	1766	rBV	262	282	0.03%	0.005%
41	6.978	1766	1769	1775	rVV2	219	227	0.03%	0.004%
42	7.032	1783	1786	1793	rVB2	274	265	0.03%	0.004%
43	7.081	1793	1801	1802	rBV2	182	237	0.03%	0.004%
44	7.126	1810	1815	1819	rVB2	250	256	0.03%	0.004%
45	7.155	1819	1824	1831	rVB2	226	199	0.02%	0.003%
46	7.196	1833	1837	1840	rBV2	385	279	0.03%	0.005%
47	7.412	1901	1904	1909	rVB2	318	246	0.03%	0.004%
48	7.463	1918	1920	1924	rVV	201	182	0.02%	0.003%
49	7.560	1939	1950	1967	rBV	97797	178410	20.43%	2.909%
50	7.653	1977	1979	1982	rVB	532	240	0.03%	0.004%
51	7.672	1982	1985	1989	rVB2	412	320	0.04%	0.005%
52	7.894	2041	2054	2078	rBV	358779	627668	71.89%	10.234%
53	8.174	2131	2141	2159	rVV2	66642	119505	13.69%	1.948%
54	8.630	2272	2283	2318	rBV	229935	463772	53.12%	7.562%
55	8.852	2348	2352	2356	rVB2	305	240	0.03%	0.004%
56	8.942	2377	2380	2386	rVB3	342	279	0.03%	0.005%
57	9.010	2398	2401	2409	rVB2	152	184	0.02%	0.003%
58	9.055	2413	2415	2420	rVB	421	355	0.04%	0.006%
59	9.412	2514	2526	2563	rBV	304414	522973	59.90%	8.527%
60	9.563	2570	2573	2576	rBV2	336	219	0.03%	0.004%
61	9.692	2609	2613	2616	rBV2	328	295	0.03%	0.005%
62	9.839	2655	2659	2665	rVB2	357	295	0.03%	0.005%
63	10.232	2777	2781	2783	rBV2	351	248	0.03%	0.004%
64	10.637	2904	2907	2912	rVB2	278	246	0.03%	0.004%
65	10.679	2917	2920	2926	rBV2	263	253	0.03%	0.004%
66	10.749	2927	2942	2960	rBV	288002	463888	53.13%	7.564%
67	10.888	2982	2985	2990	rBV2	450	354	0.04%	0.006%
68	10.952	3000	3005	3010	rBV	236	320	0.04%	0.005%
69	11.068	3038	3041	3045	rBV2	295	238	0.03%	0.004%
70	11.097	3045	3050	3053	rVV2	276	268	0.03%	0.004%
71	11.116	3053	3056	3060	rVB2	277	196	0.02%	0.003%
72	11.167	3068	3072	3077	rBV2	294	294	0.03%	0.005%
73	11.254	3095	3099	3100	rBV	286	180	0.02%	0.003%
74	11.531	3181	3185	3189	rBV2	200	202	0.02%	0.003%
75	11.746	3249	3252	3257	rBV	330	347	0.04%	0.006%
76	11.807	3257	3271	3293	rBV	255931	424352	48.60%	6.919%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
 Data File : VU058966.D
 Acq On : 24 May 2024 13:18
 Operator : MD/SY
 Sample : VU0524WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

77	11.939	3309	3312	3313	rBV3	371	219	0.03%	0.004%
78	12.048	3342	3346	3349	rBV3	303	242	0.03%	0.004%
79	12.187	3377	3389	3413	rBV	295642	508193	58.21%	8.286%
80	12.341	3434	3437	3441	rVB2	525	325	0.04%	0.005%
81	12.360	3441	3443	3445	rVB2	394	189	0.02%	0.003%
82	12.553	3500	3503	3506	rBV	415	297	0.03%	0.005%
83	12.585	3510	3513	3516	rVB2	352	255	0.03%	0.004%
84	13.154	3687	3690	3693	rBV2	289	199	0.02%	0.003%
85	13.379	3757	3760	3764	rBV2	271	186	0.02%	0.003%
86	13.402	3764	3767	3777	rBV2	327	453	0.05%	0.007%
87	13.444	3777	3780	3784	rVV2	201	180	0.02%	0.003%
88	13.466	3785	3787	3793	rVB	310	245	0.03%	0.004%
89	13.611	3828	3832	3836	rBV2	374	423	0.05%	0.007%
90	13.656	3841	3846	3848	rBV2	232	242	0.03%	0.004%
91	13.759	3876	3878	3883	rVB2	388	255	0.03%	0.004%
92	13.978	3943	3946	3950	rBV	262	196	0.02%	0.003%
93	14.273	4034	4038	4042	rBV2	357	374	0.04%	0.006%
94	14.434	4085	4088	4090	rBV2	284	188	0.02%	0.003%
95	14.505	4108	4110	4116	rBV	218	186	0.02%	0.003%
96	14.537	4116	4120	4124	rBV3	496	425	0.05%	0.007%
97	14.656	4151	4157	4161	rBV2	397	619	0.07%	0.010%
98	14.949	4244	4248	4250	rBV2	499	388	0.04%	0.006%
99	14.981	4255	4258	4261	rBV	398	324	0.04%	0.005%
100	15.051	4275	4280	4283	rBV2	483	531	0.06%	0.009%




Sum of corrected areas: 6133182

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058966.D
Acq On : 24 May 2024 13:18
Operator : MD/SY
Sample : VU0524WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

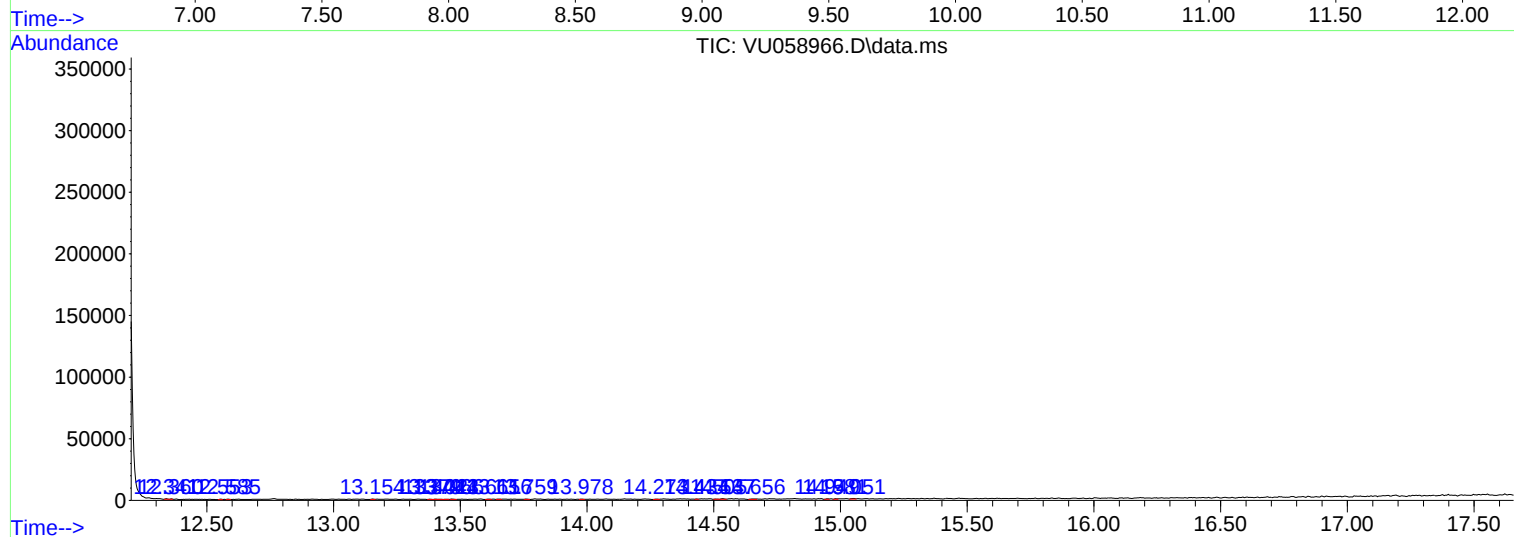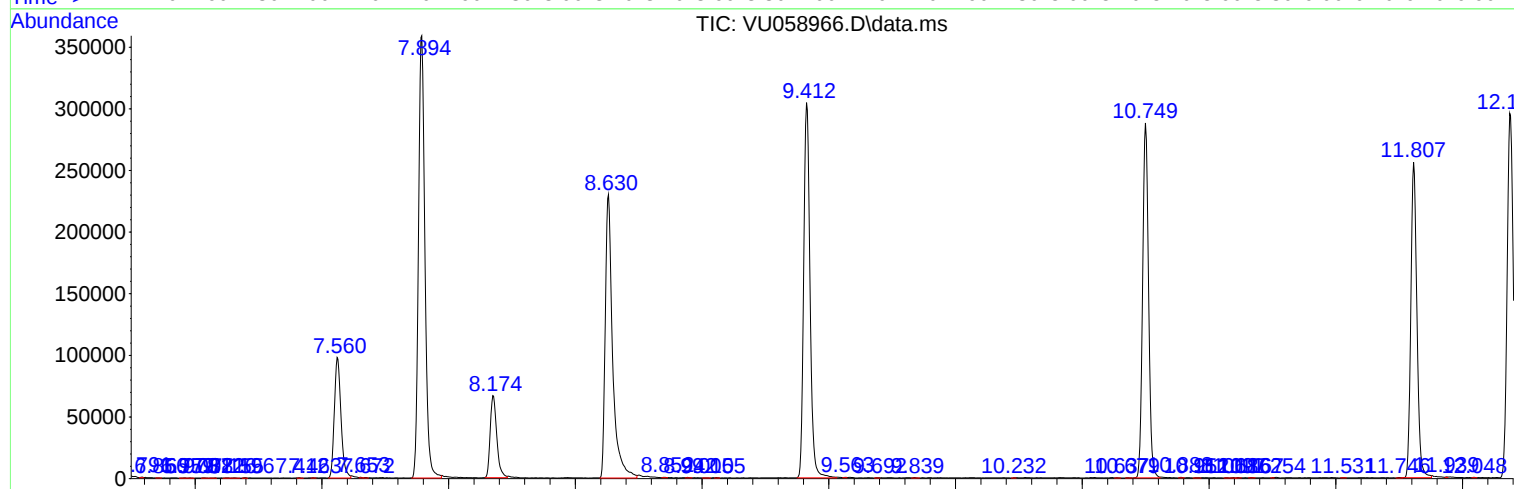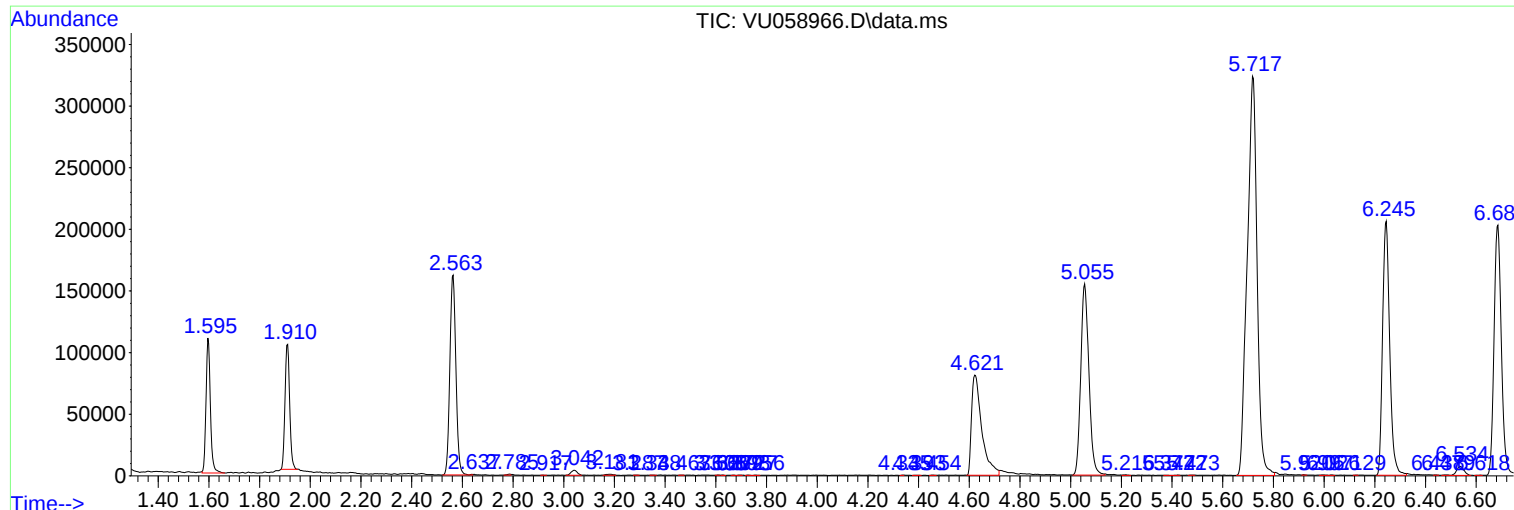

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058966.D
Acq On : 24 May 2024 13:18
Operator : MD/SY
Sample : VU0524WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058966.D
Acq On : 24 May 2024 13:18
Operator : MD/SY
Sample : VU0524WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------