

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
 Data File : VU058969.D
 Acq On : 24 May 2024 14:30
 Operator : MD/SY
 Sample : P2566-03DL 4000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHS7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M

Title : VOC Analysis

Signal : TIC: VU058969.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	118	rVB	114707	145943	14.84%	1.967%
2	1.907	185	192	206	rBV	117481	176761	17.98%	2.382%
3	2.557	382	394	411	rBV	186290	307382	31.26%	4.142%
4	2.782	458	464	472	rVB2	910	1441	0.15%	0.019%
5	2.997	528	531	534	rBV3	253	183	0.02%	0.002%
6	3.033	534	542	553	rVV4	3742	7279	0.74%	0.098%
7	3.078	553	556	559	rVB2	227	138	0.01%	0.002%
8	3.107	559	565	573	rBV2	314	538	0.05%	0.007%
9	3.177	573	587	609	rVV	9269	23044	2.34%	0.311%
10	3.293	621	623	626	rBV	263	159	0.02%	0.002%
11	3.358	640	643	644	rBV	167	84	0.01%	0.001%
12	3.467	674	677	678	rBV	128	74	0.01%	0.001%
13	3.525	692	695	700	rBV	164	105	0.01%	0.001%
14	3.583	710	713	716	rBV	260	182	0.02%	0.002%
15	3.618	720	724	727	rBV2	167	123	0.01%	0.002%
16	3.637	727	730	732	rBV2	150	113	0.01%	0.002%
17	3.714	750	754	756	rBV2	182	124	0.01%	0.002%
18	3.750	763	765	768	rVB2	166	80	0.01%	0.001%
19	3.769	768	771	774	rVB	161	91	0.01%	0.001%
20	3.788	775	777	783	rVB2	211	173	0.02%	0.002%
21	3.824	783	788	795	rBV	450	489	0.05%	0.007%
22	3.849	795	796	797	rVV	201	39	0.00%	0.001%
23	3.862	797	800	803	rVV	148	98	0.01%	0.001%
24	3.907	807	814	821	rBV2	274	377	0.04%	0.005%
25	3.936	821	823	826	rBV2	108	50	0.01%	0.001%
26	4.091	866	871	875	rBV2	311	276	0.03%	0.004%
27	4.155	887	891	895	rBV2	228	232	0.02%	0.003%
28	4.193	900	903	907	rVB2	219	148	0.02%	0.002%
29	4.216	907	910	913	rBV	172	149	0.02%	0.002%
30	4.312	938	940	942	rBV	140	86	0.01%	0.001%
31	4.354	951	953	955	rBV	106	53	0.01%	0.001%
32	4.396	964	966	969	rVB	186	100	0.01%	0.001%
33	4.419	969	973	975	rBV2	179	124	0.01%	0.002%
34	4.435	975	978	982	rBV	152	155	0.02%	0.002%
35	4.489	991	995	998	rBV	247	191	0.02%	0.003%
36	4.628	1027	1038	1073	rBV2	79845	242809	24.69%	3.272%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
 Data File : VU058969.D
 Acq On : 24 May 2024 14:30
 Operator : MD/SY
 Sample : P2566-03DL 4000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHS7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

37	4.997	1149	1153	1154	rBV2	268	178	0.02%	0.002%
38	5.052	1155	1170	1193	rVV	173122	383959	39.05%	5.174%
39	5.210	1216	1219	1221	rVB3	446	241	0.02%	0.003%
40	5.280	1239	1241	1242	rVB	119	45	0.00%	0.001%
41	5.303	1245	1248	1249	rBV	81	40	0.00%	0.001%
42	5.345	1257	1261	1264	rBV2	290	197	0.02%	0.003%
43	5.383	1271	1273	1275	rVB2	190	80	0.01%	0.001%
44	5.492	1305	1307	1309	rBV2	172	88	0.01%	0.001%
45	5.595	1336	1339	1346	rBV2	315	342	0.03%	0.005%
46	5.621	1346	1347	1349	rBV2	111	48	0.00%	0.001%
47	5.634	1349	1351	1354	rVB2	159	80	0.01%	0.001%
48	5.650	1354	1356	1357	rBV	107	51	0.01%	0.001%
49	5.714	1357	1376	1409	rBV2	361902	983290	100.00%	13.251%
50	6.004	1463	1466	1468	rBV	199	116	0.01%	0.002%
51	6.039	1476	1477	1478	rBV	251	93	0.01%	0.001%
52	6.119	1498	1502	1504	rBV	249	201	0.02%	0.003%
53	6.242	1527	1540	1568	rBV	238212	465877	47.38%	6.278%
54	6.489	1614	1617	1619	rBB2	282	142	0.01%	0.002%
55	6.534	1619	1631	1653	rBV2	286325	552887	56.23%	7.451%
56	6.682	1664	1677	1701	rBV	228284	446951	45.45%	6.023%
57	6.904	1743	1746	1749	rBV	147	92	0.01%	0.001%
58	6.920	1749	1751	1755	rBV2	242	187	0.02%	0.003%
59	7.004	1773	1777	1780	rBV2	192	173	0.02%	0.002%
60	7.033	1783	1786	1791	rVB2	199	150	0.02%	0.002%
61	7.055	1791	1793	1797	rBV2	144	88	0.01%	0.001%
62	7.078	1797	1800	1803	rBV	115	83	0.01%	0.001%
63	7.119	1807	1813	1815	rBV	192	198	0.02%	0.003%
64	7.152	1820	1823	1824	rBV2	143	92	0.01%	0.001%
65	7.232	1844	1848	1851	rBV4	472	375	0.04%	0.005%
66	7.351	1881	1885	1886	rBV	210	147	0.01%	0.002%
67	7.447	1912	1915	1918	rBV	159	97	0.01%	0.001%
68	7.560	1938	1950	1975	rBV	113188	205526	20.90%	2.770%
69	7.891	2041	2053	2079	rBV	402735	716345	72.85%	9.654%
70	8.174	2131	2141	2158	rBV	74641	133417	13.57%	1.798%
71	8.296	2176	2179	2183	rVB2	140	108	0.01%	0.001%
72	8.325	2186	2188	2190	rVB	141	58	0.01%	0.001%
73	8.344	2191	2194	2195	rBV	257	143	0.01%	0.002%
74	8.393	2206	2209	2213	rVB2	269	187	0.02%	0.003%
75	8.467	2226	2232	2237	rBV	540	707	0.07%	0.010%
76	8.547	2254	2257	2263	rBV2	529	422	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
 Data File : VU058969.D
 Acq On : 24 May 2024 14:30
 Operator : MD/SY
 Sample : P2566-03DL 4000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHS7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

77	8.634	2272	2284	2320	rBV	236400	508015	51.66%	6.846%
78	8.939	2376	2379	2381	rBV2	373	202	0.02%	0.003%
79	9.004	2393	2399	2402	rBV3	483	490	0.05%	0.007%
80	9.242	2468	2473	2481	rVB2	332	426	0.04%	0.006%
81	9.412	2513	2526	2553	rBV	334643	576394	58.62%	7.768%
82	9.640	2594	2597	2599	rBV2	194	141	0.01%	0.002%
83	9.946	2689	2692	2695	rVB	245	148	0.02%	0.002%
84	9.962	2695	2697	2699	rBV	158	92	0.01%	0.001%
85	9.997	2706	2708	2711	rBV	215	130	0.01%	0.002%
86	10.097	2736	2739	2743	rBV3	407	398	0.04%	0.005%
87	10.270	2790	2793	2795	rBV	188	143	0.01%	0.002%
88	10.749	2929	2942	2963	rBV	314355	512101	52.08%	6.901%
89	10.859	2974	2976	2979	rBV2	388	254	0.03%	0.003%
90	11.023	3025	3027	3029	rBV	188	97	0.01%	0.001%
91	11.129	3059	3060	3062	rBV	225	84	0.01%	0.001%
92	11.209	3082	3085	3091	rBV2	342	445	0.05%	0.006%
93	11.383	3136	3139	3140	rBV	348	218	0.02%	0.003%
94	11.428	3149	3153	3158	rBV2	437	478	0.05%	0.006%
95	11.743	3248	3251	3254	rBV2	304	272	0.03%	0.004%
96	11.807	3259	3271	3290	rBV	290944	469617	47.76%	6.329%
97	12.187	3378	3389	3417	rBV	323094	547376	55.67%	7.377%




Sum of corrected areas: 7420415

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058969.D
Acq On : 24 May 2024 14:30
Operator : MD/SY
Sample : P2566-03DL 4000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

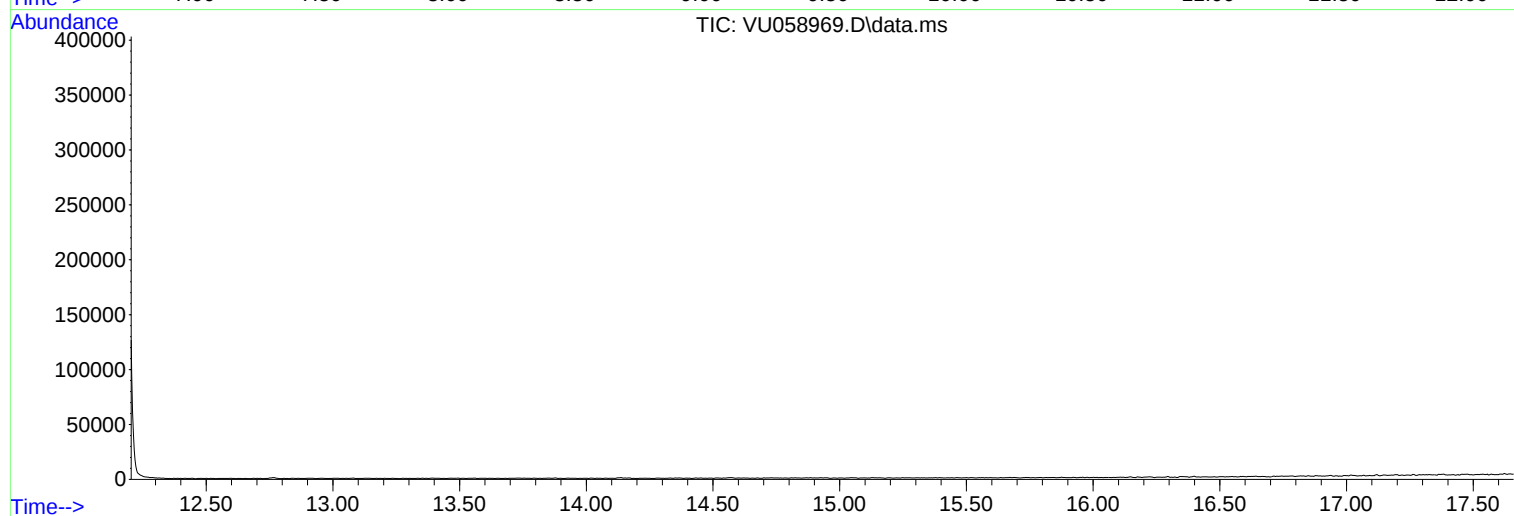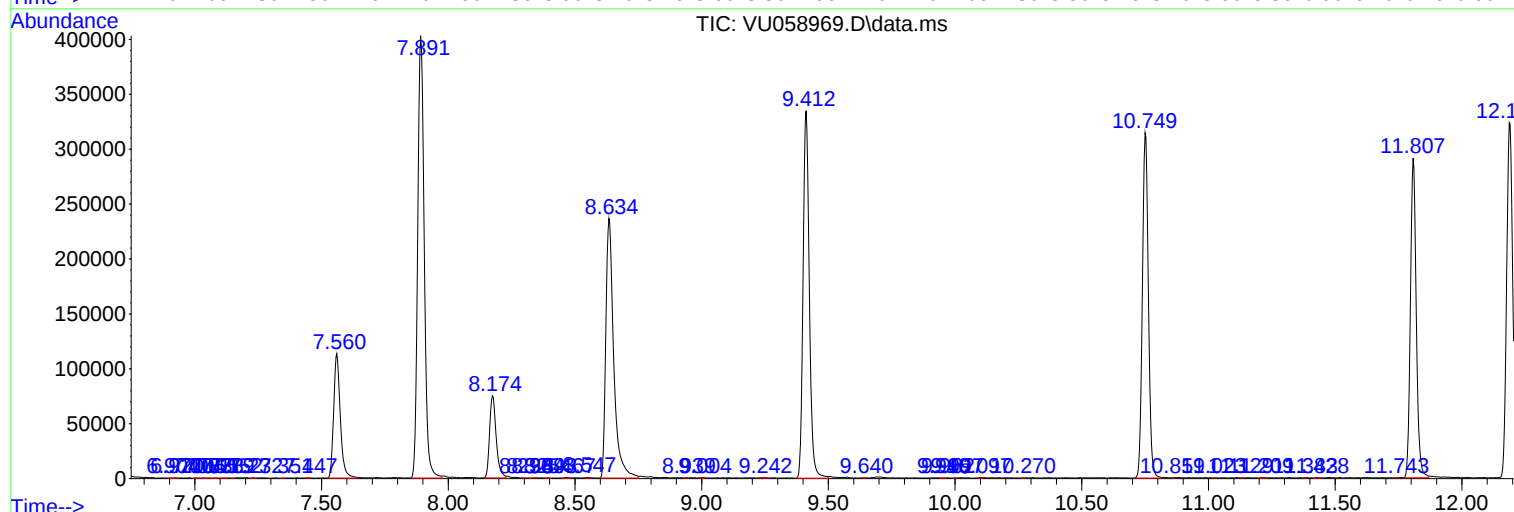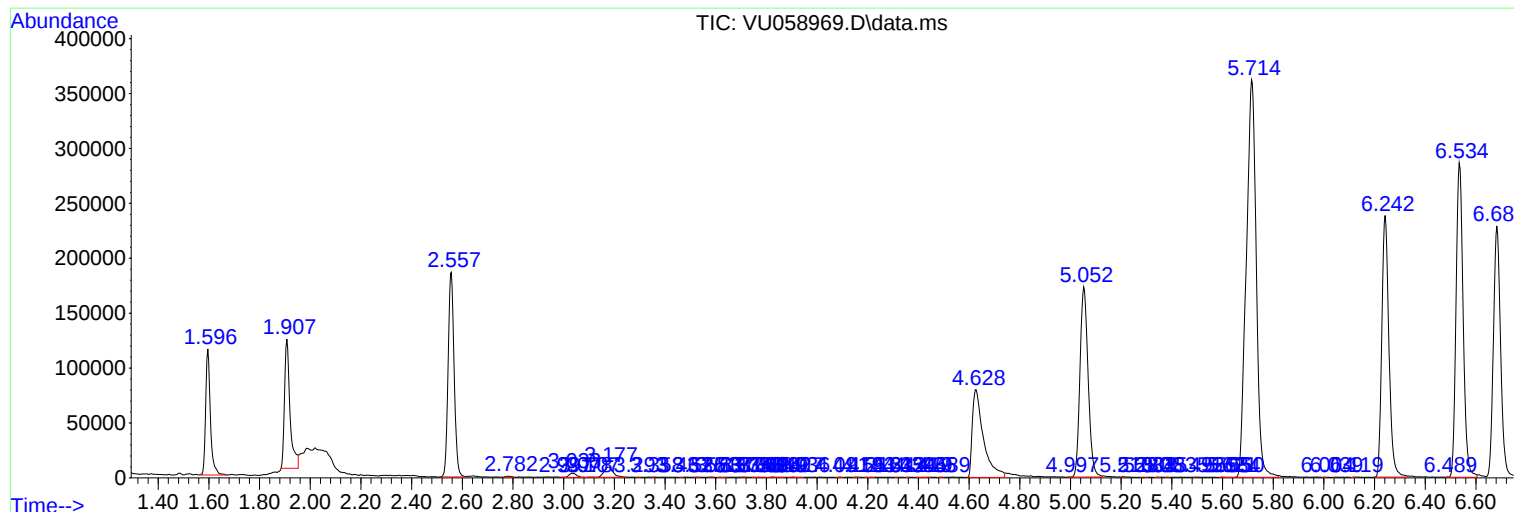

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058969.D
Acq On : 24 May 2024 14:30
Operator : MD/SY
Sample : P2566-03DL 4000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058969.D
Acq On : 24 May 2024 14:30
Operator : MD/SY
Sample : P2566-03DL 4000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------