

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
 Data File : VU058982.D
 Acq On : 24 May 2024 19:48
 Operator : MD/SY
 Sample : P2566-12DL 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M

Title : VOC Analysis

Signal : TIC: VU058982.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.480	54	59	66	rVB2	4099	4287	0.47%	0.063%
2	1.592	86	94	114	rBV	101044	127757	14.05%	1.888%
3	1.814	138	163	164	rBV8	52237	150356	16.54%	2.222%
4	1.872	177	181	203	rVB	148490	201783	22.20%	2.982%
5	2.547	379	391	406	rBV	170261	276407	30.40%	4.085%
6	2.625	408	415	418	rBV4	1531	1804	0.20%	0.027%
7	2.686	429	434	435	rBV	240	212	0.02%	0.003%
8	2.772	453	461	468	rBV4	1155	1988	0.22%	0.029%
9	2.801	468	470	474	rBV2	275	205	0.02%	0.003%
10	2.943	509	514	516	rBV2	315	309	0.03%	0.005%
11	3.030	533	541	554	rVB4	3907	6990	0.77%	0.103%
12	3.174	571	586	608	rBV	13603	36044	3.96%	0.533%
13	3.367	641	646	650	rVB	265	252	0.03%	0.004%
14	3.528	692	696	704	rVB2	246	297	0.03%	0.004%
15	3.605	717	720	724	rBV2	215	204	0.02%	0.003%
16	3.743	759	763	769	rVV2	210	229	0.03%	0.003%
17	3.805	778	782	783	rBV	323	216	0.02%	0.003%
18	3.856	795	798	801	rBV	315	217	0.02%	0.003%
19	4.062	855	862	867	rVB2	262	278	0.03%	0.004%
20	4.149	884	889	893	rBV2	234	267	0.03%	0.004%
21	4.570	1017	1020	1023	rBV2	282	216	0.02%	0.003%
22	4.612	1023	1033	1076	rVV	92424	257939	28.37%	3.812%
23	5.049	1154	1169	1196	rBV	162828	359325	39.53%	5.311%
24	5.210	1214	1219	1225	rVB2	310	382	0.04%	0.006%
25	5.483	1299	1304	1308	rVB2	297	264	0.03%	0.004%
26	5.547	1321	1324	1330	rBV	256	203	0.02%	0.003%
27	5.714	1354	1376	1401	rBV2	333509	909086	100.00%	13.436%
28	5.975	1450	1457	1460	rBV4	721	651	0.07%	0.010%
29	6.078	1484	1489	1492	rBV2	287	266	0.03%	0.004%
30	6.239	1527	1539	1571	rBV	221295	428613	47.15%	6.335%
31	6.531	1617	1630	1642	rBV5	8029	15651	1.72%	0.231%
32	6.592	1642	1649	1650	rBV2	849	834	0.09%	0.012%
33	6.682	1664	1677	1705	rBV	211661	416558	45.82%	6.156%
34	6.795	1709	1712	1717	rVV4	590	422	0.05%	0.006%
35	6.930	1749	1754	1759	rBV2	214	288	0.03%	0.004%
36	6.965	1762	1765	1769	rVB2	278	224	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
 Data File : VU058982.D
 Acq On : 24 May 2024 19:48
 Operator : MD/SY
 Sample : P2566-12DL 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

37	7.129	1812	1816	1821	rBV2	184	238	0.03%	0.004%
38	7.190	1830	1835	1838	rBV2	584	633	0.07%	0.009%
39	7.210	1838	1841	1844	rVV2	606	578	0.06%	0.009%
40	7.226	1844	1846	1850	rVB3	418	250	0.03%	0.004%
41	7.377	1891	1893	1901	rVB2	330	328	0.04%	0.005%
42	7.560	1932	1950	1968	rBV	103997	184054	20.25%	2.720%
43	7.702	1992	1994	1996	rBV2	552	273	0.03%	0.004%
44	7.714	1996	1998	2002	rVB	605	397	0.04%	0.006%
45	7.782	2016	2019	2021	rBV	514	259	0.03%	0.004%
46	7.891	2041	2053	2074	rBV	373532	647430	71.22%	9.569%
47	8.100	2116	2118	2121	rVB2	467	233	0.03%	0.003%
48	8.174	2131	2141	2160	rVV	71903	123824	13.62%	1.830%
49	8.296	2177	2179	2183	rVV2	279	217	0.02%	0.003%
50	8.351	2191	2196	2199	rVB2	388	352	0.04%	0.005%
51	8.428	2215	2220	2225	rBV2	271	339	0.04%	0.005%
52	8.460	2227	2230	2235	rBV3	493	485	0.05%	0.007%
53	8.631	2272	2283	2321	rBV	276628	537633	59.14%	7.946%
54	8.859	2349	2354	2358	rBV4	433	456	0.05%	0.007%
55	9.062	2411	2417	2423	rVB2	349	490	0.05%	0.007%
56	9.097	2423	2428	2429	rBV	333	230	0.03%	0.003%
57	9.126	2434	2437	2441	rVV2	301	248	0.03%	0.004%
58	9.242	2470	2473	2479	rBV	278	289	0.03%	0.004%
59	9.412	2514	2526	2552	rBV	312086	525113	57.76%	7.761%
60	9.528	2560	2562	2565	rVB2	389	230	0.03%	0.003%
61	9.698	2607	2615	2625	rBV5	1265	2327	0.26%	0.034%
62	9.743	2625	2629	2632	rVB2	318	205	0.02%	0.003%
63	9.798	2639	2646	2651	rBV2	279	389	0.04%	0.006%
64	10.097	2736	2739	2740	rBV	380	242	0.03%	0.004%
65	10.274	2789	2794	2796	rBV	259	237	0.03%	0.004%
66	10.309	2801	2805	2809	rBV	303	214	0.02%	0.003%
67	10.422	2838	2840	2848	rVB2	413	396	0.04%	0.006%
68	10.666	2912	2916	2921	rVB	391	324	0.04%	0.005%
69	10.750	2929	2942	2963	rBV	317762	522029	57.42%	7.715%
70	10.885	2980	2984	2991	rVB3	619	751	0.08%	0.011%
71	10.975	3007	3012	3014	rBV	273	287	0.03%	0.004%
72	10.988	3014	3016	3020	rVB2	396	218	0.02%	0.003%
73	11.026	3025	3028	3032	rBV	276	243	0.03%	0.004%
74	11.325	3116	3121	3124	rBV	332	274	0.03%	0.004%
75	11.386	3137	3140	3147	rVV2	210	249	0.03%	0.004%
76	11.740	3244	3250	3254	rBV2	266	327	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
 Data File : VU058982.D
 Acq On : 24 May 2024 19:48
 Operator : MD/SY
 Sample : P2566-12DL 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

77	11.807	3259	3271	3298	rVV	280201	454291	49.97%	6.714%
78	11.920	3302	3306	3309	rBV2	454	385	0.04%	0.006%
79	11.981	3319	3325	3330	rBV4	631	745	0.08%	0.011%
80	12.190	3377	3390	3417	rBV	329309	549670	60.46%	8.124%
81	12.650	3528	3533	3536	rVB	383	339	0.04%	0.005%
82	12.840	3589	3592	3597	rVB2	363	286	0.03%	0.004%
83	12.923	3615	3618	3620	rBV	306	241	0.03%	0.004%
84	13.039	3652	3654	3657	rBV	320	218	0.02%	0.003%
85	13.377	3755	3759	3765	rBV2	254	352	0.04%	0.005%
86	13.447	3778	3781	3783	rBV	410	230	0.03%	0.003%
87	13.563	3814	3817	3821	rVB	402	286	0.03%	0.004%
88	13.708	3858	3862	3864	rBV2	328	262	0.03%	0.004%
89	13.756	3875	3877	3884	rVB2	347	303	0.03%	0.004%
90	13.859	3906	3909	3913	rBV	350	295	0.03%	0.004%
91	13.968	3939	3943	3945	rBV2	425	309	0.03%	0.005%
92	14.106	3983	3986	3990	rBV	540	420	0.05%	0.006%
93	14.193	4010	4013	4015	rBV	460	351	0.04%	0.005%
94	14.296	4042	4045	4046	rBV	360	220	0.02%	0.003%
95	14.348	4059	4061	4065	rBV2	317	224	0.02%	0.003%
96	14.373	4065	4069	4072	rBV3	442	348	0.04%	0.005%
97	14.737	4175	4182	4188	rBV2	756	1198	0.13%	0.018%
98	15.129	4301	4304	4308	rBV3	404	402	0.04%	0.006%
99	15.981	4567	4569	4572	rBV	538	303	0.03%	0.004%
100	16.341	4679	4681	4683	rVB3	733	248	0.03%	0.004%




Sum of corrected areas: 6766241

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058982.D
Acq On : 24 May 2024 19:48
Operator : MD/SY
Sample : P2566-12DL 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

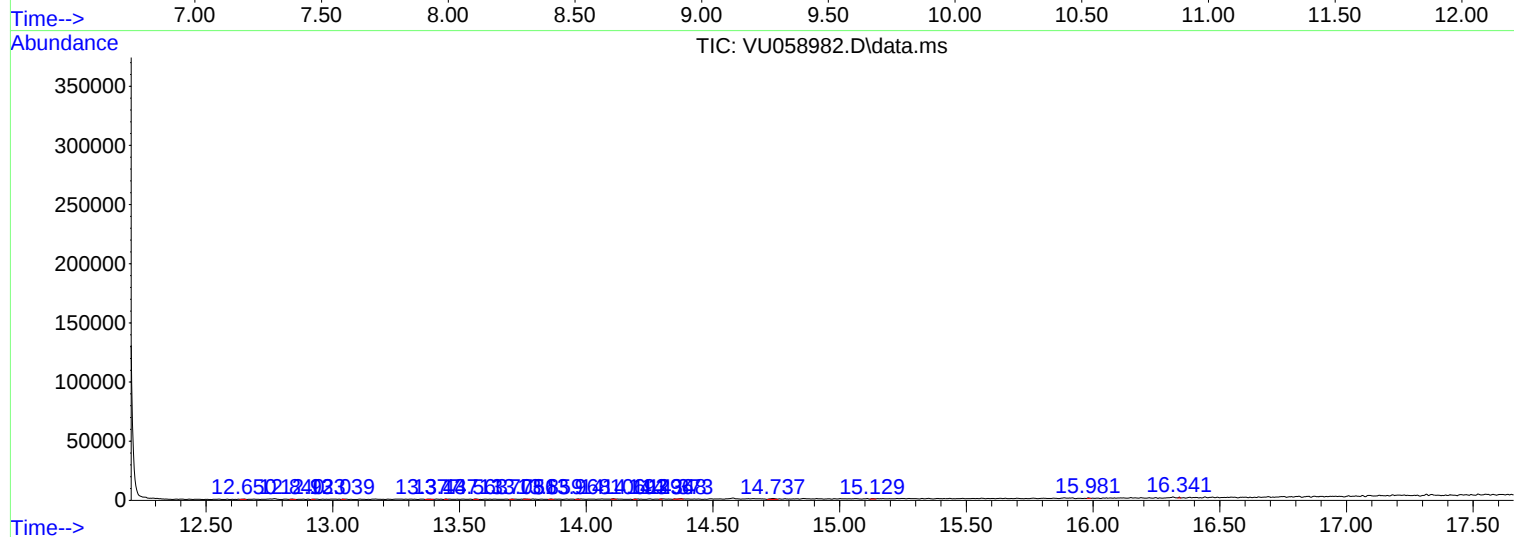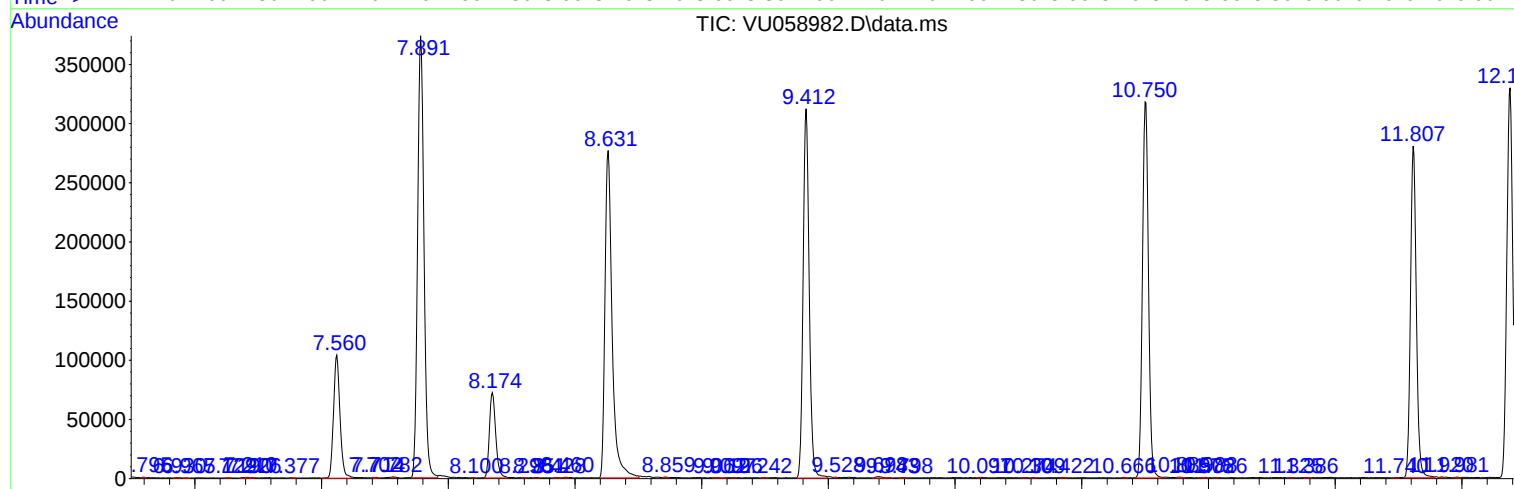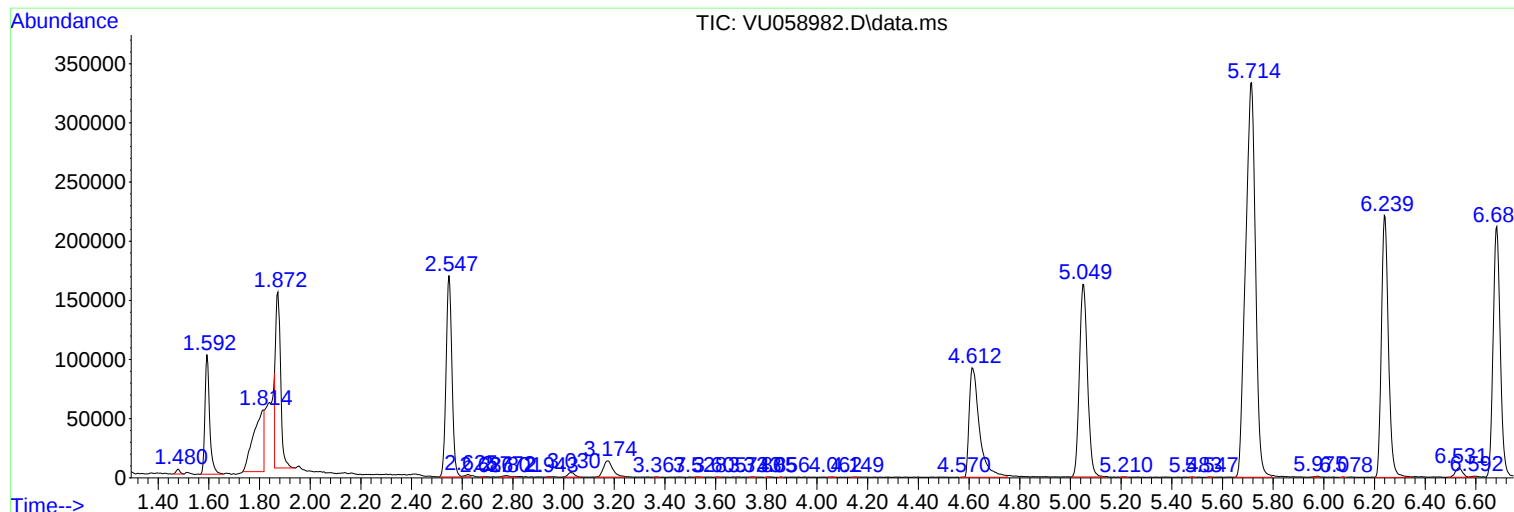

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058982.D
Acq On : 24 May 2024 19:48
Operator : MD/SY
Sample : P2566-12DL 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058982.D
Acq On : 24 May 2024 19:48
Operator : MD/SY
Sample : P2566-12DL 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------