

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
 Data File : VU058984.D
 Acq On : 24 May 2024 20:38
 Operator : MD/SY
 Sample : P2566-14 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

Signal : TIC: VU058984.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	87	94	114	rVB	100862	122573	14.48%	2.036%
2	1.885	178	185	200	rVB	81927	114369	13.51%	1.900%
3	2.554	381	393	407	rBV	149919	245188	28.96%	4.073%
4	2.750	448	454	455	rBV2	713	660	0.08%	0.011%
5	3.026	533	540	542	rBV4	4044	4543	0.54%	0.075%
6	3.084	557	558	559	rBV	133	33	0.00%	0.001%
7	3.120	566	569	571	rBV	204	122	0.01%	0.002%
8	3.174	571	586	604	rVB	17069	38935	4.60%	0.647%
9	3.396	651	655	659	rBV	431	353	0.04%	0.006%
10	3.560	703	706	712	rVB	328	312	0.04%	0.005%
11	3.592	712	716	718	rBV	140	100	0.01%	0.002%
12	3.653	732	735	737	rBV	122	75	0.01%	0.001%
13	3.685	742	745	750	rVB2	146	115	0.01%	0.002%
14	3.714	750	754	756	rBV2	247	195	0.02%	0.003%
15	3.772	768	772	774	rBV2	152	134	0.02%	0.002%
16	4.046	855	857	860	rBV	95	57	0.01%	0.001%
17	4.103	872	875	877	rBV2	134	91	0.01%	0.002%
18	4.120	878	880	882	rVV2	169	84	0.01%	0.001%
19	4.245	912	919	924	rBV2	288	425	0.05%	0.007%
20	4.306	936	938	940	rBV2	123	70	0.01%	0.001%
21	4.493	993	996	998	rBV	160	93	0.01%	0.002%
22	4.518	1001	1004	1007	rBV2	174	135	0.02%	0.002%
23	4.608	1022	1032	1065	rBV	99537	252085	29.77%	4.188%
24	4.972	1142	1145	1148	rBV2	346	292	0.03%	0.005%
25	5.052	1154	1170	1196	rBV	154134	338015	39.92%	5.615%
26	5.181	1207	1210	1216	rBV2	325	285	0.03%	0.005%
27	5.300	1244	1247	1249	rBV	218	158	0.02%	0.003%
28	5.396	1274	1277	1283	rBV2	227	265	0.03%	0.004%
29	5.454	1292	1295	1298	rBV	157	116	0.01%	0.002%
30	5.486	1303	1305	1309	rBV	189	124	0.01%	0.002%
31	5.544	1320	1323	1328	rBV2	282	295	0.03%	0.005%
32	5.621	1342	1347	1354	rVB2	386	362	0.04%	0.006%
33	5.714	1355	1376	1404	rBV2	306292	846754	100.00%	14.067%
34	5.949	1445	1449	1451	rBV	243	179	0.02%	0.003%
35	6.013	1467	1469	1470	rBV	252	77	0.01%	0.001%
36	6.074	1485	1488	1489	rBV2	107	54	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
 Data File : VU058984.D
 Acq On : 24 May 2024 20:38
 Operator : MD/SY
 Sample : P2566-14 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

37	6.242	1527	1540	1563	rBV	208919	404374	47.76%	6.718%
38	6.454	1603	1606	1608	rBV2	309	226	0.03%	0.004%
39	6.534	1617	1631	1644	rVB2	5770	12423	1.47%	0.206%
40	6.595	1647	1650	1651	rBV2	392	185	0.02%	0.003%
41	6.682	1663	1677	1705	rBV	197448	392386	46.34%	6.519%
42	6.811	1714	1717	1719	rBV3	305	171	0.02%	0.003%
43	6.936	1752	1756	1759	rBV2	200	185	0.02%	0.003%
44	7.033	1783	1786	1788	rVB	124	63	0.01%	0.001%
45	7.100	1802	1807	1809	rBV	280	222	0.03%	0.004%
46	7.148	1820	1822	1824	rBV	128	69	0.01%	0.001%
47	7.271	1858	1860	1863	rVB	147	79	0.01%	0.001%
48	7.290	1863	1866	1867	rBV	61	33	0.00%	0.001%
49	7.303	1867	1870	1874	rBV	187	119	0.01%	0.002%
50	7.335	1877	1880	1882	rBV	191	135	0.02%	0.002%
51	7.496	1927	1930	1931	rBV	153	91	0.01%	0.002%
52	7.560	1938	1950	1970	rBV	95625	171652	20.27%	2.852%
53	7.772	2014	2016	2017	rBV	461	235	0.03%	0.004%
54	7.817	2028	2030	2034	rBV2	280	148	0.02%	0.002%
55	7.891	2040	2053	2081	rBV	335149	586436	69.26%	9.742%
56	8.090	2112	2115	2120	rVB2	415	367	0.04%	0.006%
57	8.174	2129	2141	2166	rBV	67882	116358	13.74%	1.933%
58	8.261	2166	2168	2171	rVB2	326	217	0.03%	0.004%
59	8.280	2171	2174	2178	rBV3	178	174	0.02%	0.003%
60	8.303	2179	2181	2185	rVB	307	174	0.02%	0.003%
61	8.393	2208	2209	2210	rBV	166	56	0.01%	0.001%
62	8.434	2218	2222	2226	rBV	256	245	0.03%	0.004%
63	8.550	2256	2258	2260	rBV2	108	61	0.01%	0.001%
64	8.627	2271	2282	2317	rBV	264332	502493	59.34%	8.348%
65	8.914	2369	2371	2374	rBV	416	270	0.03%	0.004%
66	9.042	2408	2411	2413	rBV	224	127	0.01%	0.002%
67	9.174	2446	2452	2457	rBV	364	521	0.06%	0.009%
68	9.412	2514	2526	2557	rBV	294587	495561	58.52%	8.233%
69	9.772	2635	2638	2643	rBV2	223	164	0.02%	0.003%
70	10.373	2823	2825	2828	rBV	207	149	0.02%	0.002%
71	10.750	2930	2942	2962	rBV	287224	464069	54.81%	7.710%
72	10.875	2976	2981	2983	rBV3	379	367	0.04%	0.006%
73	11.264	3099	3102	3106	rBV2	271	257	0.03%	0.004%
74	11.807	3259	3271	3291	rBV	254228	415434	49.06%	6.902%
75	12.187	3377	3389	3413	rBV	288260	485395	57.32%	8.064%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058984.D
Acq On : 24 May 2024 20:38
Operator : MD/SY
Sample : P2566-14 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Title : VOC Analysis




Sum of corrected areas: 6019414

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058984.D
Acq On : 24 May 2024 20:38
Operator : MD/SY
Sample : P2566-14 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

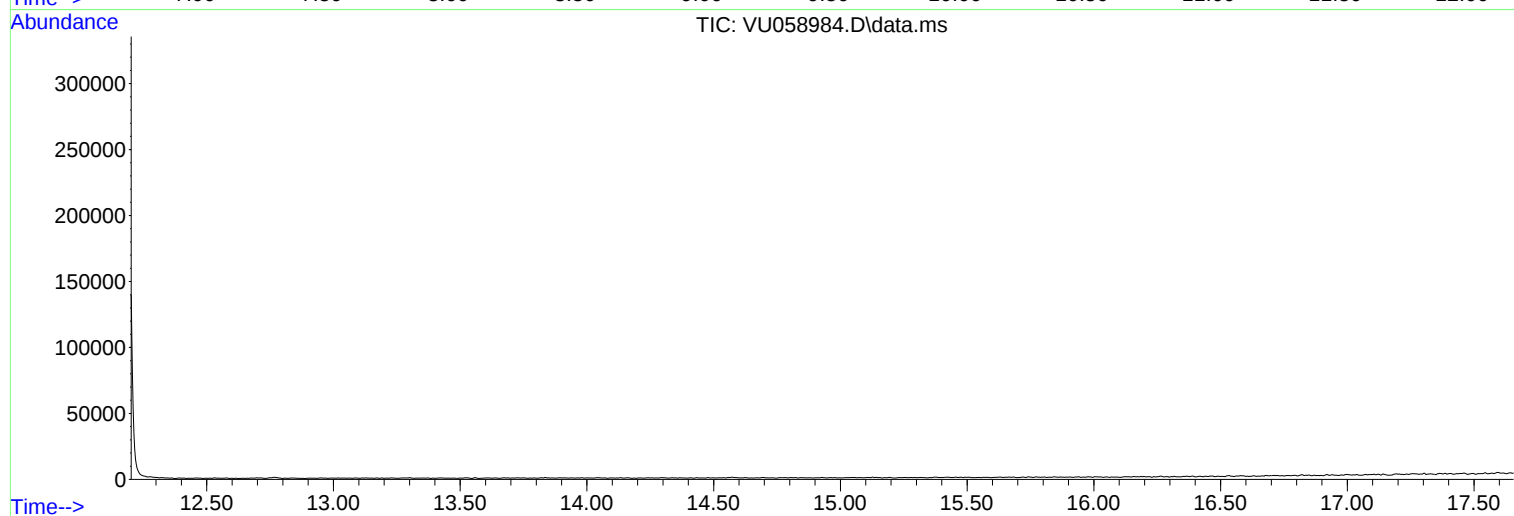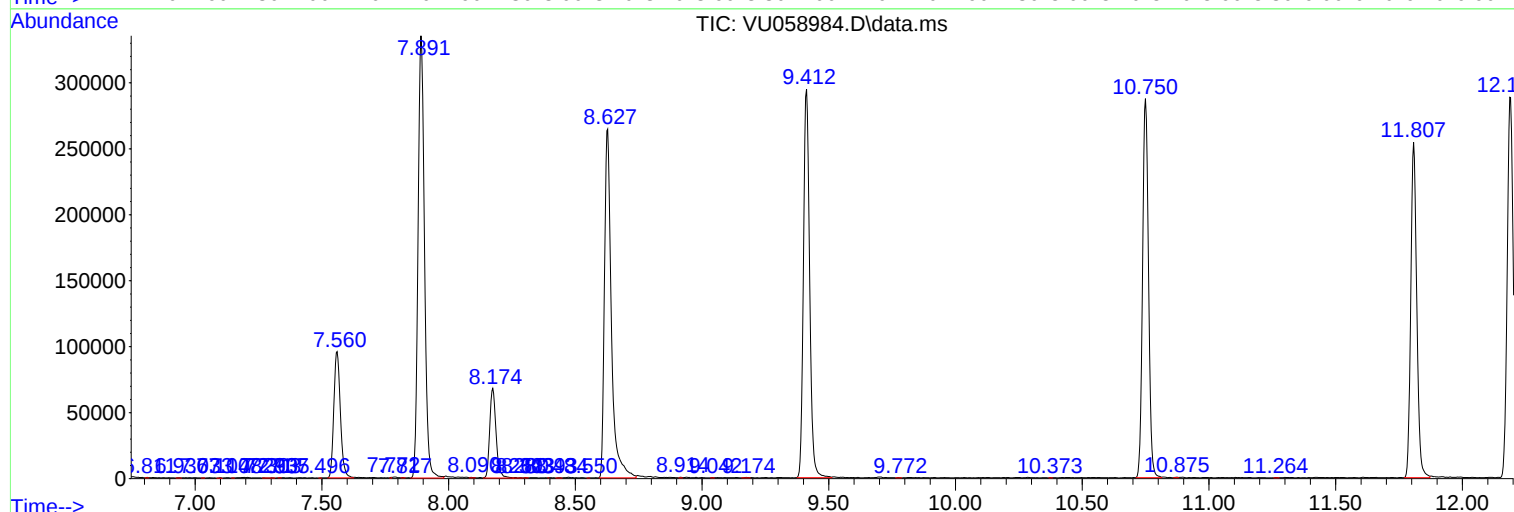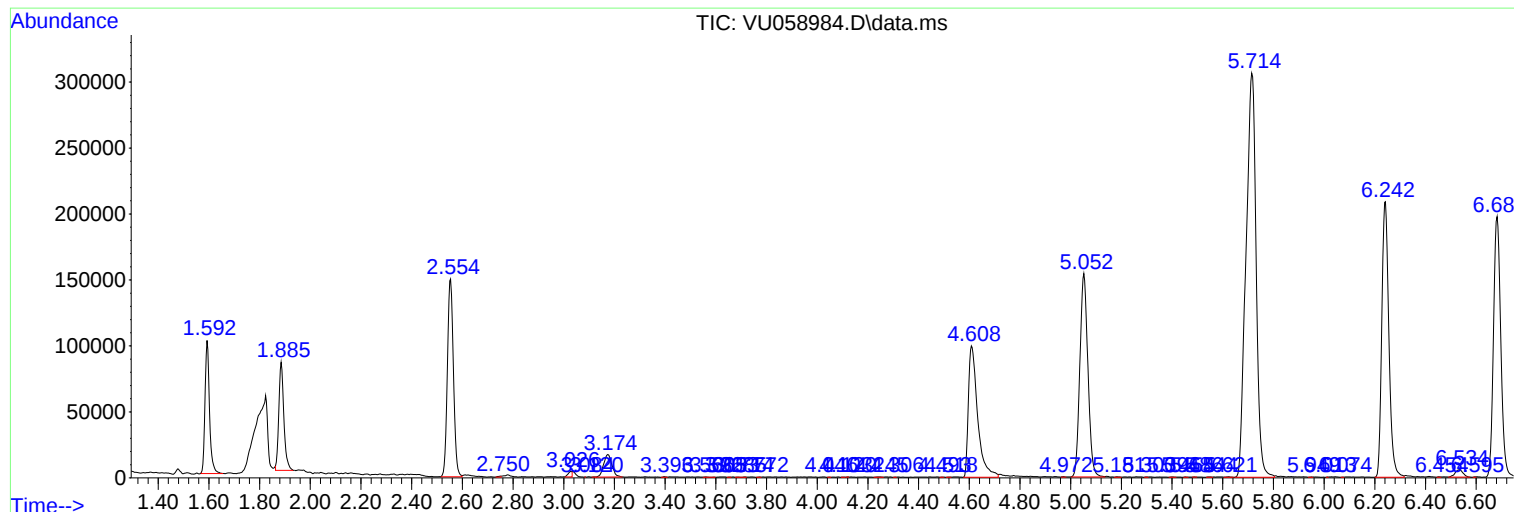

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058984.D
Acq On : 24 May 2024 20:38
Operator : MD/SY
Sample : P2566-14 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058984.D
Acq On : 24 May 2024 20:38
Operator : MD/SY
Sample : P2566-14 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------